

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039376.D
 Acq On : 19 Dec 2023 22:46
 Operator : JC/MD
 Sample : 05835-13DL 5X
 Misc : 2.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039376.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	23	25	28	rBV2	1782	2354	0.30%	0.037%
2	1.368	43	46	56	rBV	90143	102769	13.13%	1.615%
3	1.654	90	93	103	rVB	57601	82749	10.57%	1.301%
4	2.300	193	199	210	rBV	163269	263229	33.62%	4.138%
5	2.374	210	211	216	rVB4	2016	2544	0.32%	0.040%
6	2.703	260	265	271	rVV	2833	5897	0.75%	0.093%
7	2.788	274	279	289	rVB5	1679	3743	0.48%	0.059%
8	2.855	289	290	295	rBV3	203	248	0.03%	0.004%
9	2.947	295	305	314	rBV2	7759	18778	2.40%	0.295%
10	3.117	330	333	335	rBV	276	276	0.04%	0.004%
11	3.325	364	367	368	rBV2	208	238	0.03%	0.004%
12	3.550	402	404	410	rBV2	189	380	0.05%	0.006%
13	3.697	425	428	431	rBV2	282	390	0.05%	0.006%
14	3.800	442	445	446	rVB2	188	187	0.02%	0.003%
15	3.861	453	455	458	rBV2	214	281	0.04%	0.004%
16	3.965	470	472	474	rBV	180	198	0.03%	0.003%
17	4.050	482	486	487	rBV2	182	251	0.03%	0.004%
18	4.385	539	541	543	rVB	235	183	0.02%	0.003%
19	4.452	543	552	570	rBV	68989	204008	26.06%	3.207%
20	5.056	639	651	670	rBV2	96021	307379	39.26%	4.832%
21	5.245	681	682	686	rVB2	204	177	0.02%	0.003%
22	5.397	704	707	710	rVB2	273	353	0.05%	0.006%
23	5.501	719	724	726	rBV	237	420	0.05%	0.007%
24	5.544	730	731	732	rBV	295	171	0.02%	0.003%
25	5.617	741	743	746	rBV2	179	181	0.02%	0.003%
26	5.727	759	761	764	rBV2	210	234	0.03%	0.004%
27	5.775	767	769	771	rBV2	232	252	0.03%	0.004%
28	5.964	789	800	815	rBV2	258317	782927	100.00%	12.307%
29	6.245	844	846	847	rBV	200	167	0.02%	0.003%
30	6.336	859	861	864	rBV2	145	170	0.02%	0.003%
31	6.361	864	865	867	rVV	225	181	0.02%	0.003%
32	6.397	869	871	874	rVB2	220	189	0.02%	0.003%
33	6.422	874	875	878	rBV	211	220	0.03%	0.003%
34	6.556	893	897	899	rBV2	301	331	0.04%	0.005%
35	6.757	922	930	945	rBV	200285	484410	61.87%	7.615%
36	7.062	979	980	983	rBV2	253	233	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039376.D
 Acq On : 19 Dec 2023 22:46
 Operator : JC/MD
 Sample : 05835-13DL 5X
 Misc : 2.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.117	983	989	995	rVB6	1183	2776	0.35%	0.044%
38	7.306	1010	1020	1039	rBV	161053	358032	45.73%	5.628%
39	7.458	1043	1045	1046	rVV2	290	221	0.03%	0.003%
40	7.489	1048	1050	1052	rVV3	469	415	0.05%	0.007%
41	7.513	1052	1054	1057	rVV3	411	431	0.06%	0.007%
42	7.568	1061	1063	1066	rVB	230	239	0.03%	0.004%
43	7.970	1123	1129	1134	rVV5	1073	2206	0.28%	0.035%
44	8.141	1153	1157	1159	rVB2	178	200	0.03%	0.003%
45	8.190	1163	1165	1168	rVB2	296	274	0.03%	0.004%
46	8.324	1181	1187	1198	rBV	105339	174389	22.27%	2.741%
47	8.513	1214	1218	1219	rVB3	316	304	0.04%	0.005%
48	8.555	1223	1225	1227	rBV2	193	199	0.03%	0.003%
49	8.647	1234	1240	1261	rBV	385173	615954	78.67%	9.682%
50	8.952	1284	1290	1300	rBV	74366	116126	14.83%	1.825%
51	9.128	1318	1319	1323	rVV2	196	198	0.03%	0.003%
52	9.269	1341	1342	1345	rBV2	234	200	0.03%	0.003%
53	9.385	1356	1361	1373	rBV	341191	489764	62.56%	7.699%
54	9.708	1411	1414	1419	rVB3	771	946	0.12%	0.015%
55	9.860	1437	1439	1441	rBV	236	172	0.02%	0.003%
56	10.055	1465	1471	1473	rBV	449345	707893	90.42%	11.128%
57	10.293	1509	1510	1511	rBV	310	203	0.03%	0.003%
58	10.317	1512	1514	1516	rVV2	593	456	0.06%	0.007%
59	10.366	1519	1522	1525	rVB2	185	171	0.02%	0.003%
60	10.537	1548	1550	1554	rBV	206	198	0.03%	0.003%
61	10.598	1559	1560	1563	rBV2	203	189	0.02%	0.003%
62	10.653	1565	1569	1570	rBV2	410	427	0.05%	0.007%
63	10.890	1606	1608	1612	rVB2	193	281	0.04%	0.004%
64	10.964	1616	1620	1625	rBV4	2777	3915	0.50%	0.062%
65	11.092	1638	1641	1646	rBV2	357	483	0.06%	0.008%
66	11.189	1651	1657	1668	rBV	313064	392731	50.16%	6.173%
67	11.311	1675	1677	1680	rVB2	736	544	0.07%	0.009%
68	11.457	1698	1701	1704	rBV2	421	554	0.07%	0.009%
69	11.756	1748	1750	1753	rVV2	395	419	0.05%	0.007%
70	11.787	1753	1755	1758	rVB2	139	165	0.02%	0.003%
71	11.823	1758	1761	1762	rBV2	210	176	0.02%	0.003%
72	11.976	1782	1786	1788	rBV4	1630	2109	0.27%	0.033%
73	12.018	1788	1793	1811	rVB	499539	646745	82.61%	10.166%
74	12.317	1837	1842	1852	rBV	445259	558885	71.38%	8.785%
75	12.457	1864	1865	1869	rBV3	373	325	0.04%	0.005%
76	12.646	1893	1896	1898	rBV2	196	258	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039376.D
 Acq On : 19 Dec 2023 22:46
 Operator : JC/MD
 Sample : 05835-13DL 5X
 Misc : 2.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.762	1911	1915	1920	rVB3	2171	3074	0.39%	0.048%
78	12.853	1926	1930	1931	rBV2	179	222	0.03%	0.003%
79	13.049	1960	1962	1966	rBV2	220	226	0.03%	0.004%
80	13.091	1966	1969	1972	rVV2	162	206	0.03%	0.003%
81	13.122	1972	1974	1977	rVB3	138	173	0.02%	0.003%
82	13.256	1994	1996	1999	rVB2	246	213	0.03%	0.003%
83	13.548	2042	2044	2046	rVV	187	166	0.02%	0.003%
84	13.591	2047	2051	2058	rVB3	1391	1638	0.21%	0.026%
85	13.780	2079	2082	2083	rBV2	316	271	0.03%	0.004%
86	13.933	2105	2107	2110	rBV2	175	225	0.03%	0.004%
87	14.073	2126	2130	2133	rVB2	174	236	0.03%	0.004%
88	14.128	2133	2139	2144	rBV2	3922	5164	0.66%	0.081%
89	14.243	2155	2158	2159	rBV2	295	314	0.04%	0.005%
90	14.414	2182	2186	2187	rBV2	176	173	0.02%	0.003%
91	14.499	2198	2200	2201	rBV2	265	236	0.03%	0.004%
92	14.567	2208	2211	2212	rBV2	305	276	0.04%	0.004%
93	14.695	2229	2232	2233	rBV2	145	164	0.02%	0.003%
94	14.914	2265	2268	2270	rBV2	273	326	0.04%	0.005%
95	14.981	2277	2279	2282	rBV2	247	187	0.02%	0.003%
96	15.048	2288	2290	2292	rVB3	263	183	0.02%	0.003%
97	15.377	2342	2344	2345	rBV2	379	305	0.04%	0.005%
98	15.463	2356	2358	2359	rVB2	307	202	0.03%	0.003%
99	15.633	2384	2386	2388	rBV	273	217	0.03%	0.003%
100	16.700	2558	2561	2562	rBV2	381	319	0.04%	0.005%

Sum of corrected areas: 6361587




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039376.D
Acq On : 19 Dec 2023 22:46
Operator : JC/MD
Sample : 05835-13DL 5X
Misc : 2.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

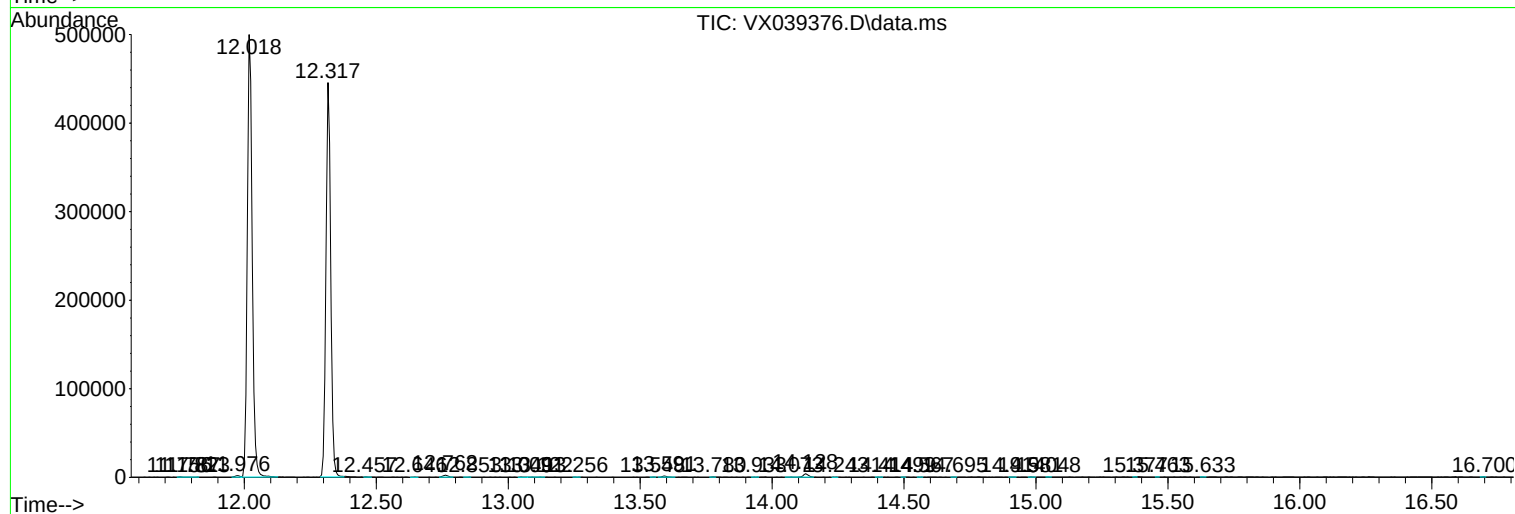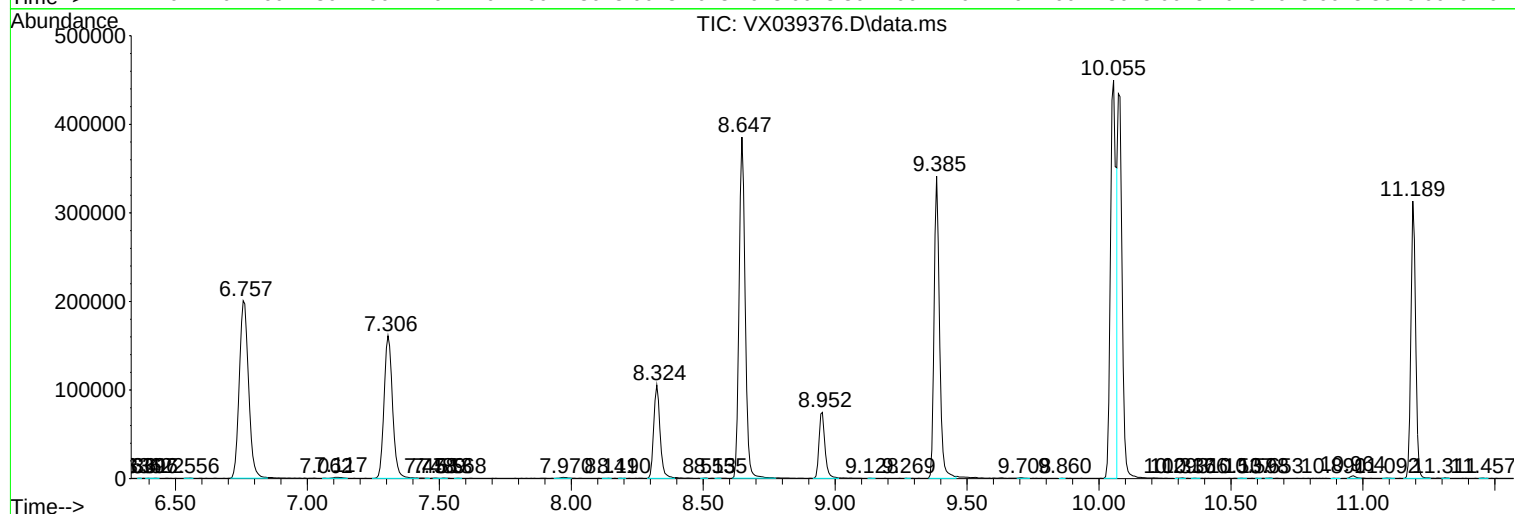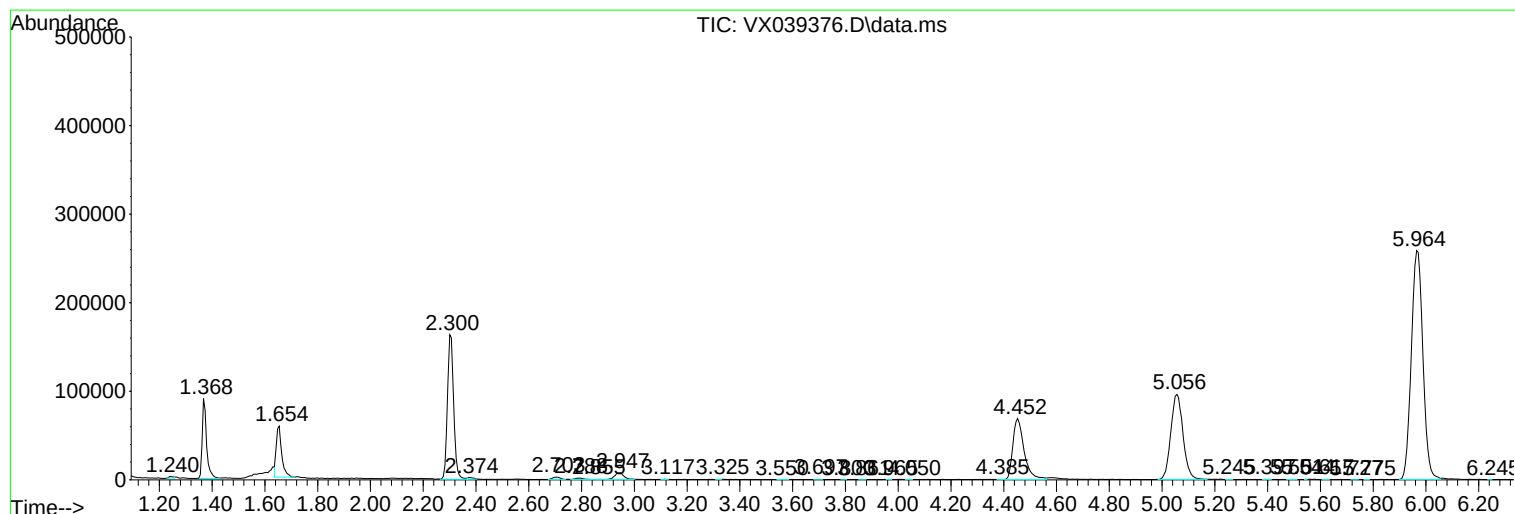

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039376.D
Acq On : 19 Dec 2023 22:46
Operator : JC/MD
Sample : 05835-13DL 5X
Misc : 2.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039376.D
Acq On : 19 Dec 2023 22:46
Operator : JC/MD
Sample : 05835-13DL 5X
Misc : 2.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc