

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039377.D
 Acq On : 19 Dec 2023 23:09
 Operator : JC/MD
 Sample : 05835-16DL 5X
 Misc : 4.62g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039377.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	32	rBV4	1987	3801	0.50%	0.063%
2	1.368	43	46	57	rBV	85593	100959	13.22%	1.670%
3	1.648	89	92	103	rVB	61440	87070	11.40%	1.440%
4	2.300	193	199	210	rBV	160913	255404	33.45%	4.224%
5	2.483	225	229	230	rBV2	269	423	0.06%	0.007%
6	2.550	238	240	241	rBV	480	399	0.05%	0.007%
7	2.709	260	266	271	rBV3	1652	3190	0.42%	0.053%
8	2.788	274	279	285	rVV4	1563	2981	0.39%	0.049%
9	2.947	299	305	314	rVB3	2365	5736	0.75%	0.095%
10	3.014	314	316	317	rVB2	295	197	0.03%	0.003%
11	3.032	317	319	320	rBV	203	203	0.03%	0.003%
12	3.044	320	321	325	rVB2	258	223	0.03%	0.004%
13	3.282	358	360	364	rVB2	189	221	0.03%	0.004%
14	3.471	390	391	394	rBV2	235	191	0.03%	0.003%
15	3.556	401	405	407	rVB2	190	257	0.03%	0.004%
16	3.574	407	408	410	rBV2	237	192	0.03%	0.003%
17	3.831	449	450	455	rVB2	232	256	0.03%	0.004%
18	3.965	469	472	474	rBV2	245	320	0.04%	0.005%
19	4.013	477	480	482	rBV2	214	239	0.03%	0.004%
20	4.056	485	487	489	rBV2	181	208	0.03%	0.003%
21	4.129	497	499	502	rVB	237	233	0.03%	0.004%
22	4.172	502	506	508	rBV2	313	437	0.06%	0.007%
23	4.257	519	520	524	rBV	286	195	0.03%	0.003%
24	4.452	544	552	569	rBV	65018	192578	25.22%	3.185%
25	4.849	614	617	620	rBV	222	298	0.04%	0.005%
26	4.897	622	625	628	rBV2	221	280	0.04%	0.005%
27	5.056	639	651	668	rBV	92773	296709	38.86%	4.908%
28	5.275	685	687	689	rVB2	200	198	0.03%	0.003%
29	5.300	689	691	693	rBV	185	193	0.03%	0.003%
30	5.391	704	706	708	rBV	308	265	0.03%	0.004%
31	5.458	714	717	718	rBV	291	268	0.04%	0.004%
32	5.586	736	738	743	rVB2	154	250	0.03%	0.004%
33	5.635	744	746	750	rVB2	206	275	0.04%	0.005%
34	5.964	788	800	818	rBV3	254337	763599	100.00%	12.630%
35	6.220	840	842	847	rVB2	317	409	0.05%	0.007%
36	6.263	847	849	850	rBV2	250	223	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039377.D
 Acq On : 19 Dec 2023 23:09
 Operator : JC/MD
 Sample : 05835-16DL 5X
 Misc : 4.62g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	6.354	863	864	869	rBV2	146	234	0.03%	0.004%
38	6.403	869	872	873	rVV2	186	208	0.03%	0.003%
39	6.519	887	891	893	rBV	273	270	0.04%	0.004%
40	6.617	903	907	909	rBV2	271	354	0.05%	0.006%
41	6.757	921	930	946	rBV	190464	463801	60.74%	7.671%
42	6.921	955	957	959	rBV2	310	325	0.04%	0.005%
43	7.056	977	979	982	rVV2	223	272	0.04%	0.004%
44	7.117	983	989	994	rVV2	1341	2515	0.33%	0.042%
45	7.184	998	1000	1002	rVB2	295	201	0.03%	0.003%
46	7.305	1011	1020	1037	rBV	158524	349890	45.82%	5.787%
47	7.702	1081	1085	1088	rBV2	157	224	0.03%	0.004%
48	8.086	1146	1148	1151	rVV	231	223	0.03%	0.004%
49	8.324	1181	1187	1200	rBV	100974	169523	22.20%	2.804%
50	8.580	1227	1229	1233	rVB2	238	203	0.03%	0.003%
51	8.647	1234	1240	1259	rBV	375972	593679	77.75%	9.819%
52	8.952	1284	1290	1304	rBV	71191	112319	14.71%	1.858%
53	9.141	1319	1321	1324	rVB2	199	210	0.03%	0.003%
54	9.269	1338	1342	1346	rBV2	380	526	0.07%	0.009%
55	9.384	1356	1361	1381	rBV	334326	469001	61.42%	7.757%
56	9.988	1459	1460	1463	rVB	501	303	0.04%	0.005%
57	10.055	1465	1471	1472	rBV	434074	551737	72.25%	9.126%
58	10.189	1492	1493	1494	rBV	510	251	0.03%	0.004%
59	10.238	1499	1501	1504	rBV2	294	284	0.04%	0.005%
60	10.262	1504	1505	1508	rBV2	294	283	0.04%	0.005%
61	10.311	1511	1513	1517	rVB3	538	506	0.07%	0.008%
62	10.415	1527	1530	1534	rBV	239	266	0.03%	0.004%
63	10.506	1543	1545	1548	rBV2	159	214	0.03%	0.004%
64	10.646	1566	1568	1572	rVB3	319	395	0.05%	0.007%
65	10.963	1617	1620	1624	rBV2	326	360	0.05%	0.006%
66	11.189	1652	1657	1670	rBV	290261	379110	49.65%	6.270%
67	11.366	1681	1686	1691	rBV	20393	27280	3.57%	0.451%
68	11.421	1693	1695	1697	rVV	502	503	0.07%	0.008%
69	11.457	1697	1701	1706	rVV2	5249	7464	0.98%	0.123%
70	11.707	1740	1742	1745	rVB2	328	288	0.04%	0.005%
71	11.756	1747	1750	1757	rVB3	508	732	0.10%	0.012%
72	11.975	1782	1786	1788	rBV2	1225	1463	0.19%	0.024%
73	12.024	1788	1794	1804	rBV	457269	618382	80.98%	10.228%
74	12.213	1823	1825	1827	rBV	148	192	0.03%	0.003%
75	12.317	1837	1842	1856	rBV	415736	542468	71.04%	8.972%
76	12.762	1911	1915	1920	rVB2	1947	2675	0.35%	0.044%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039377.D
 Acq On : 19 Dec 2023 23:09
 Operator : JC/MD
 Sample : 05835-16DL 5X
 Misc : 4.62g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

77	13.012	1953	1956	1957	rVB2	302	238	0.03%	0.004%
78	13.073	1960	1966	1971	rVV2	9846	15718	2.06%	0.260%
79	13.268	1996	1998	2000	rBV2	287	195	0.03%	0.003%
80	13.432	2023	2025	2028	rVB2	272	313	0.04%	0.005%
81	13.463	2028	2030	2032	rBV	251	207	0.03%	0.003%
82	13.591	2046	2051	2055	rBV2	834	1119	0.15%	0.019%
83	13.719	2070	2072	2076	rBV2	140	235	0.03%	0.004%
84	13.786	2079	2083	2090	rBV2	516	909	0.12%	0.015%
85	13.938	2104	2108	2110	rBV2	236	237	0.03%	0.004%
86	13.963	2110	2112	2115	rBV2	419	438	0.06%	0.007%
87	14.066	2125	2129	2132	rVV3	283	434	0.06%	0.007%
88	14.127	2135	2139	2145	rVB	3261	4341	0.57%	0.072%
89	14.701	2230	2233	2234	rBV2	209	198	0.03%	0.003%
90	15.085	2294	2296	2300	rBV	222	240	0.03%	0.004%
91	15.158	2305	2308	2309	rBV2	179	213	0.03%	0.004%
92	15.554	2371	2373	2374	rVB2	319	188	0.02%	0.003%
93	15.572	2374	2376	2378	rBV2	201	202	0.03%	0.003%
94	15.670	2387	2392	2394	rBV2	409	624	0.08%	0.010%
95	15.841	2418	2420	2423	rBV2	372	285	0.04%	0.005%
96	15.908	2430	2431	2433	rVB2	354	248	0.03%	0.004%
97	15.975	2440	2442	2445	rVB2	389	362	0.05%	0.006%
98	16.078	2458	2459	2464	rVB2	339	480	0.06%	0.008%
99	16.151	2470	2471	2474	rVV2	319	318	0.04%	0.005%
100	16.194	2476	2478	2481	rBV2	253	235	0.03%	0.004%




Sum of corrected areas: 6045991

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039377.D
Acq On : 19 Dec 2023 23:09
Operator : JC/MD
Sample : 05835-16DL 5X
Misc : 4.62g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

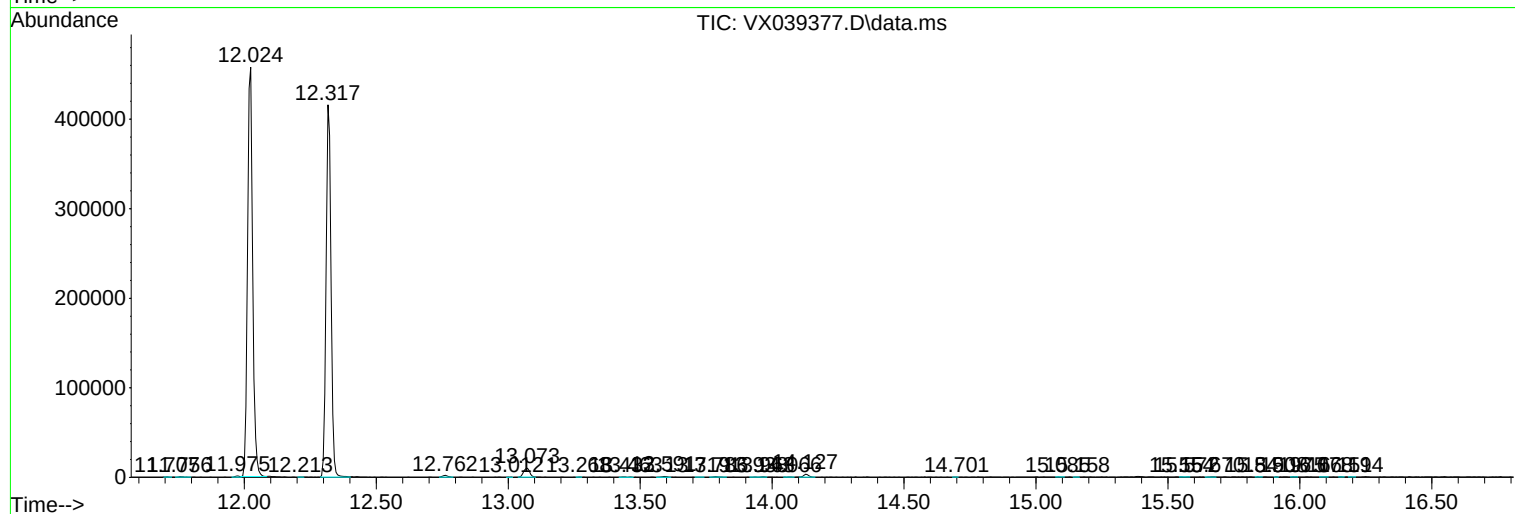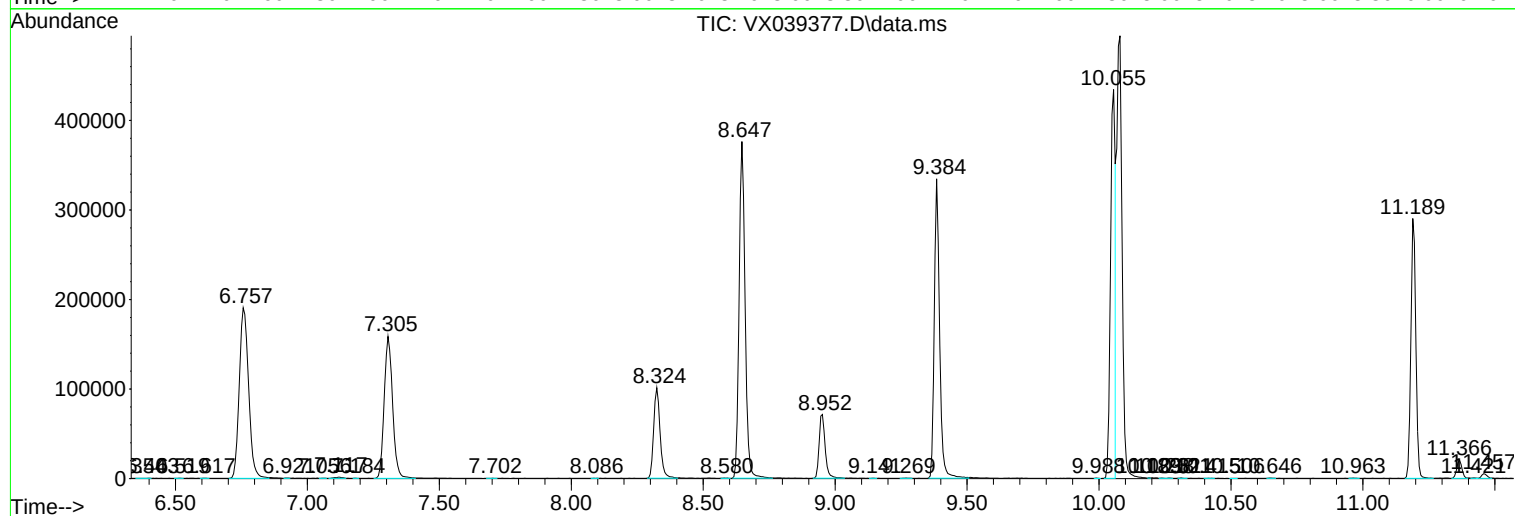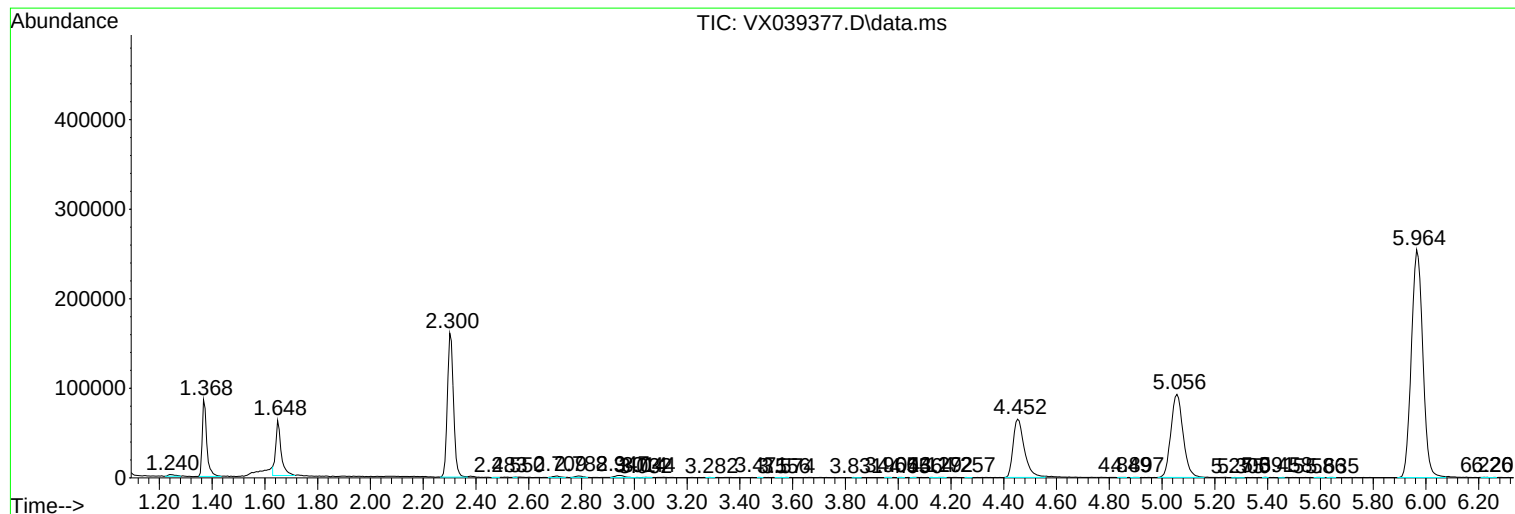

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039377.D
Acq On : 19 Dec 2023 23:09
Operator : JC/MD
Sample : 05835-16DL 5X
Misc : 4.62g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039377.D
Acq On : 19 Dec 2023 23:09
Operator : JC/MD
Sample : 05835-16DL 5X
Misc : 4.62g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc