

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039378.D
 Acq On : 19 Dec 2023 23:32
 Operator : JC/MD
 Sample : 05835-14DL 10X
 Misc : 4.07g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039378.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	57	rVB	87857	97411	12.67%	1.648%
2	1.660	90	94	110	rVB	60467	92352	12.02%	1.562%
3	2.307	193	200	211	rBV	155638	243379	31.67%	4.117%
4	2.422	217	219	222	rBV	296	217	0.03%	0.004%
5	2.691	261	263	264	rBV	443	299	0.04%	0.005%
6	2.788	275	279	286	rVB2	2362	4244	0.55%	0.072%
7	2.941	298	304	313	rBV	6143	13682	1.78%	0.231%
8	3.044	319	321	322	rVB	296	169	0.02%	0.003%
9	3.063	322	324	325	rBV2	219	185	0.02%	0.003%
10	3.288	358	361	363	rBV2	158	177	0.02%	0.003%
11	3.325	365	367	370	rBV2	278	380	0.05%	0.006%
12	3.398	377	379	383	rVB2	239	245	0.03%	0.004%
13	3.440	383	386	387	rBV2	212	206	0.03%	0.003%
14	3.751	433	437	438	rBV	174	247	0.03%	0.004%
15	4.123	495	498	499	rBV2	160	198	0.03%	0.003%
16	4.385	538	541	543	rBV2	205	232	0.03%	0.004%
17	4.446	543	551	566	rBV	69301	199858	26.00%	3.381%
18	5.062	639	652	669	rBV	96066	304887	39.67%	5.157%
19	5.269	684	686	689	rVB2	210	206	0.03%	0.003%
20	5.422	707	711	712	rBV2	256	215	0.03%	0.004%
21	5.629	743	745	747	rBV2	271	232	0.03%	0.004%
22	5.702	756	757	762	rVB	189	195	0.03%	0.003%
23	5.782	767	770	774	rVB2	202	284	0.04%	0.005%
24	5.812	774	775	778	rBV	258	286	0.04%	0.005%
25	5.964	788	800	817	rBV2	258465	768592	100.00%	13.001%
26	6.239	843	845	847	rVB	410	321	0.04%	0.005%
27	6.263	847	849	851	rBV2	322	323	0.04%	0.005%
28	6.562	894	898	900	rBV2	230	342	0.04%	0.006%
29	6.641	909	911	913	rVB	423	315	0.04%	0.005%
30	6.672	913	916	921	rBV2	247	317	0.04%	0.005%
31	6.757	921	930	948	rBV	181480	442016	57.51%	7.477%
32	7.080	980	983	984	rBV2	285	280	0.04%	0.005%
33	7.117	984	989	994	rVB5	1364	2866	0.37%	0.048%
34	7.306	1011	1020	1039	rBV	162164	352883	45.91%	5.969%
35	7.574	1061	1064	1066	rBV	147	169	0.02%	0.003%
36	7.726	1088	1089	1093	rBV	208	227	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039378.D
 Acq On : 19 Dec 2023 23:32
 Operator : JC/MD
 Sample : 05835-14DL 10X
 Misc : 4.07g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.909	1116	1119	1121	rBV2	203	216	0.03%	0.004%
38	7.958	1124	1127	1130	rBV2	193	310	0.04%	0.005%
39	8.208	1165	1168	1170	rVB2	238	169	0.02%	0.003%
40	8.324	1181	1187	1200	rBV	106085	173539	22.58%	2.936%
41	8.531	1219	1221	1223	rVB2	301	172	0.02%	0.003%
42	8.574	1226	1228	1231	rVB	344	416	0.05%	0.007%
43	8.647	1234	1240	1256	rBV	361219	573909	74.67%	9.708%
44	8.952	1284	1290	1300	rBV	72605	114927	14.95%	1.944%
45	9.275	1340	1343	1347	rVB2	327	398	0.05%	0.007%
46	9.311	1347	1349	1352	rVB2	172	167	0.02%	0.003%
47	9.385	1355	1361	1376	rBV	317635	470909	61.27%	7.966%
48	9.702	1409	1413	1419	rVB5	657	1166	0.15%	0.020%
49	9.952	1452	1454	1457	rBV2	185	184	0.02%	0.003%
50	9.976	1457	1458	1460	rVB2	303	208	0.03%	0.004%
51	10.055	1465	1471	1472	rBV	415506	532076	69.23%	9.000%
52	10.305	1507	1512	1514	rBV2	486	658	0.09%	0.011%
53	10.384	1522	1525	1527	rVV2	211	241	0.03%	0.004%
54	10.409	1527	1529	1532	rVB2	225	268	0.03%	0.005%
55	10.500	1541	1544	1546	rBV2	189	215	0.03%	0.004%
56	10.604	1559	1561	1563	rVV	216	191	0.02%	0.003%
57	10.653	1565	1569	1571	rVV2	522	566	0.07%	0.010%
58	10.909	1608	1611	1612	rBV	174	166	0.02%	0.003%
59	10.964	1617	1620	1624	rBV3	362	327	0.04%	0.006%
60	10.994	1624	1625	1628	rVB2	237	229	0.03%	0.004%
61	11.189	1652	1657	1670	rBV	296027	382916	49.82%	6.477%
62	11.311	1675	1677	1682	rVB3	682	720	0.09%	0.012%
63	11.366	1682	1686	1692	rBV2	2672	2956	0.38%	0.050%
64	11.457	1698	1701	1708	rVB5	888	1491	0.19%	0.025%
65	11.756	1748	1750	1753	rVB2	358	361	0.05%	0.006%
66	11.793	1753	1756	1758	rBV	228	214	0.03%	0.004%
67	11.902	1771	1774	1775	rBV2	222	168	0.02%	0.003%
68	11.969	1781	1785	1788	rBV2	3801	4706	0.61%	0.080%
69	12.018	1788	1793	1804	rVB	423935	587478	76.44%	9.937%
70	12.317	1837	1842	1856	rVB	390746	514197	66.90%	8.698%
71	12.506	1869	1873	1875	rVB2	282	293	0.04%	0.005%
72	12.658	1897	1898	1900	rBV	251	207	0.03%	0.004%
73	12.762	1910	1915	1920	rVB	2646	3467	0.45%	0.059%
74	12.817	1920	1924	1925	rBV2	140	181	0.02%	0.003%
75	12.927	1941	1942	1945	rBV2	162	182	0.02%	0.003%
76	13.055	1961	1963	1964	rBV2	242	201	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039378.D
 Acq On : 19 Dec 2023 23:32
 Operator : JC/MD
 Sample : 05835-14DL 10X
 Misc : 4.07g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.384	2015	2017	2021	rVB	221	211	0.03%	0.004%
78	13.591	2049	2051	2054	rVB3	421	530	0.07%	0.009%
79	13.737	2073	2075	2079	rBV2	153	191	0.02%	0.003%
80	13.786	2079	2083	2084	rBV3	404	569	0.07%	0.010%
81	13.865	2094	2096	2099	rBV2	153	187	0.02%	0.003%
82	13.926	2105	2106	2110	rVB	228	213	0.03%	0.004%
83	13.963	2110	2112	2115	rBV3	280	312	0.04%	0.005%
84	14.061	2126	2128	2130	rBV2	202	173	0.02%	0.003%
85	14.128	2134	2139	2145	rVB	2961	4398	0.57%	0.074%
86	14.487	2196	2198	2201	rVB2	228	228	0.03%	0.004%
87	14.585	2212	2214	2215	rBV	278	181	0.02%	0.003%
88	14.603	2215	2217	2218	rBV2	170	165	0.02%	0.003%
89	14.731	2233	2238	2240	rBV2	406	529	0.07%	0.009%
90	14.786	2245	2247	2252	rBV3	229	447	0.06%	0.008%
91	14.920	2268	2269	2272	rVB	363	225	0.03%	0.004%
92	14.975	2276	2278	2279	rBV	223	180	0.02%	0.003%
93	15.005	2281	2283	2285	rBV2	360	342	0.04%	0.006%
94	15.134	2300	2304	2305	rBV2	312	372	0.05%	0.006%
95	15.390	2343	2346	2351	rVB4	744	1267	0.16%	0.021%
96	15.798	2411	2413	2417	rBV3	262	361	0.05%	0.006%
97	16.115	2463	2465	2467	rBV2	232	177	0.02%	0.003%
98	16.200	2477	2479	2482	rBV	337	297	0.04%	0.005%
99	16.463	2521	2522	2523	rBV	344	167	0.02%	0.003%
100	16.536	2531	2534	2535	rBV2	256	210	0.03%	0.004%

Sum of corrected areas: 5911734




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039378.D
Acq On : 19 Dec 2023 23:32
Operator : JC/MD
Sample : 05835-14DL 10X
Misc : 4.07g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

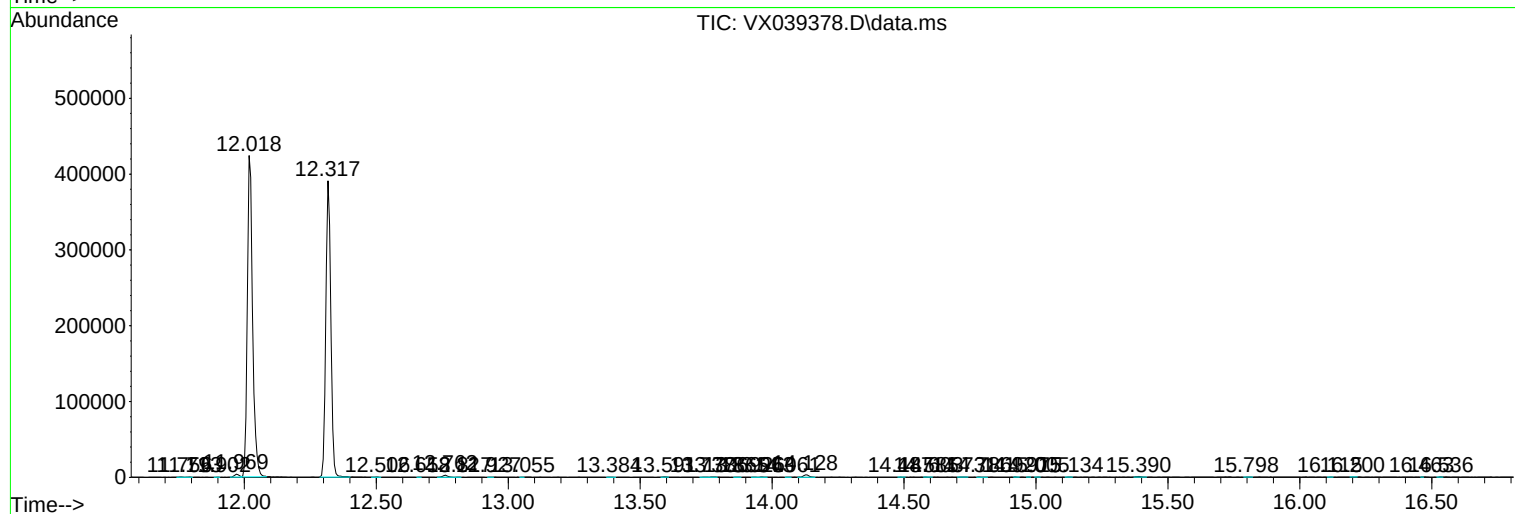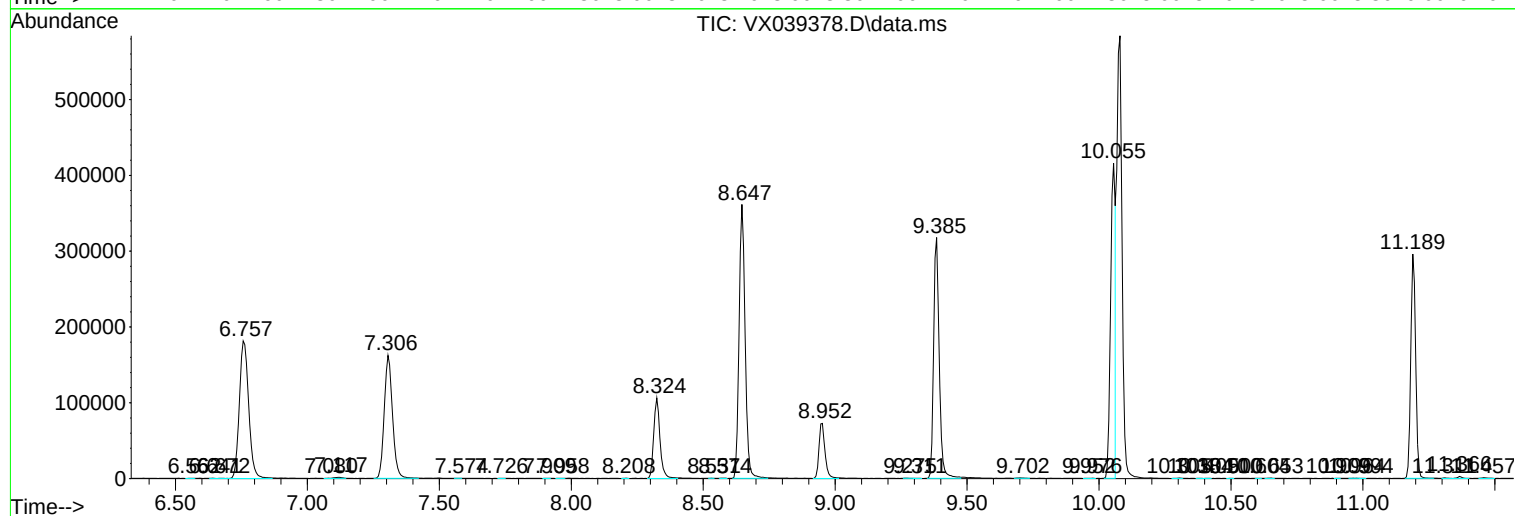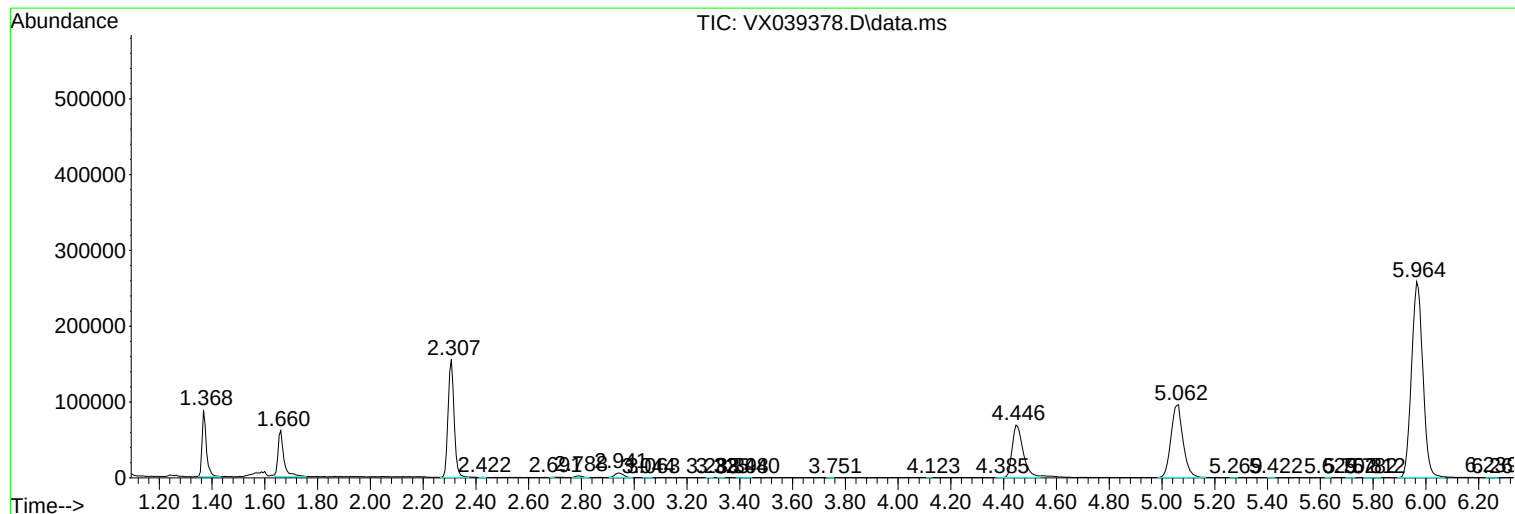

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039378.D
Acq On : 19 Dec 2023 23:32
Operator : JC/MD
Sample : 05835-14DL 10X
Misc : 4.07g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039378.D
Acq On : 19 Dec 2023 23:32
Operator : JC/MD
Sample : 05835-14DL 10X
Misc : 4.07g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc