

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039380.D
 Acq On : 20 Dec 2023 00:17
 Operator : JC/MD
 Sample : 05807-14DL 500X
 Misc : 5.52g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AZ6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039380.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	28	rBV2	1982	2385	0.31%	0.034%
2	1.368	43	46	58	rVB	89284	98849	13.05%	1.423%
3	1.673	91	96	107	rBV	58183	85584	11.30%	1.232%
4	2.307	194	200	213	rBV	161120	256444	33.87%	3.692%
5	2.788	273	279	289	rBV	6159	12634	1.67%	0.182%
6	2.941	299	304	313	rBV3	3292	7194	0.95%	0.104%
7	3.160	338	340	344	rVB2	190	239	0.03%	0.003%
8	3.556	401	405	408	rVB2	166	199	0.03%	0.003%
9	3.611	412	414	417	rVB	191	207	0.03%	0.003%
10	3.703	425	429	430	rBV	137	183	0.02%	0.003%
11	3.721	430	432	434	rVB2	324	246	0.03%	0.004%
12	3.764	434	439	440	rBV2	290	380	0.05%	0.005%
13	4.026	480	482	486	rBV2	224	299	0.04%	0.004%
14	4.105	492	495	497	rBV	204	249	0.03%	0.004%
15	4.446	543	551	564	rBV	65763	190132	25.11%	2.738%
16	4.928	628	630	632	rBV	251	201	0.03%	0.003%
17	4.977	635	638	639	rVV2	162	174	0.02%	0.003%
18	5.056	639	651	670	rVV	92755	300636	39.70%	4.329%
19	5.196	672	674	677	rVV	534	584	0.08%	0.008%
20	5.227	677	679	681	rVV2	414	390	0.05%	0.006%
21	5.288	685	689	691	rVB2	262	241	0.03%	0.003%
22	5.385	702	705	706	rBV3	322	379	0.05%	0.005%
23	5.495	721	723	725	rBV2	214	192	0.03%	0.003%
24	5.550	729	732	733	rBV2	376	359	0.05%	0.005%
25	5.769	765	768	769	rBV	220	195	0.03%	0.003%
26	5.818	775	776	780	rVB2	296	286	0.04%	0.004%
27	5.855	780	782	786	rBV	204	268	0.04%	0.004%
28	5.971	788	801	819	rBV2	249939	757197	100.00%	10.902%
29	6.245	843	846	851	rBV3	210	357	0.05%	0.005%
30	6.653	909	913	914	rBV	273	210	0.03%	0.003%
31	6.678	914	917	918	rVB2	213	179	0.02%	0.003%
32	6.757	920	930	946	rBV	196954	480533	63.46%	6.919%
33	7.117	983	989	996	rVB5	1250	2961	0.39%	0.043%
34	7.306	1011	1020	1038	rBV	158237	345321	45.61%	4.972%
35	7.519	1053	1055	1058	rVB2	299	293	0.04%	0.004%
36	7.610	1065	1070	1071	rBV2	275	404	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039380.D
 Acq On : 20 Dec 2023 00:17
 Operator : JC/MD
 Sample : 05807-14DL 500X
 Misc : 5.52g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AZ6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	8.062	1141	1144	1145	rBV2	233	177	0.02%	0.003%
38	8.324	1181	1187	1201	rBV	101584	169625	22.40%	2.442%
39	8.513	1217	1218	1222	rVB3	372	408	0.05%	0.006%
40	8.562	1224	1226	1228	rBV	206	241	0.03%	0.003%
41	8.647	1234	1240	1255	rBV	375334	595830	78.69%	8.579%
42	8.952	1284	1290	1303	rVV	73075	112353	14.84%	1.618%
43	9.061	1306	1308	1312	rVV3	398	470	0.06%	0.007%
44	9.330	1348	1352	1355	rBV2	257	402	0.05%	0.006%
45	9.385	1355	1361	1379	rVV	305297	455146	60.11%	6.553%
46	9.531	1383	1385	1386	rVB	461	254	0.03%	0.004%
47	9.695	1411	1412	1415	rVB2	379	230	0.03%	0.003%
48	10.049	1465	1470	1489	rVV	420278	612009	80.83%	8.812%
49	10.305	1511	1512	1514	rBV2	259	251	0.03%	0.004%
50	10.525	1544	1548	1550	rBV2	206	296	0.04%	0.004%
51	10.640	1565	1567	1568	rBV2	460	352	0.05%	0.005%
52	10.854	1600	1602	1606	rVB2	212	231	0.03%	0.003%
53	10.964	1617	1620	1624	rVB2	286	380	0.05%	0.005%
54	11.092	1638	1641	1643	rVB2	253	282	0.04%	0.004%
55	11.189	1652	1657	1668	rVV	304598	371511	49.06%	5.349%
56	11.317	1675	1678	1680	rVB	551	517	0.07%	0.007%
57	11.366	1684	1686	1687	rBV	266	196	0.03%	0.003%
58	11.463	1700	1702	1705	rVV3	191	206	0.03%	0.003%
59	11.933	1775	1779	1780	rBV2	201	259	0.03%	0.004%
60	11.976	1782	1786	1788	rBV2	3997	5281	0.70%	0.076%
61	12.018	1788	1793	1807	rVB2	476785	703583	92.92%	10.130%
62	12.165	1816	1817	1820	rVB	364	209	0.03%	0.003%
63	12.317	1837	1842	1858	rVB	416252	551897	72.89%	7.946%
64	12.451	1863	1864	1866	rBV	224	217	0.03%	0.003%
65	12.762	1911	1915	1919	rVV2	2350	3076	0.41%	0.044%
66	12.890	1934	1936	1939	rVB	290	193	0.03%	0.003%
67	12.927	1939	1942	1945	rBV2	676	671	0.09%	0.010%
68	13.061	1959	1964	1970	rVB5	2694	5760	0.76%	0.083%
69	13.116	1970	1973	1979	rBV4	1177	1311	0.17%	0.019%
70	13.384	2012	2017	2021	rVB2	450	611	0.08%	0.009%
71	13.414	2021	2022	2024	rBV2	217	225	0.03%	0.003%
72	13.433	2024	2025	2028	rVB	399	215	0.03%	0.003%
73	13.585	2045	2050	2069	rVB	457196	558068	73.70%	8.035%
74	13.957	2106	2111	2122	rVV	94471	121771	16.08%	1.753%
75	14.128	2135	2139	2144	rVV2	3012	3957	0.52%	0.057%
76	14.170	2144	2146	2149	rVV2	206	234	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039380.D
 Acq On : 20 Dec 2023 00:17
 Operator : JC/MD
 Sample : 05807-14DL 500X
 Misc : 5.52g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AZ6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	14.237	2153	2157	2158	rVV	264	241	0.03%	0.003%
78	14.317	2168	2170	2172	rVB2	227	175	0.02%	0.003%
79	14.353	2172	2176	2178	rVB2	223	279	0.04%	0.004%
80	14.384	2178	2181	2184	rBV2	351	458	0.06%	0.007%
81	14.463	2192	2194	2196	rBV2	219	207	0.03%	0.003%
82	14.542	2202	2207	2209	rBV2	551	658	0.09%	0.009%
83	14.628	2218	2221	2225	rBV4	626	806	0.11%	0.012%
84	14.780	2239	2246	2251	rBV2	17600	26072	3.44%	0.375%
85	14.835	2253	2255	2258	rVB2	265	300	0.04%	0.004%
86	14.865	2258	2260	2261	rBV2	273	228	0.03%	0.003%
87	14.926	2264	2270	2272	rBV3	558	889	0.12%	0.013%
88	15.042	2287	2289	2292	rBV2	194	256	0.03%	0.004%
89	15.243	2317	2322	2329	rVV	60525	85184	11.25%	1.227%
90	15.310	2332	2333	2336	rVB3	299	202	0.03%	0.003%
91	15.597	2379	2380	2383	rBV3	272	255	0.03%	0.004%
92	15.658	2388	2390	2394	rVB	289	213	0.03%	0.003%
93	15.743	2402	2404	2405	rBV2	295	210	0.03%	0.003%
94	15.877	2424	2426	2428	rBV	234	211	0.03%	0.003%
95	16.005	2445	2447	2449	rBV	383	317	0.04%	0.005%
96	16.085	2459	2460	2462	rBV2	335	237	0.03%	0.003%
97	16.438	2516	2518	2521	rVB2	278	282	0.04%	0.004%
98	16.511	2523	2530	2533	rBV3	961	1614	0.21%	0.023%
99	16.560	2536	2538	2540	rVB2	355	272	0.04%	0.004%
100	16.578	2540	2541	2543	rBV2	252	204	0.03%	0.003%

Sum of corrected areas: 6945259




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039380.D
Acq On : 20 Dec 2023 00:17
Operator : JC/MD
Sample : 05807-14DL 500X
Misc : 5.52g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AZ6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

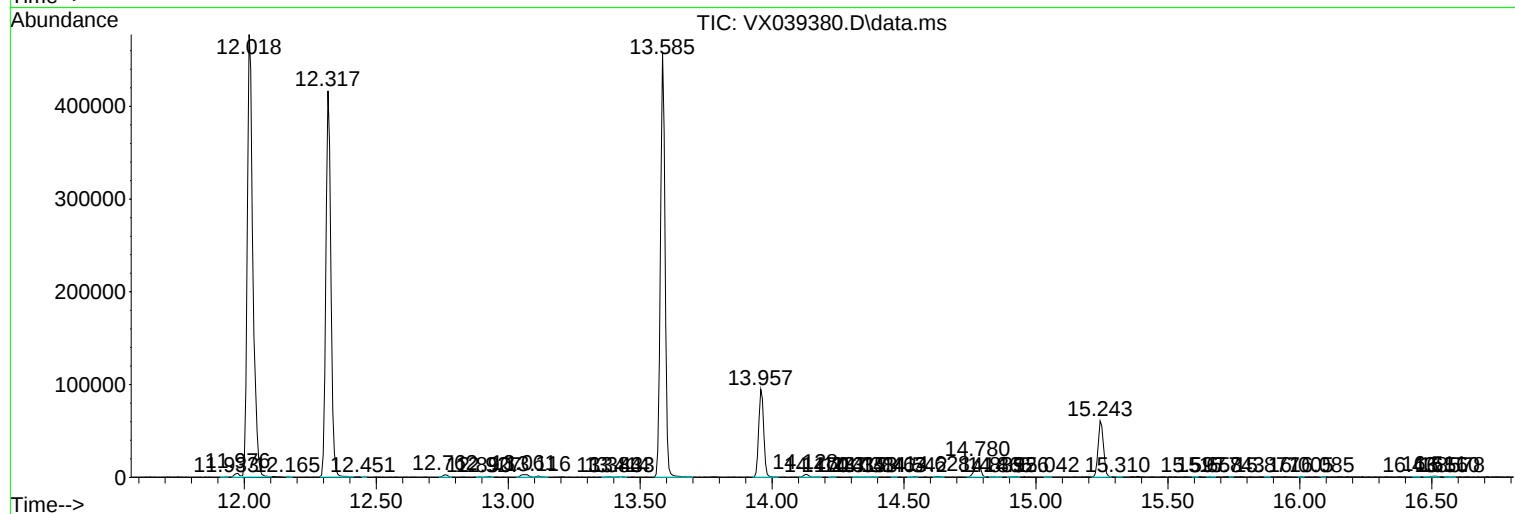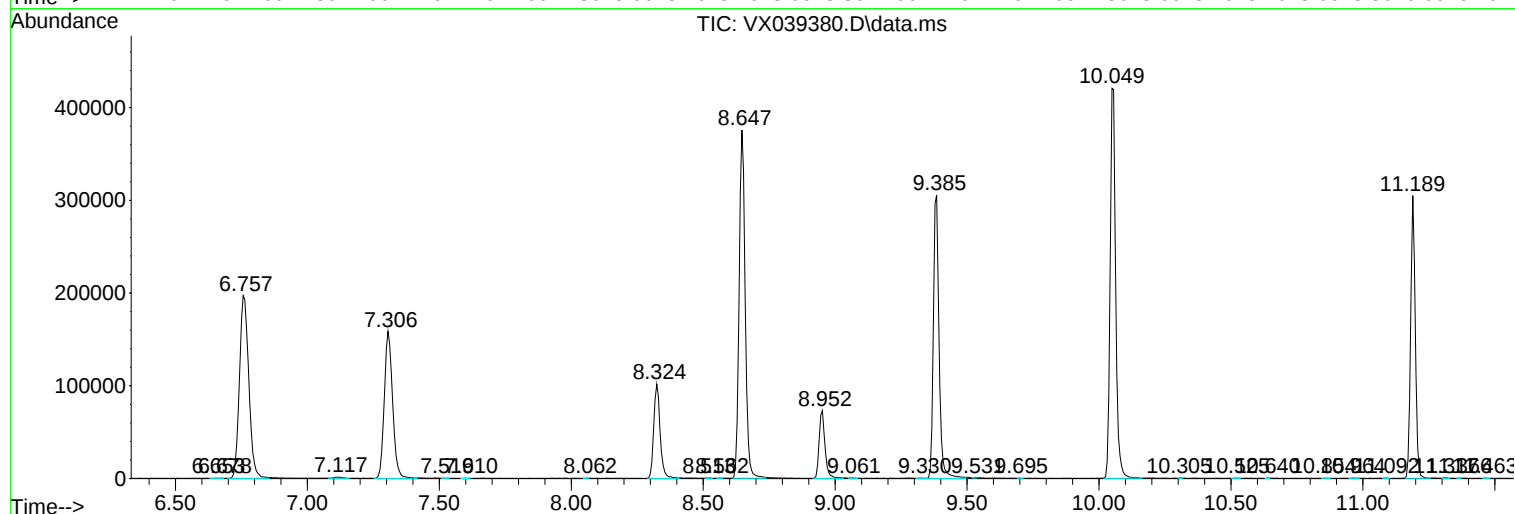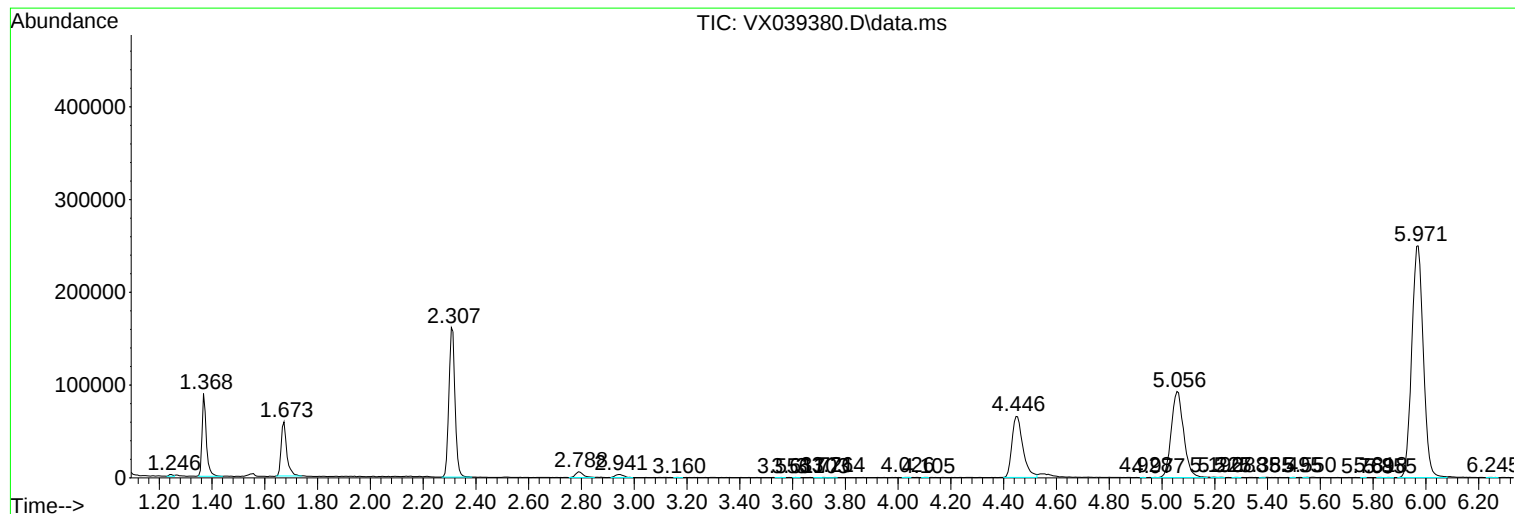

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039380.D
Acq On : 20 Dec 2023 00:17
Operator : JC/MD
Sample : 05807-14DL 500X
Misc : 5.52g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AZ6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039380.D
Acq On : 20 Dec 2023 00:17
Operator : JC/MD
Sample : 05807-14DL 500X
Misc : 5.52g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AZ6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc