

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039382.D
 Acq On : 20 Dec 2023 01:03
 Operator : JC/MD
 Sample : 05869-08 100X
 Misc : 3.72g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AT4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039382.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	61	rBV	96094	106248	13.75%	1.753%
2	1.666	91	95	107	rVB	61409	92297	11.95%	1.522%
3	2.307	194	200	216	rVB	168997	269385	34.87%	4.444%
4	2.416	216	218	220	rVB	367	257	0.03%	0.004%
5	2.441	220	222	223	rVB2	367	235	0.03%	0.004%
6	2.459	223	225	227	rBV	254	244	0.03%	0.004%
7	2.569	242	243	246	rBV2	213	189	0.02%	0.003%
8	2.697	262	264	266	rBV	367	299	0.04%	0.005%
9	2.788	275	279	285	rVB4	1513	2734	0.35%	0.045%
10	2.867	288	292	295	rBV2	228	389	0.05%	0.006%
11	2.941	297	304	313	rVV	3823	8210	1.06%	0.135%
12	3.014	315	316	321	rVB	250	192	0.02%	0.003%
13	3.050	321	322	324	rVB	277	181	0.02%	0.003%
14	3.117	331	333	336	rBV2	231	250	0.03%	0.004%
15	3.373	372	375	377	rBV2	183	251	0.03%	0.004%
16	3.520	396	399	400	rVB2	219	207	0.03%	0.003%
17	3.532	400	401	402	rBV	287	162	0.02%	0.003%
18	3.550	402	404	406	rVV2	222	207	0.03%	0.003%
19	3.727	430	433	434	rBV2	182	198	0.03%	0.003%
20	3.800	442	445	448	rBV2	171	257	0.03%	0.004%
21	3.843	448	452	455	rBV2	180	277	0.04%	0.005%
22	3.983	472	475	476	rBV2	176	199	0.03%	0.003%
23	4.014	479	480	484	rVV2	290	337	0.04%	0.006%
24	4.129	497	499	503	rVV2	223	280	0.04%	0.005%
25	4.288	523	525	528	rBV	153	166	0.02%	0.003%
26	4.446	542	551	565	rBV	66394	192343	24.90%	3.173%
27	5.056	639	651	672	rBV	93808	303727	39.31%	5.010%
28	5.385	701	705	708	rBV4	342	525	0.07%	0.009%
29	5.452	714	716	721	rVB2	337	365	0.05%	0.006%
30	5.623	740	744	747	rVB2	189	254	0.03%	0.004%
31	5.647	747	748	750	rBV	219	173	0.02%	0.003%
32	5.727	759	761	762	rVV	294	157	0.02%	0.003%
33	5.971	788	801	819	rBV2	256620	772584	100.00%	12.744%
34	6.233	842	844	847	rVB2	326	286	0.04%	0.005%
35	6.355	862	864	867	rBV2	213	259	0.03%	0.004%
36	6.422	874	875	878	rVB	204	182	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039382.D
 Acq On : 20 Dec 2023 01:03
 Operator : JC/MD
 Sample : 05869-08 100X
 Misc : 3.72g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COAT4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	6.672	913	916	919	rBV2	153	207	0.03%	0.003%
38	6.757	921	930	944	rBV	194421	472960	61.22%	7.802%
39	7.111	984	988	995	rVB3	1343	2450	0.32%	0.040%
40	7.202	1000	1003	1005	rBV2	222	227	0.03%	0.004%
41	7.306	1012	1020	1034	rBV	160676	351088	45.44%	5.791%
42	7.665	1077	1079	1080	rBV	300	188	0.02%	0.003%
43	7.891	1114	1116	1120	rBV2	247	258	0.03%	0.004%
44	7.958	1124	1127	1129	rVV2	274	236	0.03%	0.004%
45	8.165	1160	1161	1164	rVB2	221	181	0.02%	0.003%
46	8.214	1167	1169	1172	rVB2	255	238	0.03%	0.004%
47	8.257	1172	1176	1177	rBV2	241	240	0.03%	0.004%
48	8.324	1181	1187	1202	rBV	105602	175138	22.67%	2.889%
49	8.470	1209	1211	1213	rVB2	328	191	0.02%	0.003%
50	8.519	1216	1219	1220	rBV3	279	236	0.03%	0.004%
51	8.580	1227	1229	1234	rBV2	491	658	0.09%	0.011%
52	8.647	1234	1240	1249	rBV	391145	608137	78.71%	10.032%
53	8.952	1284	1290	1302	rBV	72997	114394	14.81%	1.887%
54	9.086	1311	1312	1318	rBV2	258	374	0.05%	0.006%
55	9.275	1340	1343	1348	rBV3	295	421	0.05%	0.007%
56	9.385	1355	1361	1375	rBV	307639	452629	58.59%	7.466%
57	9.653	1403	1405	1409	rBV2	278	384	0.05%	0.006%
58	9.689	1409	1411	1412	rBV	360	300	0.04%	0.005%
59	9.860	1438	1439	1442	rVB2	251	187	0.02%	0.003%
60	10.055	1465	1471	1489	rVB	407107	602560	77.99%	9.940%
61	10.439	1531	1534	1536	rBV2	304	332	0.04%	0.005%
62	10.464	1536	1538	1540	rVV2	261	222	0.03%	0.004%
63	10.488	1540	1542	1544	rVB	455	378	0.05%	0.006%
64	10.512	1544	1546	1549	rBV	189	254	0.03%	0.004%
65	10.653	1565	1569	1572	rVB3	382	543	0.07%	0.009%
66	10.823	1596	1597	1599	rBV	305	168	0.02%	0.003%
67	11.189	1652	1657	1666	rBV	296246	372349	48.20%	6.142%
68	11.366	1682	1686	1691	rVB2	3405	4522	0.59%	0.075%
69	11.451	1697	1700	1706	rBV2	412	817	0.11%	0.013%
70	11.622	1726	1728	1731	rBV2	160	205	0.03%	0.003%
71	11.713	1737	1743	1745	rBV2	265	544	0.07%	0.009%
72	11.976	1782	1786	1788	rBV3	621	844	0.11%	0.014%
73	12.018	1788	1793	1804	rBV	467696	603917	78.17%	9.962%
74	12.317	1837	1842	1849	rBV	406052	527144	68.23%	8.695%
75	12.512	1872	1874	1876	rVB2	343	192	0.02%	0.003%
76	12.549	1878	1880	1882	rVB2	270	240	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039382.D
 Acq On : 20 Dec 2023 01:03
 Operator : JC/MD
 Sample : 05869-08 100X
 Misc : 3.72g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AT4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

77	12.597	1886	1888	1890	rBV2	186	197	0.03%	0.003%
78	12.762	1911	1915	1919	rBV	1135	1450	0.19%	0.024%
79	12.811	1922	1923	1927	rBV	215	309	0.04%	0.005%
80	12.914	1938	1940	1942	rBV	267	181	0.02%	0.003%
81	12.969	1946	1949	1950	rBV2	135	183	0.02%	0.003%
82	13.384	2013	2017	2019	rBV	214	188	0.02%	0.003%
83	13.591	2048	2051	2056	rBV2	1342	1627	0.21%	0.027%
84	13.847	2089	2093	2094	rBV2	196	265	0.03%	0.004%
85	13.963	2109	2112	2116	rBV	425	586	0.08%	0.010%
86	14.128	2135	2139	2144	rVB2	2162	2953	0.38%	0.049%
87	14.243	2156	2158	2161	rBV	237	288	0.04%	0.005%
88	14.280	2163	2164	2165	rBV	249	163	0.02%	0.003%
89	14.640	2221	2223	2226	rBV2	171	209	0.03%	0.003%
90	14.713	2234	2235	2238	rBV2	224	196	0.03%	0.003%
91	14.762	2241	2243	2246	rVV2	211	177	0.02%	0.003%
92	14.884	2262	2263	2265	rVB	382	205	0.03%	0.003%
93	15.158	2307	2308	2309	rBV	328	170	0.02%	0.003%
94	15.249	2320	2323	2329	rVB4	273	432	0.06%	0.007%
95	15.646	2386	2388	2389	rVB	314	158	0.02%	0.003%
96	16.072	2456	2458	2461	rVB	456	318	0.04%	0.005%
97	16.109	2461	2464	2465	rBV2	281	256	0.03%	0.004%
98	16.267	2488	2490	2493	rVB2	250	239	0.03%	0.004%
99	16.499	2526	2528	2530	rBV2	309	225	0.03%	0.004%
100	16.676	2554	2557	2558	rBV3	257	235	0.03%	0.004%



Sum of corrected areas: 6062269

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039382.D
Acq On : 20 Dec 2023 01:03
Operator : JC/MD
Sample : 05869-08 100X
Misc : 3.72g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AT4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

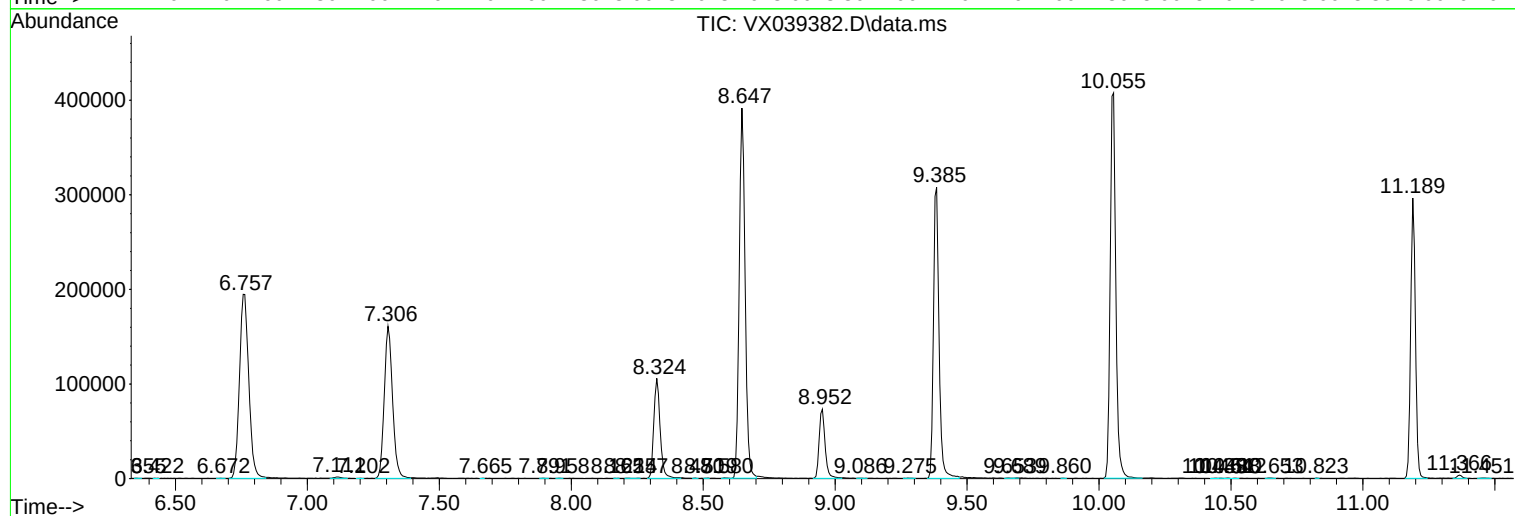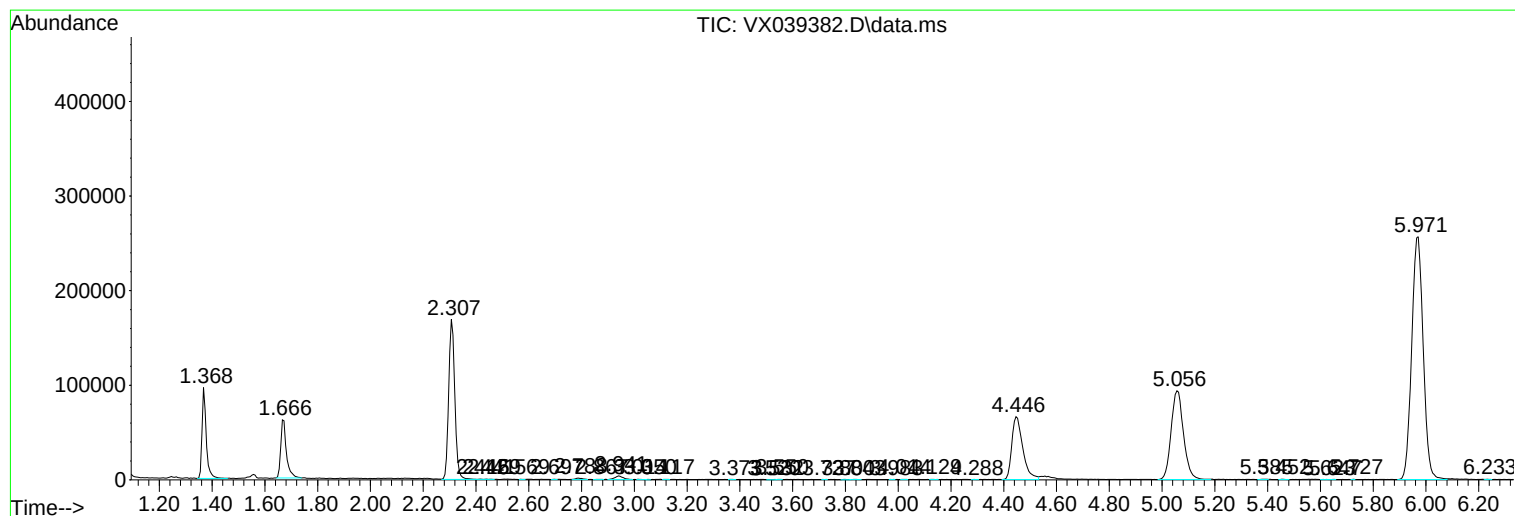

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039382.D
Acq On : 20 Dec 2023 01:03
Operator : JC/MD
Sample : 05869-08 100X
Misc : 3.72g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AT4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039382.D
Acq On : 20 Dec 2023 01:03
Operator : JC/MD
Sample : 05869-08 100X
Misc : 3.72g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AT4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------