

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039383.D
 Acq On : 20 Dec 2023 01:26
 Operator : JC/MD
 Sample : 05835-19 100X
 Misc : 4.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039383.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	58	rVB	88069	98423	4.71%	1.136%
2	1.672	91	96	107	rVB	54933	85774	4.11%	0.990%
3	2.306	194	200	221	rVB	158217	250891	12.01%	2.895%
4	2.690	261	263	264	rBV	340	260	0.01%	0.003%
5	2.794	275	280	284	rBV2	1567	2608	0.12%	0.030%
6	2.946	297	305	311	rVV2	3550	8096	0.39%	0.093%
7	3.093	327	329	331	rBV	286	315	0.02%	0.004%
8	3.312	363	365	366	rBV	293	231	0.01%	0.003%
9	3.361	371	373	375	rVB	243	169	0.01%	0.002%
10	3.648	419	420	423	rBV2	238	241	0.01%	0.003%
11	3.727	431	433	439	rVB2	214	327	0.02%	0.004%
12	3.776	439	441	443	rBV2	182	213	0.01%	0.002%
13	3.983	473	475	477	rVV2	175	197	0.01%	0.002%
14	4.129	497	499	502	rBV	173	172	0.01%	0.002%
15	4.446	542	551	564	rBV	66721	194451	9.31%	2.244%
16	4.928	629	630	633	rBV2	223	186	0.01%	0.002%
17	5.056	638	651	671	rBV	92979	301166	14.42%	3.475%
18	5.391	704	706	708	rVV	254	292	0.01%	0.003%
19	5.434	711	713	716	rVV2	221	227	0.01%	0.003%
20	5.470	717	719	723	rVV2	190	173	0.01%	0.002%
21	5.873	783	785	787	rVB2	268	179	0.01%	0.002%
22	5.970	789	801	809	rBV2	246157	753401	36.07%	8.693%
23	6.330	857	860	861	rBV2	164	167	0.01%	0.002%
24	6.513	886	890	893	rVB	198	179	0.01%	0.002%
25	6.543	893	895	899	rBV2	203	194	0.01%	0.002%
26	6.598	901	904	907	rBV2	186	305	0.01%	0.004%
27	6.763	921	931	946	rBV	187645	453260	21.70%	5.230%
28	7.110	984	988	989	rBV3	1114	1397	0.07%	0.016%
29	7.171	996	998	999	rBV	316	168	0.01%	0.002%
30	7.214	1003	1005	1006	rBV	316	236	0.01%	0.003%
31	7.305	1011	1020	1032	rBV	155626	343574	16.45%	3.964%
32	7.610	1068	1070	1076	rVB2	184	234	0.01%	0.003%
33	7.659	1076	1078	1081	rVB	200	237	0.01%	0.003%
34	7.690	1081	1083	1086	rBV	188	232	0.01%	0.003%
35	7.915	1118	1120	1121	rBV	178	170	0.01%	0.002%
36	7.982	1129	1131	1134	rVB2	234	263	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039383.D
 Acq On : 20 Dec 2023 01:26
 Operator : JC/MD
 Sample : 05835-19 100X
 Misc : 4.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	8.055	1140	1143	1145	rVV	161	168	0.01%	0.002%
38	8.177	1159	1163	1165	rVB2	162	166	0.01%	0.002%
39	8.324	1181	1187	1202	rVV	101431	167107	8.00%	1.928%
40	8.525	1218	1220	1222	rVB2	214	202	0.01%	0.002%
41	8.647	1234	1240	1259	rBV	370704	586196	28.07%	6.763%
42	8.951	1284	1290	1301	rBV	72727	112170	5.37%	1.294%
43	9.128	1316	1319	1320	rVB2	200	182	0.01%	0.002%
44	9.275	1340	1343	1347	rBV	243	286	0.01%	0.003%
45	9.384	1355	1361	1374	rBV	312909	461708	22.11%	5.327%
46	9.695	1409	1412	1416	rVB2	486	789	0.04%	0.009%
47	10.079	1465	1475	1491	rBV2	1117510	2088451	100.00%	24.096%
48	10.305	1508	1512	1516	rBV4	352	598	0.03%	0.007%
49	10.354	1519	1520	1523	rVB2	235	177	0.01%	0.002%
50	10.390	1523	1526	1529	rVB	212	251	0.01%	0.003%
51	10.415	1529	1530	1532	rBV	283	206	0.01%	0.002%
52	10.433	1532	1533	1536	rVB	409	204	0.01%	0.002%
53	10.500	1539	1544	1547	rBV2	178	339	0.02%	0.004%
54	10.640	1565	1567	1572	rVB2	350	480	0.02%	0.006%
55	10.701	1575	1577	1580	rVB2	202	179	0.01%	0.002%
56	10.732	1580	1582	1583	rBV	271	186	0.01%	0.002%
57	10.750	1583	1585	1588	rVB2	197	196	0.01%	0.002%
58	10.878	1602	1606	1608	rVB2	171	231	0.01%	0.003%
59	10.902	1608	1610	1614	rVB2	208	219	0.01%	0.003%
60	10.945	1614	1617	1618	rBV	224	198	0.01%	0.002%
61	11.097	1640	1642	1645	rBV2	272	253	0.01%	0.003%
62	11.189	1652	1657	1667	rBV	291811	372369	17.83%	4.296%
63	11.366	1682	1686	1690	rBV	1106	1645	0.08%	0.019%
64	11.463	1697	1702	1704	rBV4	769	884	0.04%	0.010%
65	11.731	1744	1746	1748	rBV2	179	194	0.01%	0.002%
66	11.969	1780	1785	1789	rBV	43197	54467	2.61%	0.628%
67	12.036	1789	1796	1807	rVB2	845664	1601581	76.69%	18.479%
68	12.189	1820	1821	1822	rBV	330	170	0.01%	0.002%
69	12.317	1837	1842	1860	rBV2	418514	632772	30.30%	7.301%
70	12.591	1886	1887	1891	rVV2	244	344	0.02%	0.004%
71	12.640	1893	1895	1899	rVV2	191	204	0.01%	0.002%
72	12.725	1905	1909	1910	rVB2	205	232	0.01%	0.003%
73	12.762	1910	1915	1919	rBV2	2336	3305	0.16%	0.038%
74	13.018	1955	1957	1959	rVV2	205	173	0.01%	0.002%
75	13.067	1959	1965	1969	rVV3	6366	12101	0.58%	0.140%
76	13.115	1970	1973	1978	rVV2	1335	1681	0.08%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039383.D
 Acq On : 20 Dec 2023 01:26
 Operator : JC/MD
 Sample : 05835-19 100X
 Misc : 4.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

77	13.390	2014	2018	2021	rVV2	225	302	0.01%	0.003%
78	13.585	2046	2050	2063	rVV	24599	34207	1.64%	0.395%
79	13.786	2079	2083	2087	rVB2	427	594	0.03%	0.007%
80	13.829	2087	2090	2092	rBV2	200	211	0.01%	0.002%
81	13.963	2107	2112	2118	rVB2	14158	19126	0.92%	0.221%
82	14.127	2135	2139	2143	rVB2	2630	3263	0.16%	0.038%
83	14.237	2154	2157	2160	rBV2	291	254	0.01%	0.003%
84	14.524	2201	2204	2208	rBV2	275	368	0.02%	0.004%
85	14.688	2226	2231	2235	rBV2	306	647	0.03%	0.007%
86	14.749	2237	2241	2242	rBV	353	370	0.02%	0.004%
87	14.780	2242	2246	2249	rVB3	465	541	0.03%	0.006%
88	14.816	2249	2252	2255	rBV2	324	468	0.02%	0.005%
89	14.883	2260	2263	2264	rBV	262	203	0.01%	0.002%
90	14.975	2276	2278	2280	rBV2	215	285	0.01%	0.003%
91	15.085	2294	2296	2297	rBV	385	192	0.01%	0.002%
92	15.103	2297	2299	2301	rVB	294	196	0.01%	0.002%
93	15.255	2319	2324	2330	rBV3	1123	1921	0.09%	0.022%
94	15.395	2342	2347	2352	rVB4	543	812	0.04%	0.009%
95	15.517	2365	2367	2368	rBV	328	238	0.01%	0.003%
96	15.536	2368	2370	2371	rBV	238	161	0.01%	0.002%
97	15.670	2390	2392	2393	rBV	289	209	0.01%	0.002%
98	15.761	2404	2407	2408	rVB	386	304	0.01%	0.004%
99	16.072	2455	2458	2459	rBV2	229	226	0.01%	0.003%
100	16.084	2459	2460	2461	rBV	370	193	0.01%	0.002%




Sum of corrected areas: 8667163

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039383.D
Acq On : 20 Dec 2023 01:26
Operator : JC/MD
Sample : 05835-19 100X
Misc : 4.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

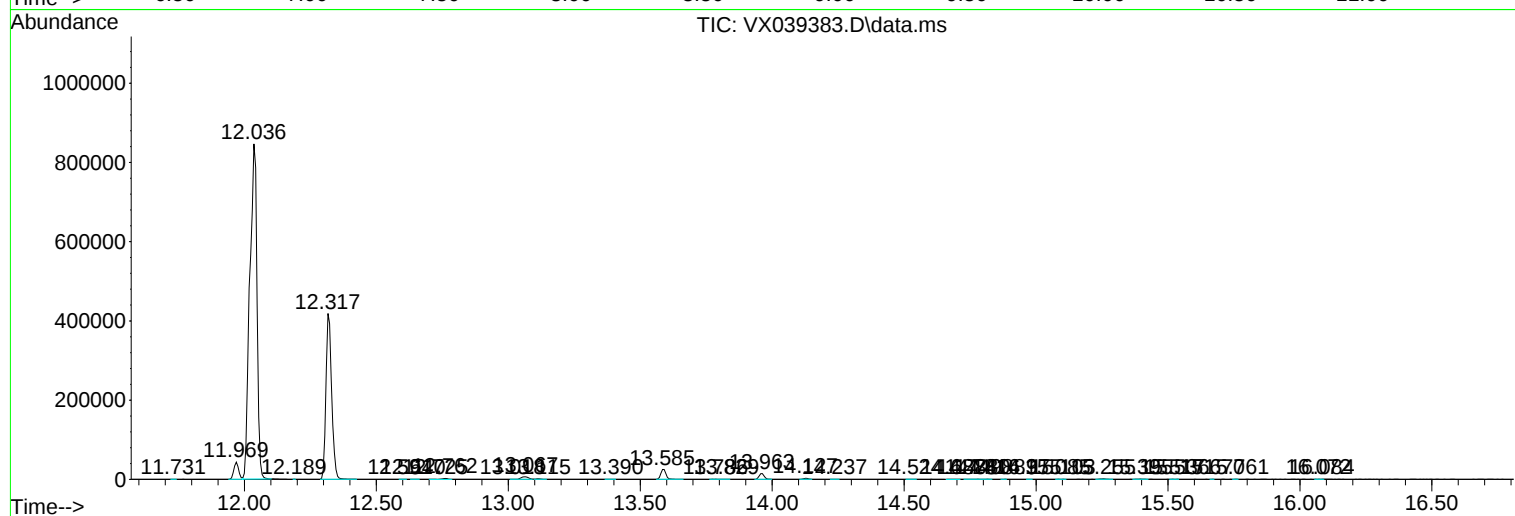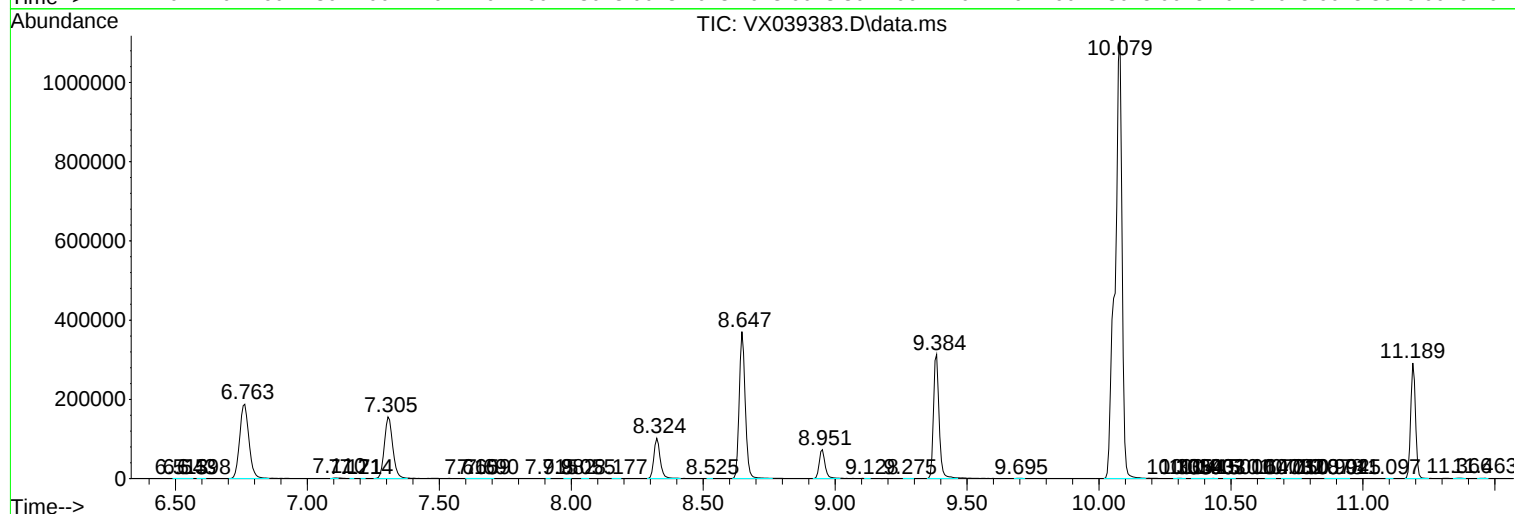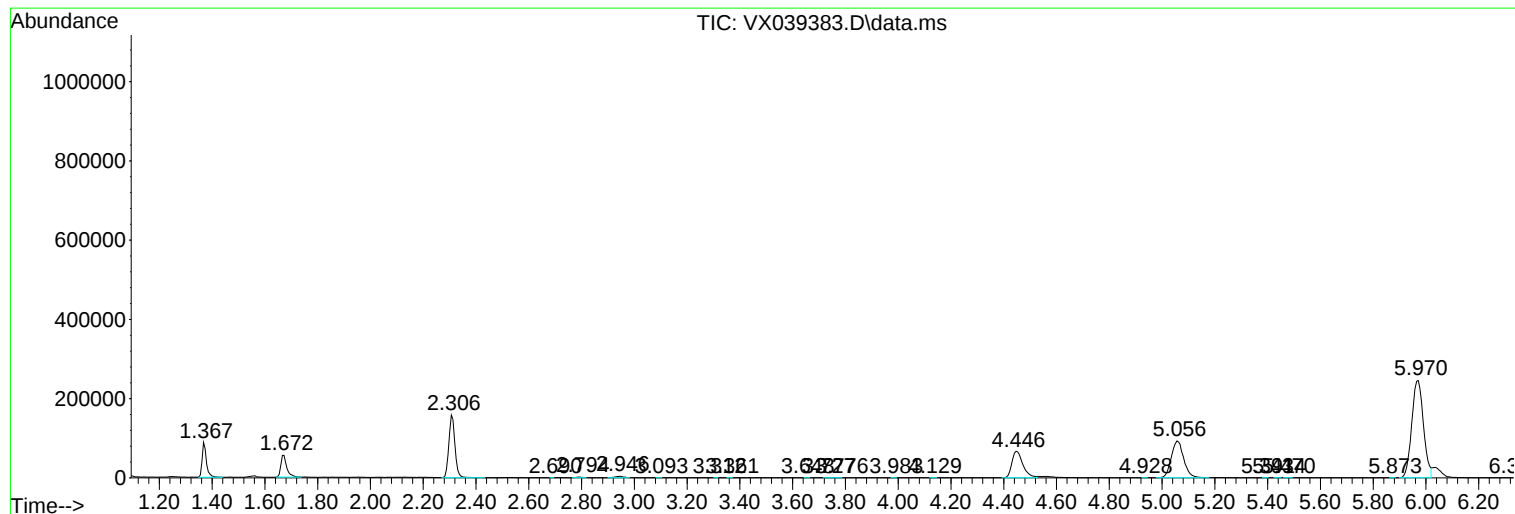

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039383.D
Acq On : 20 Dec 2023 01:26
Operator : JC/MD
Sample : 05835-19 100X
Misc : 4.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039383.D
Acq On : 20 Dec 2023 01:26
Operator : JC/MD
Sample : 05835-19 100X
Misc : 4.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------