
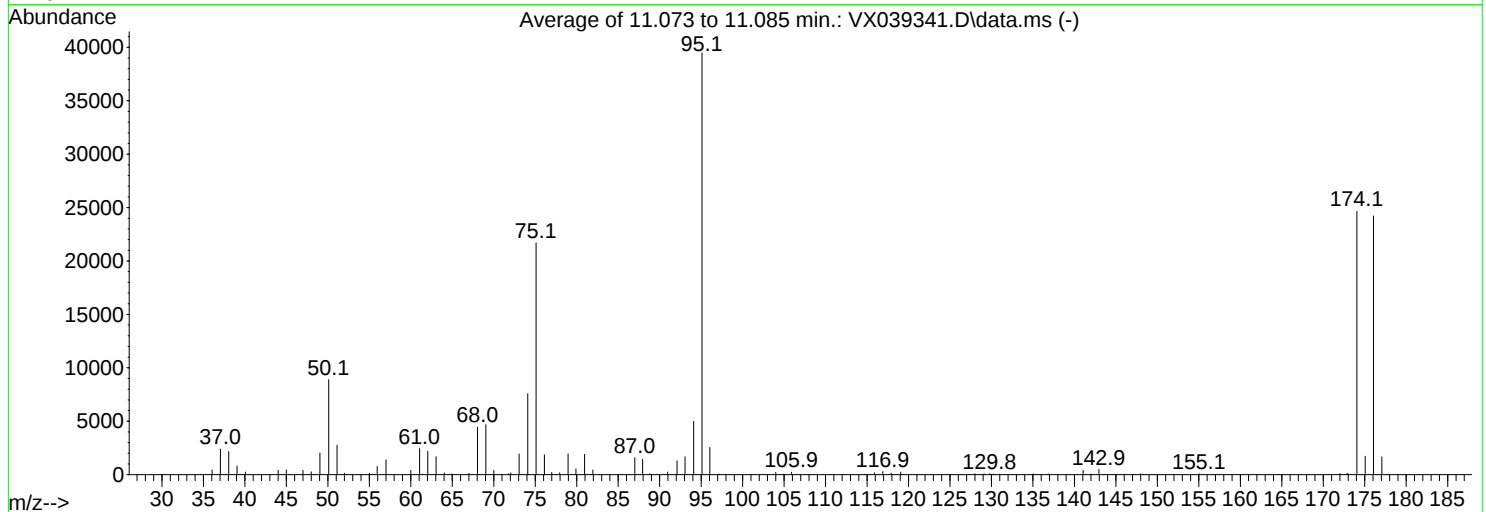


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039341.D
Acq On : 19 Dec 2023 08:59
Operator : JC/MD
Sample : BFB657
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB657

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Title : VOC Analysis
Last Update : Fri Dec 22 00:41:09 2023

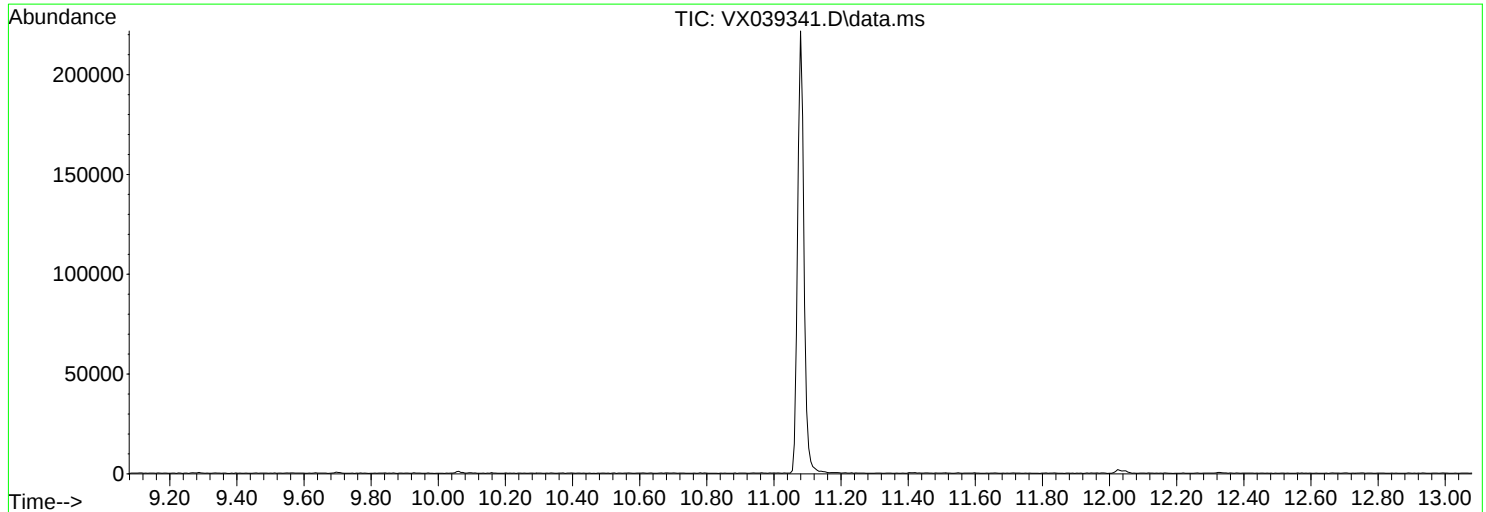

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	8892	PASS
75	95	30	80	54.9	21696	PASS
95	95	100	100	100.0	39485	PASS
96	95	5	9	6.5	2548	PASS
173	174	0.00	2	0.5	135	PASS
174	95	50	120	62.4	24653	PASS
175	174	5	9	7.0	1724	PASS
176	174	95	101	98.2	24216	PASS
177	176	5	9	6.9	1671	PASS

m/z	Abundance
39.80	223.0
44.00	155.0

Instrument :
MSVOA_X
ClientSampleId :
BFB657

m/z	Abundance
36.00	348.0
37.00	2283.0
38.10	2266.0
39.10	880.0
40.10	245.0
44.00	654.0
45.00	472.0
47.00	345.0
48.00	262.0
49.00	1916.0
50.10	8498.0
51.10	2484.0
52.00	123.0
55.00	157.0
56.00	793.0
57.00	1408.0
59.90	385.0
61.00	2300.0
62.00	1819.0
63.00	1610.0
64.00	178.0
64.90	85.0
67.00	97.0
68.00	4267.0
69.10	4109.0
70.00	292.0
71.80	255.0
73.10	1640.0
74.10	6717.0
75.10	19560.0
76.10	1845.0
77.00	234.0
78.00	169.0
78.90	1740.0
79.90	477.0
80.90	1834.0
81.90	260.0
87.00	1182.0
87.90	1064.0
88.80	93.0
91.00	265.0
92.10	1064.0
93.10	1627.0
94.10	4745.0
95.10	36088.0
96.10	2425.0
97.20	51.0
104.00	194.0
104.90	68.0
105.90	157.0
112.10	51.0
115.90	165.0
116.90	192.0
117.90	113.0
119.00	231.0
129.10	60.0
129.80	143.0
131.00	60.0
135.10	62.0
136.80	91.0
141.10	322.0
143.00	328.0
146.00	51.0
147.90	120.0
155.10	63.0
172.00	103.0
172.80	167.0
174.00	18360.0
175.00	1309.0
176.00	18328.0
177.10	1373.0

Instrument :
MSVOA_X
ClientSampleId :
BFB657

m/z	Abundance
36.10	576.0
37.00	2832.0
38.10	2486.0
39.10	798.0
40.00	245.0
44.00	607.0
45.00	452.0
47.10	467.0
48.00	352.0
49.00	2490.0
50.10	10465.0
51.10	3351.0
52.00	120.0
55.00	188.0
55.90	984.0
57.00	1716.0
60.00	398.0
61.10	2952.0
62.00	2656.0
63.10	1956.0
64.10	191.0
65.00	65.0
67.00	183.0
68.10	4972.0
69.00	5566.0
70.00	506.0
72.10	257.0
73.10	2316.0
74.10	8960.0
75.10	26224.0
76.10	2215.0
77.00	249.0
77.80	128.0
79.00	2312.0
79.90	642.0
81.00	2124.0
82.00	620.0
82.80	54.0
87.00	2076.0
88.00	1692.0
88.80	147.0
91.00	250.0
92.10	1492.0
93.00	1913.0
94.10	5798.0
95.10	46136.0
96.10	2855.0
97.20	78.0
104.00	258.0
104.90	57.0
105.90	328.0
109.90	57.0
112.10	56.0
114.80	79.0
115.90	202.0
116.90	339.0
117.80	177.0
119.00	255.0
128.00	154.0
129.10	104.0
129.80	162.0
131.00	71.0
135.10	66.0
136.90	109.0
141.00	532.0
142.00	82.0
142.90	571.0
145.10	58.0
146.00	86.0
147.10	91.0
148.00	74.0
155.00	65.0
172.00	103.0
172.50	82.0
173.00	194.0
174.10	29384.0
175.10	2000.0
176.10	27944.0
177.00	1920.0
177.90	77.0

Instrument :
MSVOA_X
ClientSampleId :
BFB657

m/z	Abundance
36.00	398.0
37.10	2070.0
38.00	1732.0
39.00	738.0
40.00	229.0
44.00	427.0
45.00	367.0
46.90	385.0
48.10	198.0
49.10	1653.0
50.10	7714.0
51.10	2439.0
52.00	155.0
55.10	70.0
56.00	523.0
57.00	1051.0
60.10	449.0
61.00	2081.0
62.10	2074.0
63.10	1453.0
64.00	136.0
64.90	71.0
67.00	98.0
68.10	4087.0
69.00	4328.0
70.00	380.0
72.00	235.0
73.00	1832.0
74.10	7082.0
75.10	19304.0
76.10	1500.0
77.10	129.0
78.00	240.0
79.00	1806.0
79.90	497.0
80.90	1769.0
81.90	417.0
87.00	1498.0
88.00	1611.0
90.90	214.0
92.10	1301.0
93.00	1460.0
94.10	4438.0
95.10	36232.0
96.00	2363.0
104.00	174.0
105.90	172.0
115.90	169.0
116.90	322.0
118.00	162.0
119.10	225.0
128.00	133.0
129.10	54.0
130.20	123.0
131.00	68.0
135.00	78.0
141.00	409.0
142.00	81.0
143.00	570.0
147.90	97.0
155.00	91.0
156.80	52.0
172.00	103.0
172.90	211.0
174.00	26216.0
175.00	1862.0
176.10	26376.0
177.10	1719.0
177.90	97.0

Instrument :
MSVOA_X
ClientSampleId :
BFB657