


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX122018\  
Data File : VX006661.D  
Acq On : 20 Dec 2018 08:31  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X121818W.M  
Title : SW846 8260  
Last Update : Wed Dec 19 15:20:58 2018

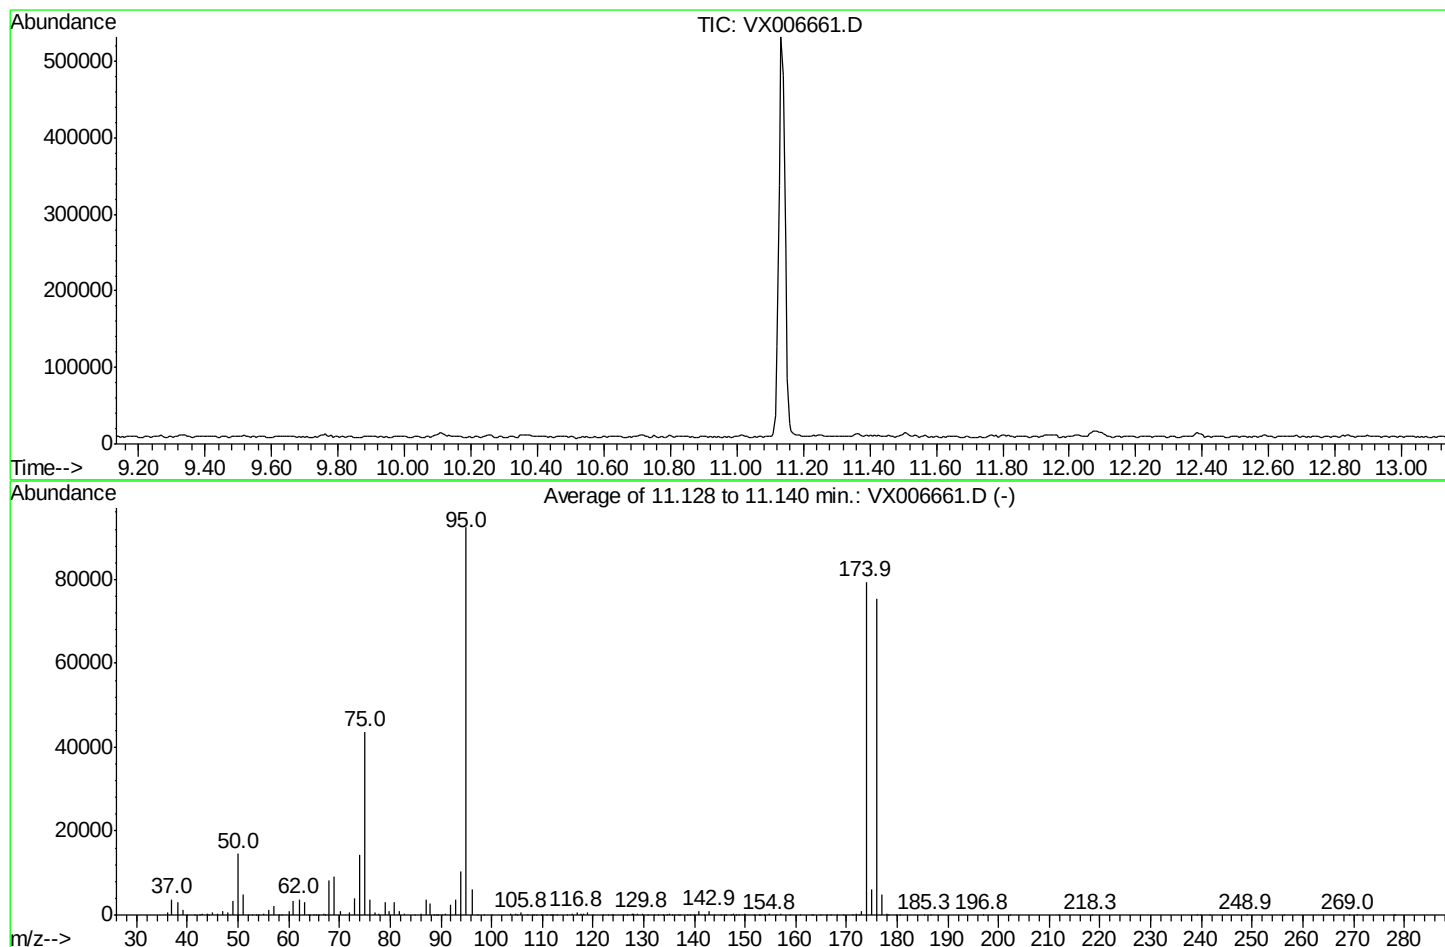

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1626

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 15.8      | 14618   | PASS             |
| 75          | 95           | 30           | 60           | 47.3      | 43736   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 92416   | PASS             |
| 96          | 95           | 5            | 9            | 6.6       | 6126    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.2       | 976     | PASS             |
| 174         | 95           | 50           | 100          | 85.9      | 79378   | PASS             |
| 175         | 174          | 5            | 9            | 7.7       | 6110    | PASS             |
| 176         | 174          | 95           | 101          | 94.9      | 75330   | PASS             |
| 177         | 176          | 5            | 9            | 6.6       | 4970    | PASS             |