


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX122018\
Data File : VX006688.D
Acq On : 20 Dec 2018 20:41
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121818W.M
Title : SW846 8260
Last Update : Wed Dec 19 15:20:58 2018

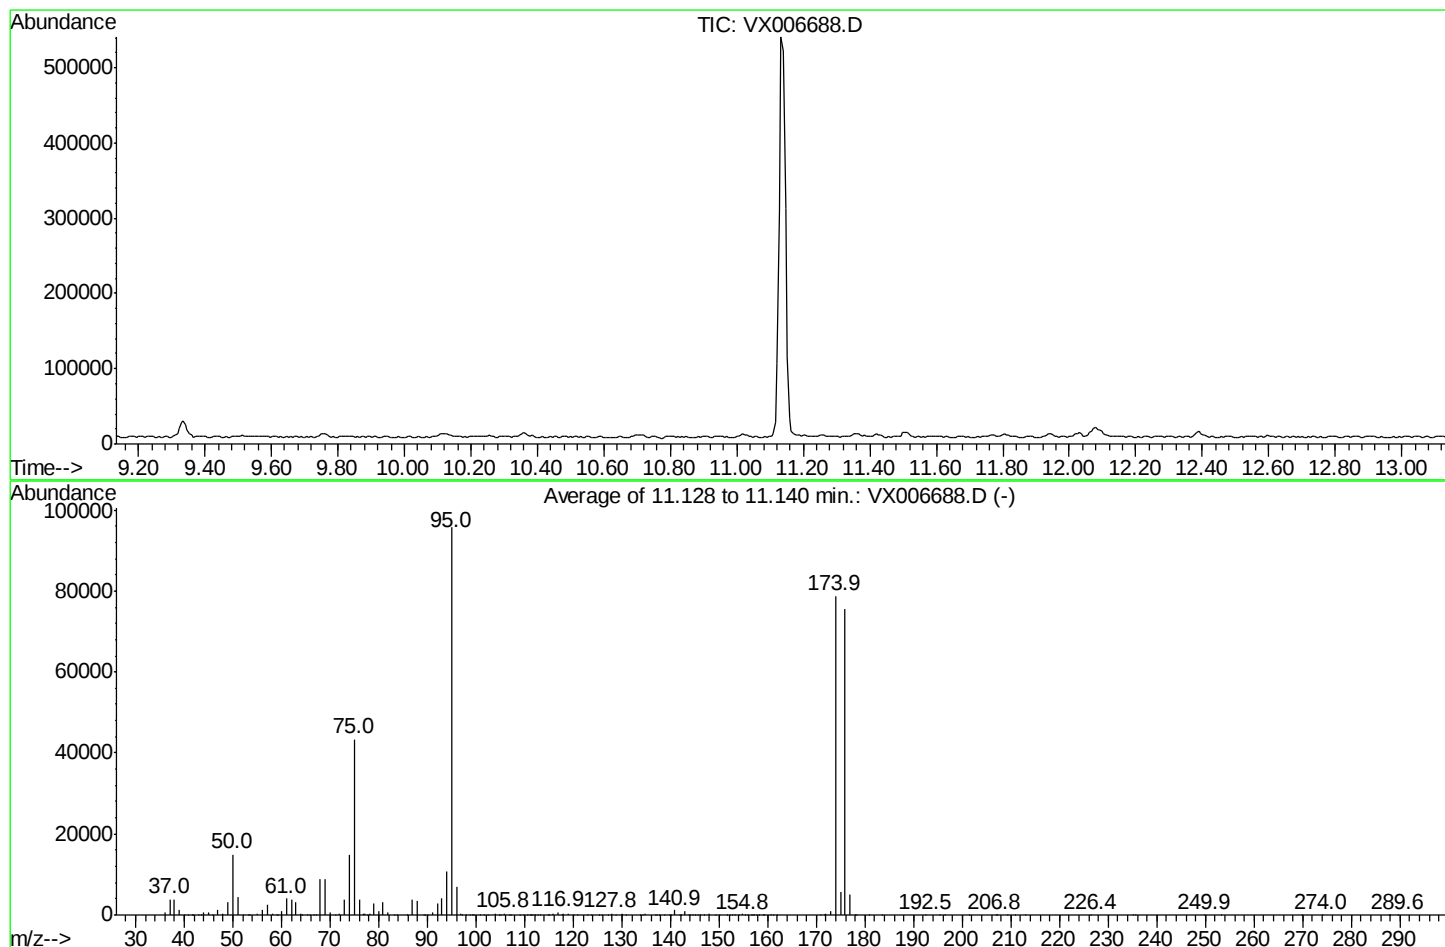

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	15005	PASS
75	95	30	60	45.3	43403	PASS
95	95	100	100	100.0	95714	PASS
96	95	5	9	7.2	6879	PASS
173	174	0.00	2	1.2	921	PASS
174	95	50	100	82.2	78701	PASS
175	174	5	9	7.2	5650	PASS
176	174	95	101	96.0	75541	PASS
177	176	5	9	6.6	4987	PASS