

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025923.D
 Acq On : 20 Dec 2021 18:51
 Operator : JC/MD
 Sample : M5150-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW1

Quant Time: Dec 21 02:03:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 21 01:32:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	159251	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	156694	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	67831	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	62772	48.892	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	97.780%		
7) Chloroethane-d5	1.666	69	54197	50.551	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	101.100%		
11) 1,1-Dichloroethene-d2	2.306	63	86847	38.946	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	77.900%		
21) 2-Butanone-d5	4.458	46	99804	107.755	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	107.760%		
24) Chloroform-d	5.062	84	119013	48.357	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.720%		
26) 1,2-Dichloroethane-d4	5.958	65	81888	51.015	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.040%		
32) Benzene-d6	5.976	84	236829	49.887	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.780%		
36) 1,2-Dichloropropane-d6	7.312	67	72772	50.329	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	100.660%		
41) Toluene-d8	8.653	98	215586	47.828	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.660%		
43) trans-1,3-Dichloroprop...	8.951	79	27361	42.858	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	85.720%		
47) 2-Hexanone-d5	9.384	63	67871	104.421	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	104.420%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	100475	49.051	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.100%		
66) 1,2-Dichlorobenzene-d4	12.323	152	73122	51.142	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.280%		
Target Compounds					Qvalue	
13) Acetone	2.379	43	14198	19.161	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025923.D
Acq On : 20 Dec 2021 18:51
Operator : JC/MD
Sample : M5150-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBW1

Quant Time: Dec 21 02:03:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 21 01:32:07 2021
Response via : Initial Calibration

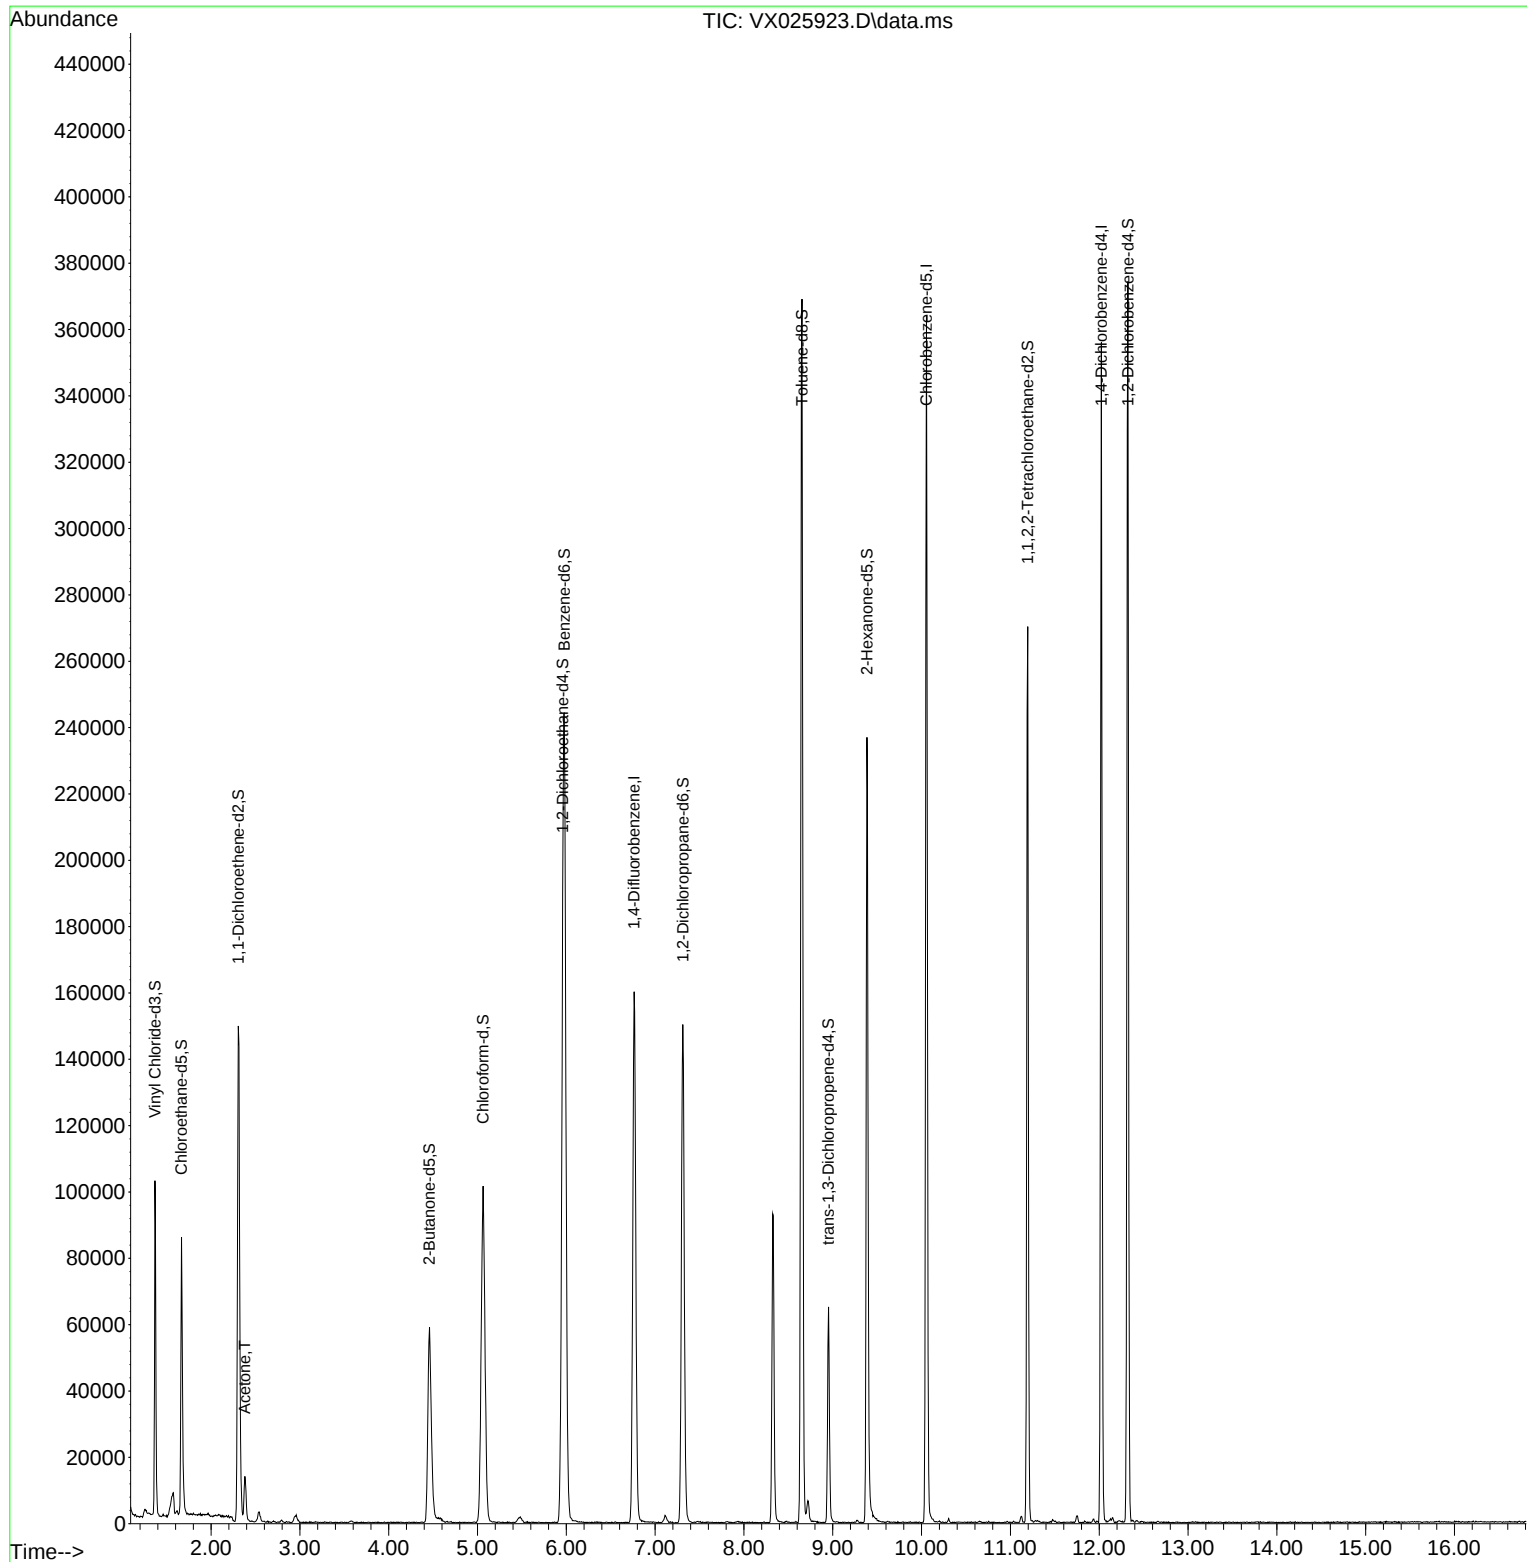

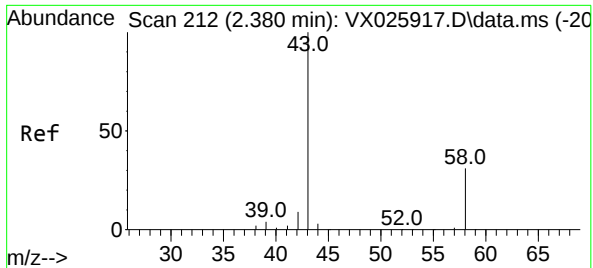

#13
 Acetone
 Concen: 19.161 ug/L
 RT: 2.379 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VX025923.D
 Acq: 20 Dec 2021 18:51

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW1

Tgt Ion: 43 Resp: 14198
 Ion Ratio Lower Upper
 43 100
 58 30.6 0.0 65.6

