

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX122021\  
 Data File : VX025924.D  
 Acq On : 20 Dec 2021 19:15  
 Operator : JC/MD  
 Sample : M5150-04  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 GBBW2

Quant Time: Dec 21 02:03:58 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXML122021WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Tue Dec 21 01:32:07 2021  
 Response via : Initial Calibration


| Compound                      | R.T.    | QIon  | Response | Conc     | Units  | Dev(Min) |
|-------------------------------|---------|-------|----------|----------|--------|----------|
| -----                         |         |       |          |          |        |          |
| Internal Standards            |         |       |          |          |        |          |
| 1) 1,4-Difluorobenzene        | 6.763   | 114   | 155637   | 50.000   | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 10.055  | 117   | 151581   | 50.000   | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 12.024  | 152   | 65028    | 50.000   | ug/L   | 0.00     |
|                               |         |       |          |          |        |          |
| System Monitoring Compounds   |         |       |          |          |        |          |
| 4) Vinyl Chloride-d3          | 1.368   | 65    | 61491    | 49.006   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 60 - 135 | Recovery | =      | 98.020%  |
| 7) Chloroethane-d5            | 1.666   | 69    | 53726    | 51.275   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 70 - 130 | Recovery | =      | 102.560% |
| 11) 1,1-Dichloroethene-d2     | 2.306   | 63    | 85760    | 39.351   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 60 - 125 | Recovery | =      | 78.700%  |
| 21) 2-Butanone-d5             | 4.458   | 46    | 99753    | 110.201  | ug/L   | 0.00     |
| Spiked Amount                 | 100.000 | Range | 40 - 130 | Recovery | =      | 110.200% |
| 24) Chloroform-d              | 5.062   | 84    | 120139   | 49.948   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 70 - 125 | Recovery | =      | 99.900%  |
| 26) 1,2-Dichloroethane-d4     | 5.958   | 65    | 81353    | 51.859   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 70 - 125 | Recovery | =      | 103.720% |
| 32) Benzene-d6                | 5.976   | 84    | 240648   | 52.401   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 70 - 125 | Recovery | =      | 104.800% |
| 36) 1,2-Dichloropropane-d6    | 7.312   | 67    | 72219    | 51.631   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 70 - 120 | Recovery | =      | 103.260% |
| 41) Toluene-d8                | 8.653   | 98    | 219583   | 50.358   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 80 - 120 | Recovery | =      | 100.720% |
| 43) trans-1,3-Dichloroprop... | 8.952   | 79    | 27702    | 44.856   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 60 - 125 | Recovery | =      | 89.720%  |
| 47) 2-Hexanone-d5             | 9.384   | 63    | 67717    | 107.698  | ug/L   | 0.00     |
| Spiked Amount                 | 100.000 | Range | 45 - 130 | Recovery | =      | 107.700% |
| 56) 1,1,2,2-Tetrachloroeth... | 11.195  | 84    | 100910   | 50.925   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 65 - 120 | Recovery | =      | 101.860% |
| 66) 1,2-Dichlorobenzene-d4    | 12.323  | 152   | 71984    | 52.517   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000  | Range | 80 - 120 | Recovery | =      | 105.040% |
|                               |         |       |          |          |        |          |
| Target Compounds              |         |       |          |          | Qvalue |          |
| 13) Acetone                   | 2.380   | 43    | 9783     | 13.509   | ug/L   | 90       |
| -----                         |         |       |          |          |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX122021\  
Data File : VX025924.D  
Acq On : 20 Dec 2021 19:15  
Operator : JC/MD  
Sample : M5150-04  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
GBBW2

Quant Time: Dec 21 02:03:58 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXLM122021WMA.M  
Quant Title : VOC Analysis  
QLast Update : Tue Dec 21 01:32:07 2021  
Response via : Initial Calibration

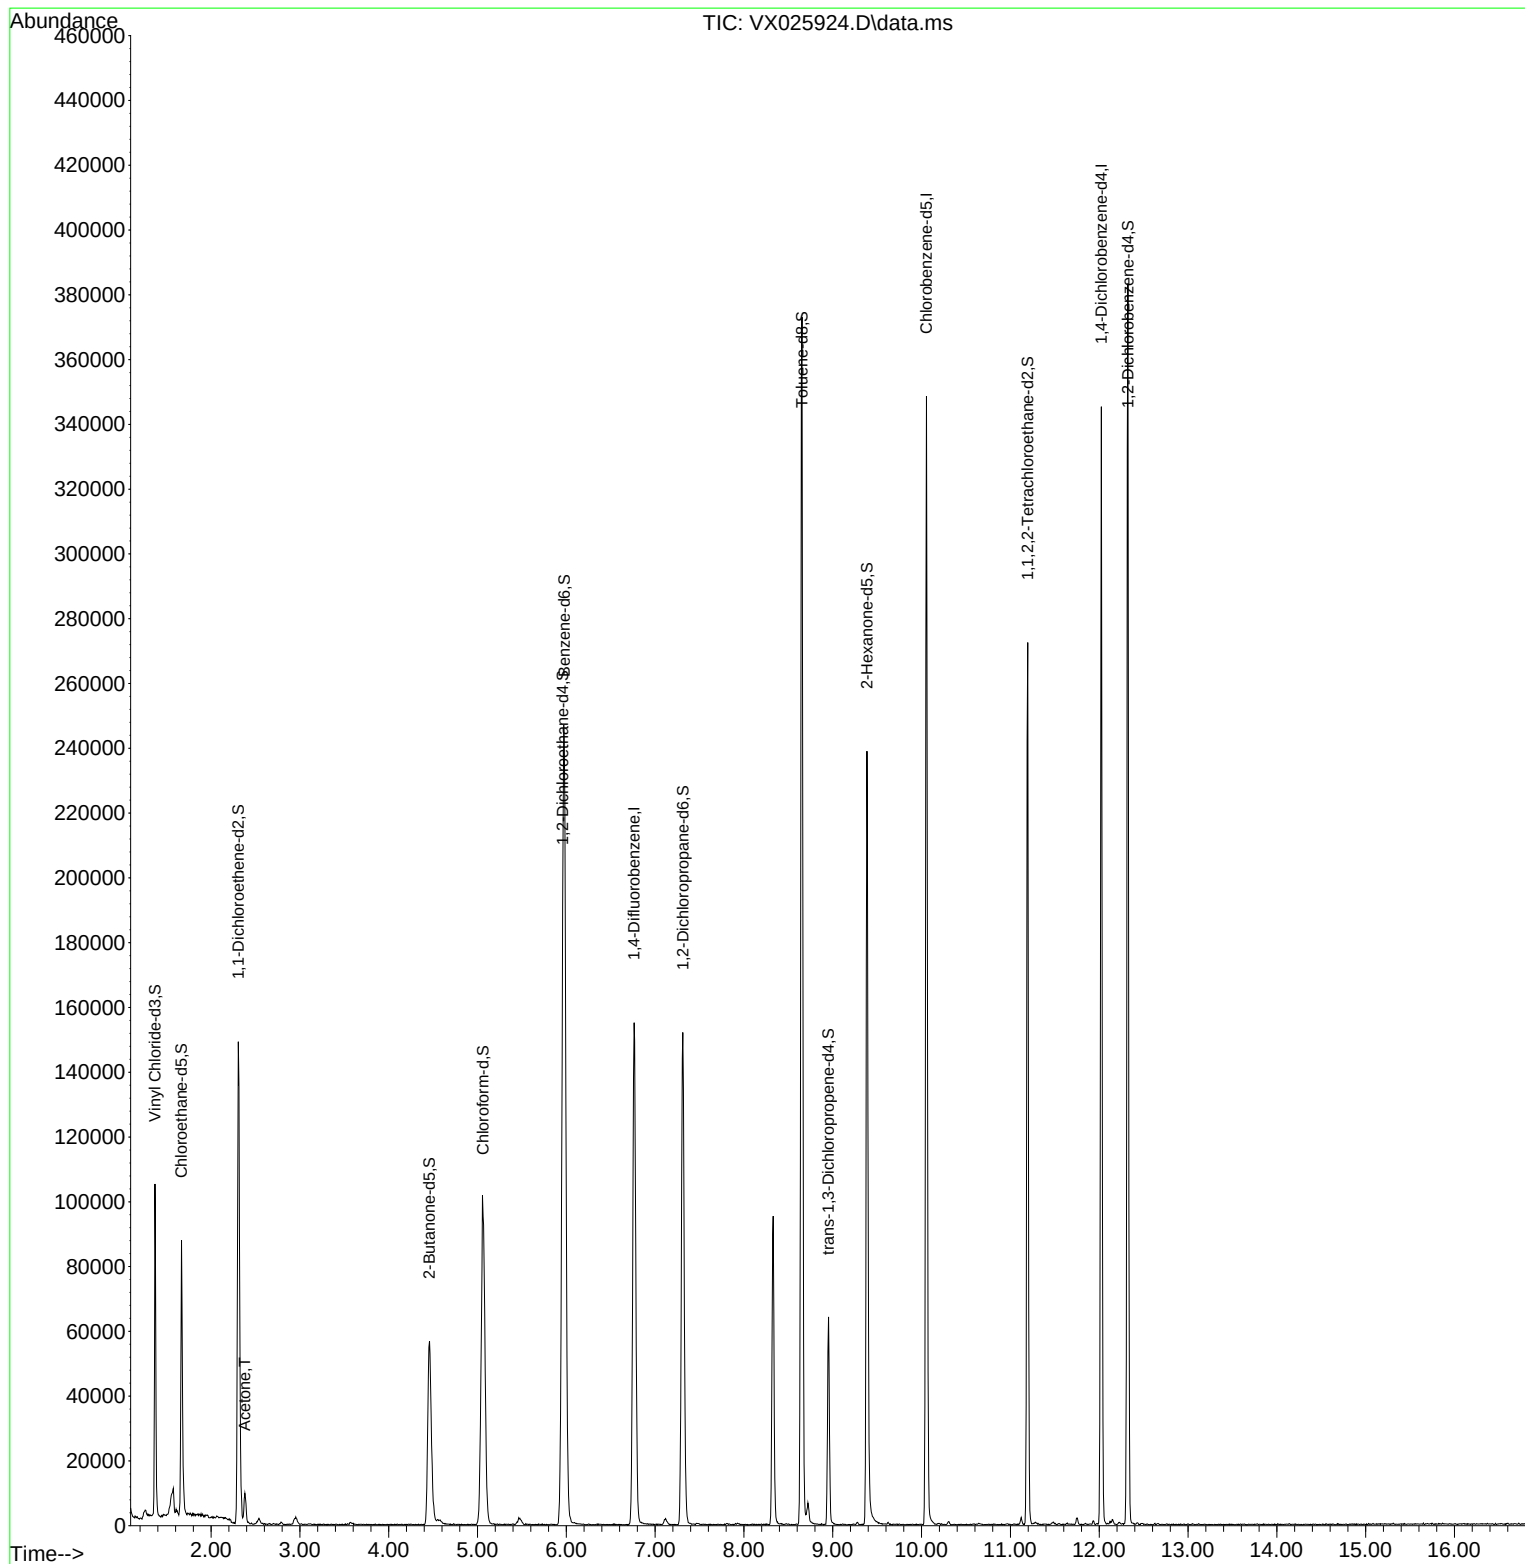

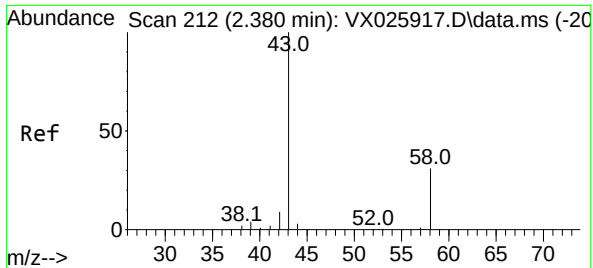

#13  
 Acetone  
 Concen: 13.509 ug/L  
 RT: 2.380 min Scan# 21  
 Delta R.T. -0.000 min  
 Lab File: VX025924.D  
 Acq: 20 Dec 2021 19:15

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 GBBW2

Tgt Ion: 43 Resp: 9783  
 Ion Ratio Lower Upper  
 43 100  
 58 27.0 0.0 65.6

