

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025926.D
 Acq On : 20 Dec 2021 20:01
 Operator : JC/MD
 Sample : M5150-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW4

Quant Time: Dec 21 02:04:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 21 01:32:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	163971	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	161372	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	69476	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	60361	45.661	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	91.320%		
7) Chloroethane-d5	1.666	69	52981	47.994	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	95.980%		
11) 1,1-Dichloroethene-d2	2.307	63	85228	37.119	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.240%		
21) 2-Butanone-d5	4.453	46	96593	101.286	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	101.290%		
24) Chloroform-d	5.062	84	118354	46.705	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.420%		
26) 1,2-Dichloroethane-d4	5.958	65	80817	48.899	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.800%		
32) Benzene-d6	5.977	84	233182	47.695	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.380%		
36) 1,2-Dichloropropane-d6	7.312	67	71411	47.956	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.920%		
41) Toluene-d8	8.653	98	213294	45.947	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.900%		
43) trans-1,3-Dichloroprop...	8.952	79	26748	40.683	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	81.360%		
47) 2-Hexanone-d5	9.385	63	65233	97.453	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	97.450%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	98714	46.794	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	93.580%		
66) 1,2-Dichlorobenzene-d4	12.323	152	71633	48.915	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.820%		
Target Compounds					Qvalue	
13) Acetone	2.386	43	6184	8.105	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025926.D
Acq On : 20 Dec 2021 20:01
Operator : JC/MD
Sample : M5150-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBW4

Quant Time: Dec 21 02:04:21 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 21 01:32:07 2021
Response via : Initial Calibration

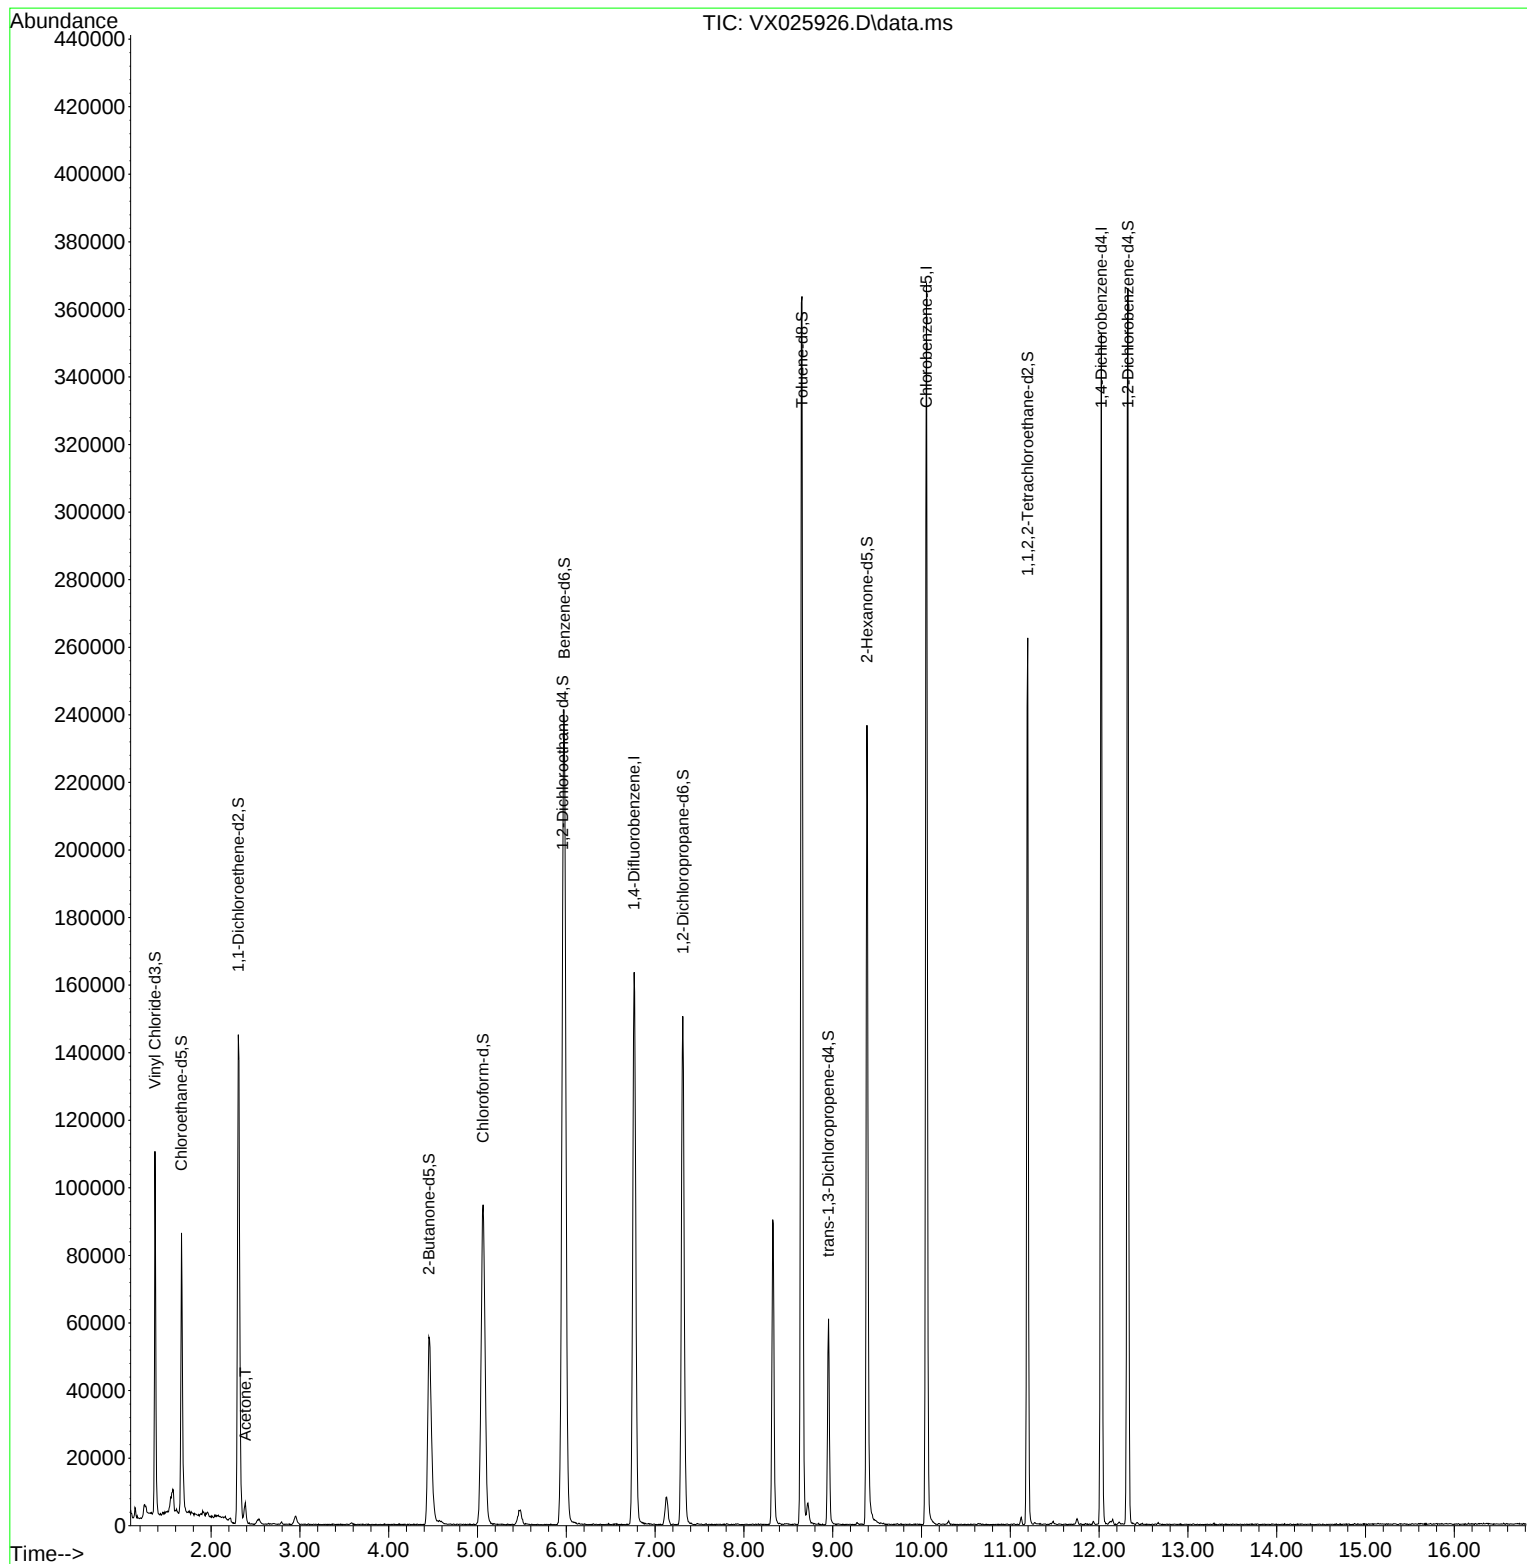

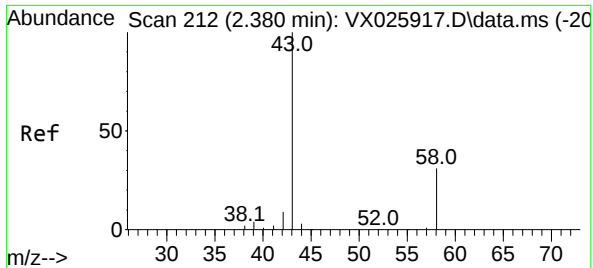

#13
 Acetone
 Concen: 8.105 ug/L
 RT: 2.386 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VX025926.D
 Acq: 20 Dec 2021 20:01

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW4

Tgt Ion: 43 Resp: 6184
 Ion Ratio Lower Upper
 43 100
 58 31.3 0.0 65.6

