

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025927.D
 Acq On : 20 Dec 2021 20:25
 Operator : JC/MD
 Sample : M5150-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW5

Quant Time: Dec 21 02:04:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 21 01:32:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	164480	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	160398	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	68268	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	60928	45.947	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	91.900%
7) Chloroethane-d5	1.666	69	54298	49.035	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	98.080%
11) 1,1-Dichloroethene-d2	2.306	63	85003	36.907	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.820%
21) 2-Butanone-d5	4.458	46	97182	101.589	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.590%
24) Chloroform-d	5.062	84	119672	47.079	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.160%
26) 1,2-Dichloroethane-d4	5.958	65	81571	49.202	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.400%
32) Benzene-d6	5.976	84	238407	49.060	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.120%
36) 1,2-Dichloropropane-d6	7.311	67	72396	48.913	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.820%
41) Toluene-d8	8.653	98	218265	47.304	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.600%
43) trans-1,3-Dichloroprop...	8.951	79	27233	41.672	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.340%
47) 2-Hexanone-d5	9.384	63	67172	100.959	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	100.960%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	100616	47.986	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.980%
66) 1,2-Dichlorobenzene-d4	12.323	152	72314	50.254	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.500%
Target Compounds						
					Qvalue	
13) Acetone	2.379	43	8465	11.061	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025927.D
Acq On : 20 Dec 2021 20:25
Operator : JC/MD
Sample : M5150-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBW5

Quant Time: Dec 21 02:04:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 21 01:32:07 2021
Response via : Initial Calibration

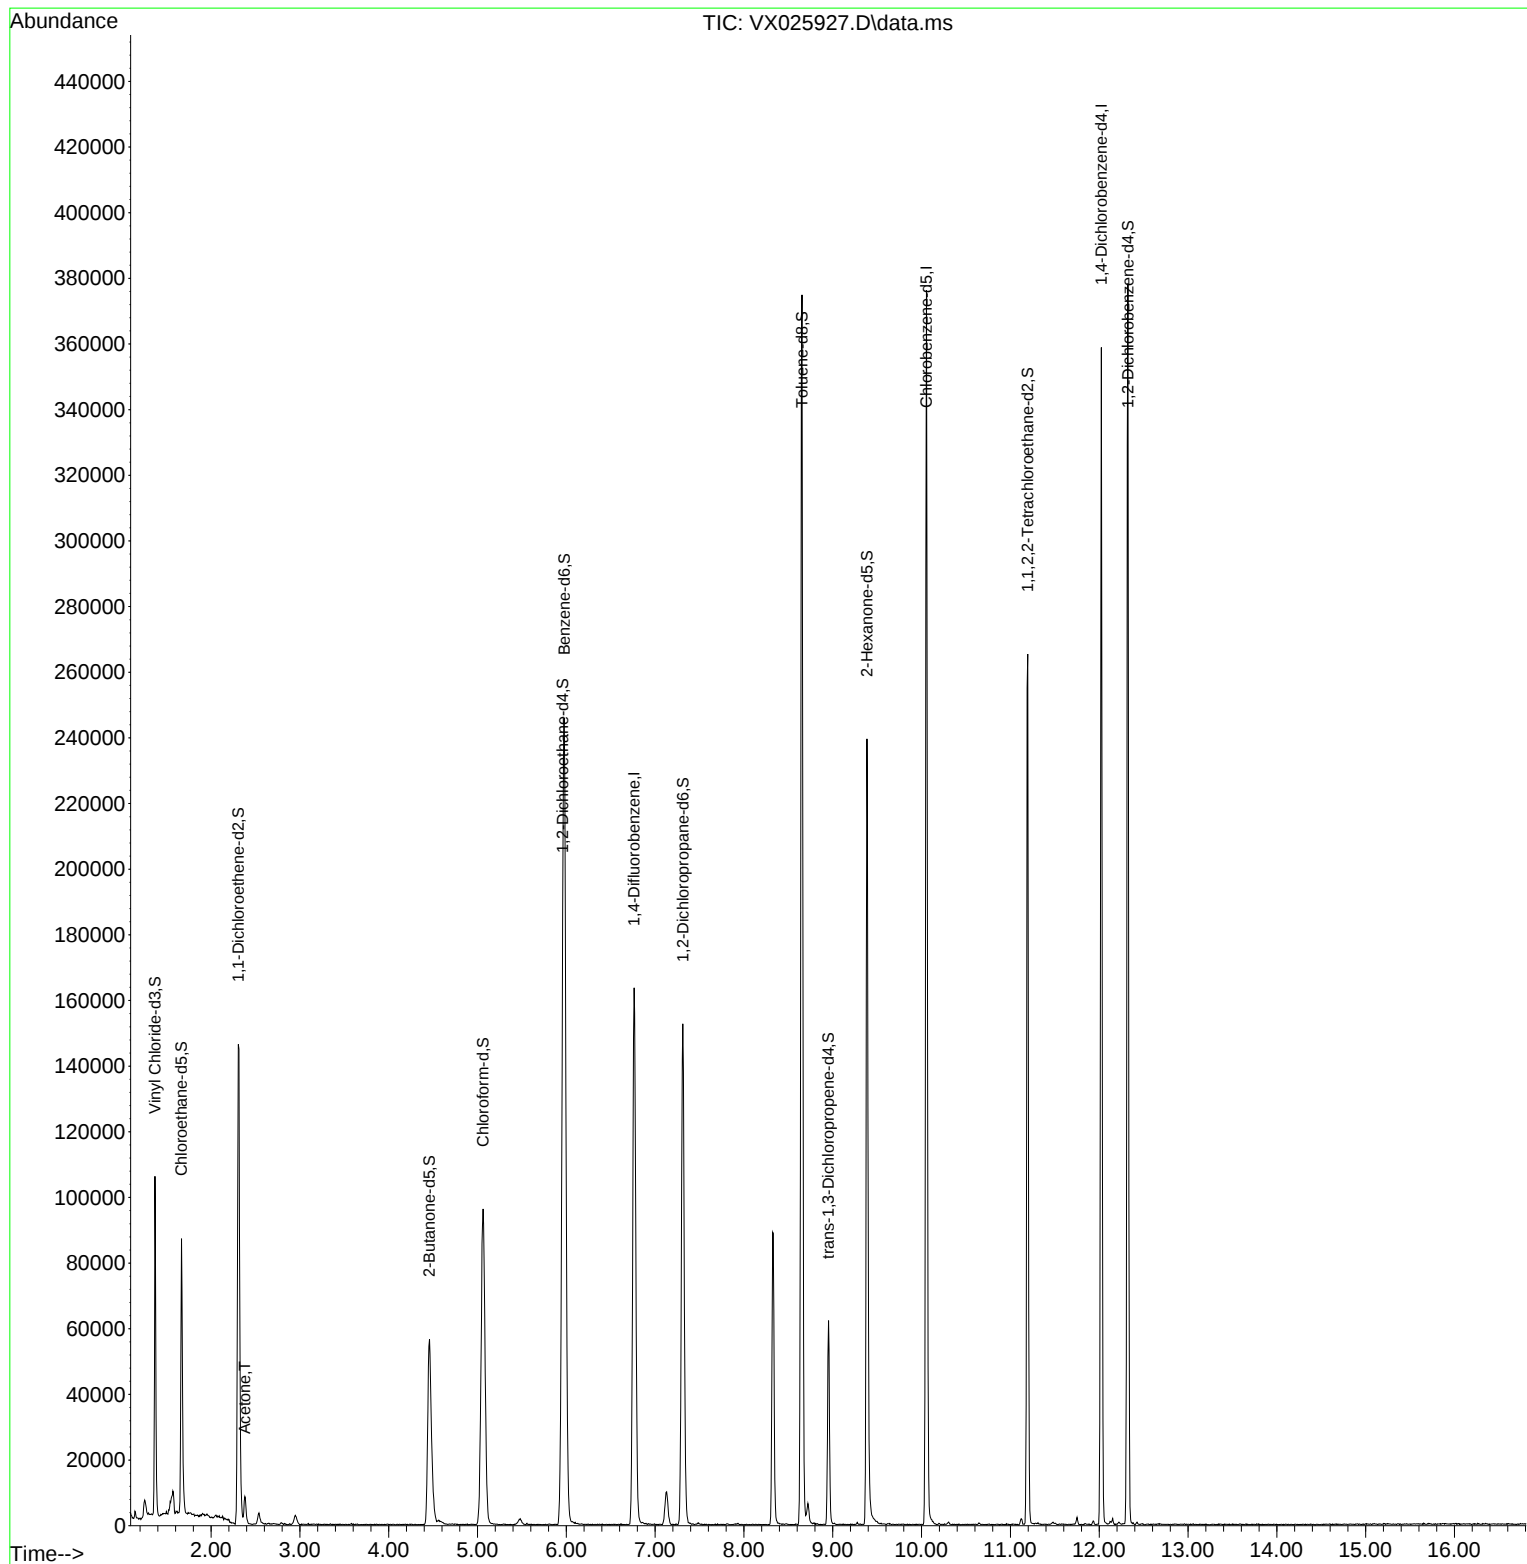

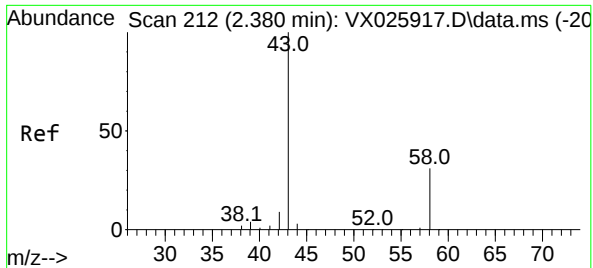

#13
 Acetone
 Concen: 11.061 ug/L
 RT: 2.379 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VX025927.D
 Acq: 20 Dec 2021 20:25

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW5

Tgt Ion: 43 Resp: 8465
 Ion Ratio Lower Upper
 43 100
 58 29.5 0.0 65.6

