

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025918.D
 Acq On : 20 Dec 2021 16:39
 Operator : JC/MD
 Sample : VX1220WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK654

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025918.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	54	rVB	113927	113269	14.47%	2.019%
2	1.666	91	95	105	rVB	86568	112061	14.32%	1.998%
3	2.306	194	200	213	rVB	165123	265689	33.95%	4.736%
4	2.514	231	234	240	rVB2	1484	2078	0.27%	0.037%
5	2.593	245	247	248	rBV	392	278	0.04%	0.005%
6	2.629	251	253	256	rBV2	289	314	0.04%	0.006%
7	2.788	275	279	285	rVB3	2322	4134	0.53%	0.074%
8	2.928	300	302	305	rBV2	391	483	0.06%	0.009%
9	2.989	310	312	313	rBV2	268	257	0.03%	0.005%
10	3.038	317	320	323	rBV2	318	445	0.06%	0.008%
11	3.257	355	356	358	rBV2	225	220	0.03%	0.004%
12	4.001	475	478	480	rBV2	189	193	0.02%	0.003%
13	4.123	496	498	502	rVB2	186	212	0.03%	0.004%
14	4.208	510	512	514	rBV	240	208	0.03%	0.004%
15	4.300	525	527	530	rBV2	256	375	0.05%	0.007%
16	4.391	540	542	543	rBV2	229	226	0.03%	0.004%
17	4.452	543	552	570	rVV	60383	173297	22.15%	3.089%
18	4.696	590	592	595	rVB3	322	324	0.04%	0.006%
19	4.757	600	602	605	rVV2	234	248	0.03%	0.004%
20	4.818	609	612	616	rVB2	281	360	0.05%	0.006%
21	4.849	616	617	619	rBV	271	241	0.03%	0.004%
22	4.970	634	637	638	rBV	181	219	0.03%	0.004%
23	5.056	638	651	666	rBV2	99622	315063	40.26%	5.616%
24	5.324	693	695	699	rVB2	189	209	0.03%	0.004%
25	5.391	702	706	710	rVB3	357	655	0.08%	0.012%
26	5.489	720	722	725	rVB2	250	255	0.03%	0.005%
27	5.867	781	784	785	rBV2	330	216	0.03%	0.004%
28	5.970	788	801	820	rBV2	260016	782523	100.00%	13.949%
29	6.245	842	846	853	rBV2	296	555	0.07%	0.010%
30	6.306	853	856	858	rVB	333	312	0.04%	0.006%
31	6.342	858	862	863	rBV2	290	404	0.05%	0.007%
32	6.519	889	891	894	rBV	195	229	0.03%	0.004%
33	6.763	920	931	946	rBV	154507	372758	47.64%	6.645%
34	6.970	964	965	967	rBV	359	253	0.03%	0.005%
35	6.994	967	969	971	rVV2	285	213	0.03%	0.004%
36	7.110	980	988	997	rBV8	3293	8238	1.05%	0.147%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025918.D
 Acq On : 20 Dec 2021 16:39
 Operator : JC/MD
 Sample : VX1220WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK654

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

37	7.312	1012	1021	1035	rBV	159745	349509	44.66%	6.230%
38	7.805	1099	1102	1103	rBV	366	351	0.04%	0.006%
39	7.933	1121	1123	1126	rBV2	350	290	0.04%	0.005%
40	8.244	1170	1174	1181	rVB4	3435	5589	0.71%	0.100%
41	8.324	1181	1187	1200	rBV	104920	173134	22.13%	3.086%
42	8.476	1209	1212	1214	rBV2	332	400	0.05%	0.007%
43	8.543	1220	1223	1225	rVB2	252	239	0.03%	0.004%
44	8.580	1225	1229	1233	rBV2	429	616	0.08%	0.011%
45	8.647	1233	1240	1248	rBV	391188	630675	80.60%	11.243%
46	8.860	1271	1275	1277	rBV2	278	337	0.04%	0.006%
47	8.951	1282	1290	1298	rBV	70762	103682	13.25%	1.848%
48	9.275	1340	1343	1347	rVB2	594	599	0.08%	0.011%
49	9.384	1355	1361	1381	rBV	261318	377657	48.26%	6.732%
50	9.701	1412	1413	1418	rVB2	316	337	0.04%	0.006%
51	10.055	1465	1471	1488	rBV	347952	464528	59.36%	8.281%
52	10.201	1491	1495	1500	rVV4	642	896	0.11%	0.016%
53	10.299	1508	1511	1516	rVV2	1293	1701	0.22%	0.030%
54	10.476	1536	1540	1543	rBV2	217	320	0.04%	0.006%
55	10.652	1564	1569	1574	rVV4	845	1280	0.16%	0.023%
56	10.963	1617	1620	1624	rVV	706	927	0.12%	0.017%
57	11.018	1627	1629	1632	rBV	275	250	0.03%	0.004%
58	11.122	1642	1646	1652	rBV3	2907	3598	0.46%	0.064%
59	11.195	1652	1658	1667	rVV	272035	361168	46.15%	6.438%
60	11.280	1669	1672	1673	rVV2	738	717	0.09%	0.013%
61	11.299	1673	1675	1678	rVV4	657	819	0.10%	0.015%
62	11.451	1697	1700	1701	rBV2	621	576	0.07%	0.010%
63	11.555	1715	1717	1718	rVB	328	223	0.03%	0.004%
64	11.628	1727	1729	1733	rVB2	315	397	0.05%	0.007%
65	11.683	1734	1738	1741	rVV2	437	616	0.08%	0.011%
66	11.713	1741	1743	1745	rVV2	567	606	0.08%	0.011%
67	11.750	1745	1749	1755	rVB3	3097	3984	0.51%	0.071%
68	11.841	1758	1764	1767	rBV3	400	896	0.11%	0.016%
69	11.933	1775	1779	1782	rBV3	1441	1735	0.22%	0.031%
70	11.975	1782	1786	1789	rVB4	1028	1400	0.18%	0.025%
71	12.024	1789	1794	1804	rBV	329247	427422	54.62%	7.619%
72	12.122	1806	1810	1812	rVV3	1106	1643	0.21%	0.029%
73	12.152	1812	1815	1819	rVB2	2083	2407	0.31%	0.043%
74	12.323	1835	1843	1853	rBV	397032	518512	66.26%	9.243%
75	12.433	1857	1861	1867	rVB3	484	779	0.10%	0.014%
76	12.481	1867	1869	1876	rVB2	366	582	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025918.D
 Acq On : 20 Dec 2021 16:39
 Operator : JC/MD
 Sample : VX1220WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK654

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

77	12.548	1876	1880	1883	rBV2	314	418	0.05%	0.007%
78	12.823	1923	1925	1929	rVB2	181	239	0.03%	0.004%
79	12.859	1929	1931	1934	rVB2	344	348	0.04%	0.006%
80	13.115	1970	1973	1978	rBV3	892	1144	0.15%	0.020%
81	13.225	1988	1991	1992	rBV2	286	350	0.04%	0.006%
82	13.554	2043	2045	2048	rVB2	427	344	0.04%	0.006%
83	13.591	2048	2051	2056	rVB3	1065	1132	0.14%	0.020%
84	13.774	2079	2081	2086	rBV3	893	1317	0.17%	0.023%
85	13.884	2097	2099	2100	rBV	284	200	0.03%	0.004%
86	13.963	2106	2112	2116	rBV2	1199	1364	0.17%	0.024%
87	14.377	2176	2180	2185	rBV2	203	473	0.06%	0.008%
88	14.627	2218	2221	2222	rBV2	217	196	0.03%	0.003%
89	14.816	2250	2252	2255	rVB2	288	220	0.03%	0.004%
90	14.877	2258	2262	2263	rBV	344	461	0.06%	0.008%
91	14.902	2263	2266	2268	rBV	330	316	0.04%	0.006%
92	15.103	2295	2299	2303	rBV3	310	531	0.07%	0.009%
93	15.170	2308	2310	2313	rBV3	249	236	0.03%	0.004%
94	15.414	2348	2350	2352	rBV2	387	454	0.06%	0.008%
95	15.621	2382	2384	2385	rBV	317	213	0.03%	0.004%
96	15.725	2399	2401	2404	rBV2	366	366	0.05%	0.007%
97	15.908	2430	2431	2433	rBV	232	213	0.03%	0.004%
98	16.194	2476	2478	2481	rBV2	300	286	0.04%	0.005%
99	16.340	2499	2502	2504	rBV2	251	224	0.03%	0.004%
100	16.548	2535	2536	2539	rVB2	354	233	0.03%	0.004%




Sum of corrected areas: 5609689

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025918.D
Acq On : 20 Dec 2021 16:39
Operator : JC/MD
Sample : VX1220WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK654

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

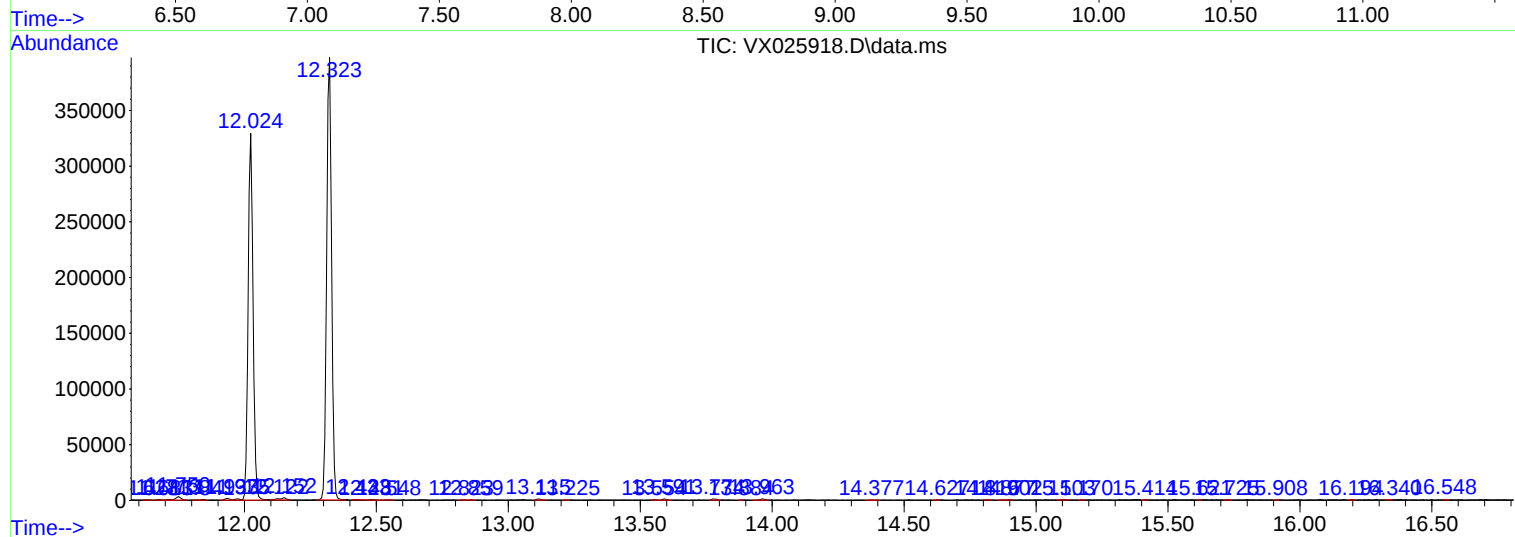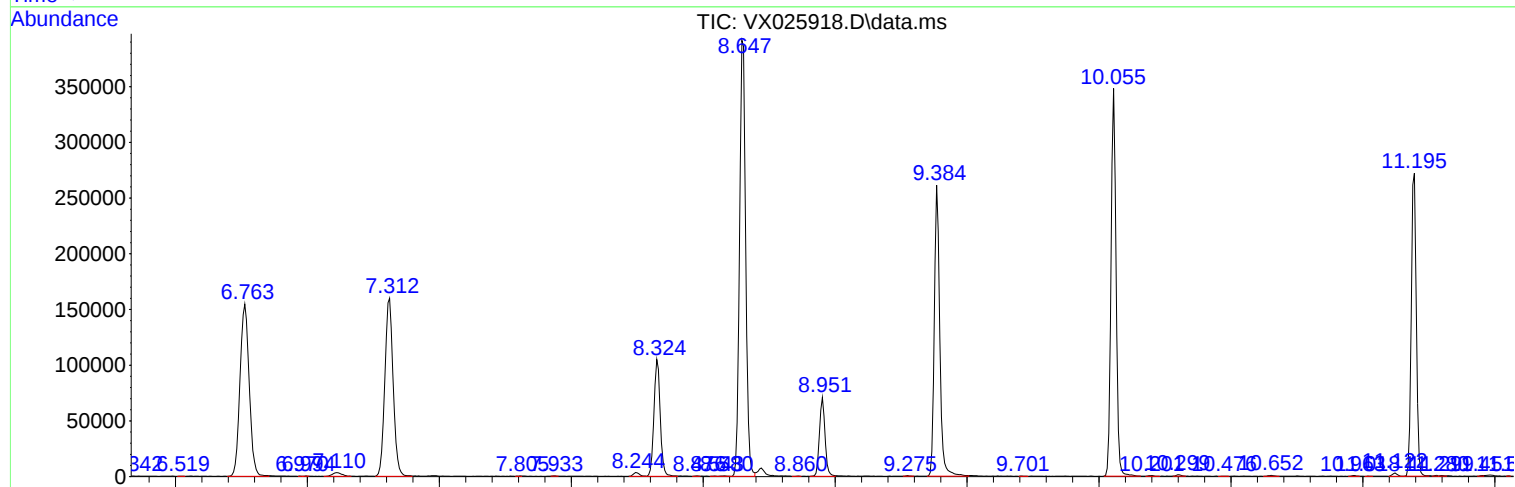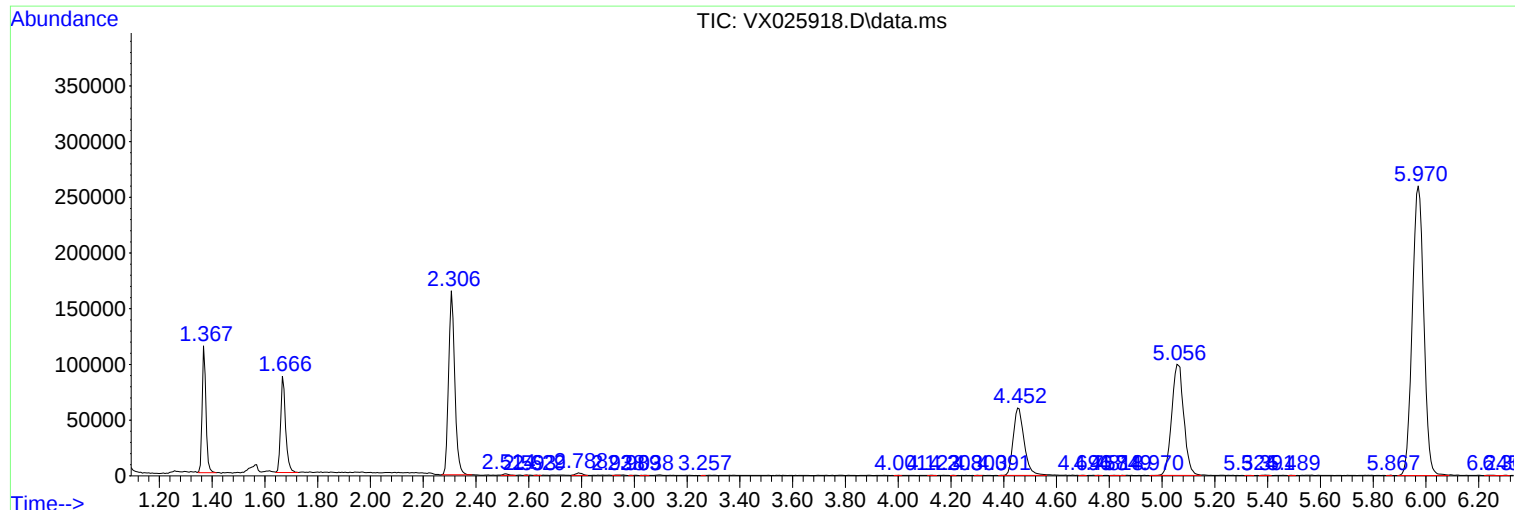

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025918.D
Acq On : 20 Dec 2021 16:39
Operator : JC/MD
Sample : VX1220WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK654

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025918.D
Acq On : 20 Dec 2021 16:39
Operator : JC/MD
Sample : VX1220WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK654

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc