

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025921.D
 Acq On : 20 Dec 2021 18:05
 Operator : JC/MD
 Sample : M5150-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBT9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025921.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	54	rVB	116909	111839	14.41%	1.969%
2	1.666	91	95	106	rVB	87293	111017	14.30%	1.955%
3	2.306	194	200	210	rBV	161622	262772	33.85%	4.626%
4	2.508	229	233	235	rBV3	757	1027	0.13%	0.018%
5	2.587	243	246	248	rBV2	421	523	0.07%	0.009%
6	2.703	263	265	267	rBV2	414	321	0.04%	0.006%
7	2.788	275	279	286	rVB4	548	1106	0.14%	0.019%
8	2.940	299	304	314	rVB2	2577	6919	0.89%	0.122%
9	3.014	314	316	318	rVB	307	213	0.03%	0.004%
10	3.239	351	353	355	rVV2	245	263	0.03%	0.005%
11	3.288	358	361	362	rVB2	269	242	0.03%	0.004%
12	3.312	362	365	367	rBV	224	240	0.03%	0.004%
13	3.373	372	375	377	rBV2	310	346	0.04%	0.006%
14	3.477	390	392	395	rVB2	301	290	0.04%	0.005%
15	4.062	485	488	490	rVB	234	276	0.04%	0.005%
16	4.178	504	507	511	rBV2	187	295	0.04%	0.005%
17	4.452	543	552	567	rBV	57866	162296	20.90%	2.857%
18	4.849	615	617	621	rVB2	247	229	0.03%	0.004%
19	5.062	638	652	667	rBV	105064	315375	40.62%	5.552%
20	5.470	713	719	725	rVB4	767	1944	0.25%	0.034%
21	5.562	730	734	735	rBV2	294	353	0.05%	0.006%
22	5.702	753	757	760	rBV2	180	313	0.04%	0.006%
23	5.787	768	771	774	rVB	141	194	0.02%	0.003%
24	5.970	788	801	819	rVV2	259643	776364	100.00%	13.668%
25	6.239	844	845	847	rBV	403	303	0.04%	0.005%
26	6.306	854	856	857	rVB2	305	220	0.03%	0.004%
27	6.458	879	881	883	rVB2	266	228	0.03%	0.004%
28	6.763	921	931	945	rBV	168387	402578	51.85%	7.088%
29	6.970	963	965	967	rBV	206	229	0.03%	0.004%
30	7.001	967	970	971	rVB	296	271	0.03%	0.005%
31	7.110	981	988	998	rVB4	3488	8529	1.10%	0.150%
32	7.305	1011	1020	1035	rBV	158099	349884	45.07%	6.160%
33	7.470	1043	1047	1054	rVB2	465	1042	0.13%	0.018%
34	7.622	1069	1072	1076	rBV2	239	359	0.05%	0.006%
35	7.818	1100	1104	1105	rVV2	369	354	0.05%	0.006%
36	7.909	1113	1119	1121	rBV2	356	499	0.06%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025921.D
 Acq On : 20 Dec 2021 18:05
 Operator : JC/MD
 Sample : M5150-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBT9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

37	7.933	1121	1123	1127	rVV3	331	489	0.06%	0.009%
38	8.129	1151	1155	1156	rVB	222	296	0.04%	0.005%
39	8.324	1181	1187	1195	rBV	102513	166482	21.44%	2.931%
40	8.488	1212	1214	1217	rVB3	365	267	0.03%	0.005%
41	8.567	1225	1227	1233	rBV3	384	509	0.07%	0.009%
42	8.647	1233	1240	1248	rBV	398026	629715	81.11%	11.087%
43	8.714	1249	1251	1259	rVB	6487	10328	1.33%	0.182%
44	8.952	1284	1290	1304	rVB	68261	102575	13.21%	1.806%
45	9.171	1324	1326	1328	rVV2	204	214	0.03%	0.004%
46	9.226	1332	1335	1340	rVV2	247	356	0.05%	0.006%
47	9.281	1340	1344	1349	rVB3	918	1307	0.17%	0.023%
48	9.384	1356	1361	1381	rBV	250423	359299	46.28%	6.326%
49	9.781	1424	1426	1428	rVV2	297	255	0.03%	0.004%
50	9.872	1439	1441	1444	rBV2	160	200	0.03%	0.004%
51	10.055	1465	1471	1487	rBV	375798	513310	66.12%	9.037%
52	10.201	1491	1495	1497	rVB2	483	617	0.08%	0.011%
53	10.305	1508	1512	1516	rVV3	1270	1566	0.20%	0.028%
54	10.640	1564	1567	1569	rBV3	459	582	0.07%	0.010%
55	10.866	1601	1604	1606	rBV3	241	300	0.04%	0.005%
56	10.963	1617	1620	1623	rBV2	353	394	0.05%	0.007%
57	11.116	1642	1645	1652	rVB	2242	2931	0.38%	0.052%
58	11.195	1652	1658	1666	rBV	272816	357718	46.08%	6.298%
59	11.451	1698	1700	1702	rBV2	391	464	0.06%	0.008%
60	11.475	1702	1704	1707	rVV	752	727	0.09%	0.013%
61	11.683	1735	1738	1741	rBV2	455	431	0.06%	0.008%
62	11.750	1745	1749	1753	rVB4	2180	3255	0.42%	0.057%
63	11.841	1761	1764	1767	rBV3	485	542	0.07%	0.010%
64	11.933	1776	1779	1782	rVV2	1115	1512	0.19%	0.027%
65	11.975	1782	1786	1788	rVV	506	639	0.08%	0.011%
66	12.024	1788	1794	1803	rVV	370621	471167	60.69%	8.295%
67	12.103	1805	1807	1808	rVV	367	283	0.04%	0.005%
68	12.128	1809	1811	1812	rVV	1012	901	0.12%	0.016%
69	12.152	1812	1815	1819	rVB2	1735	2150	0.28%	0.038%
70	12.219	1825	1826	1830	rVB	427	373	0.05%	0.007%
71	12.323	1837	1843	1851	rVB	413401	519621	66.93%	9.148%
72	12.427	1857	1860	1863	rVB3	751	651	0.08%	0.011%
73	12.658	1896	1898	1901	rBV2	256	290	0.04%	0.005%
74	12.750	1910	1913	1917	rVB3	223	313	0.04%	0.006%
75	12.817	1922	1924	1927	rVB2	202	258	0.03%	0.005%
76	12.847	1927	1929	1933	rVB2	341	447	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025921.D
 Acq On : 20 Dec 2021 18:05
 Operator : JC/MD
 Sample : M5150-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBT9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

77	13.115	1969	1973	1976	rBV3	261	426	0.05%	0.007%
78	13.237	1989	1993	1994	rBV	299	252	0.03%	0.004%
79	13.335	2007	2009	2012	rBV	347	376	0.05%	0.007%
80	13.414	2020	2022	2025	rVV	279	264	0.03%	0.005%
81	13.506	2036	2037	2041	rBV2	163	201	0.03%	0.004%
82	13.591	2048	2051	2054	rBV3	302	335	0.04%	0.006%
83	14.024	2121	2122	2125	rBV2	207	289	0.04%	0.005%
84	14.170	2145	2146	2152	rBV	293	396	0.05%	0.007%
85	14.310	2165	2169	2172	rBV2	146	208	0.03%	0.004%
86	14.402	2182	2184	2187	rBV	299	199	0.03%	0.004%
87	14.560	2206	2210	2211	rBV2	271	269	0.03%	0.005%
88	14.700	2231	2233	2235	rBV	212	197	0.03%	0.003%
89	14.743	2237	2240	2244	rBV2	286	333	0.04%	0.006%
90	14.829	2252	2254	2257	rBV2	242	250	0.03%	0.004%
91	14.926	2267	2270	2272	rBV3	364	489	0.06%	0.009%
92	15.030	2286	2287	2291	rVV3	195	199	0.03%	0.004%
93	15.304	2329	2332	2333	rBV2	245	205	0.03%	0.004%
94	15.487	2360	2362	2367	rVV3	232	397	0.05%	0.007%
95	15.865	2422	2424	2425	rBV	415	249	0.03%	0.004%
96	16.206	2478	2480	2482	rVB	455	326	0.04%	0.006%
97	16.225	2482	2483	2485	rBV2	282	273	0.04%	0.005%
98	16.267	2488	2490	2492	rBV	378	306	0.04%	0.005%
99	16.432	2515	2517	2519	rBV2	244	216	0.03%	0.004%
100	16.511	2526	2530	2532	rBV2	284	358	0.05%	0.006%




Sum of corrected areas: 5680000

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025921.D
Acq On : 20 Dec 2021 18:05
Operator : JC/MD
Sample : M5150-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBT9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

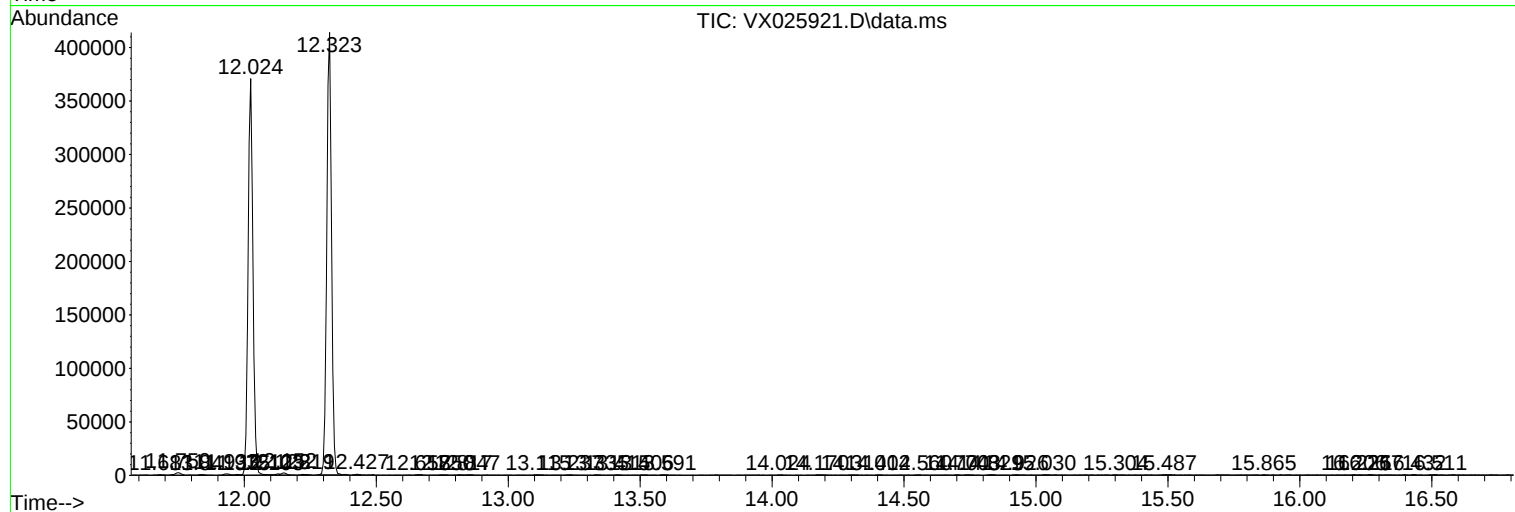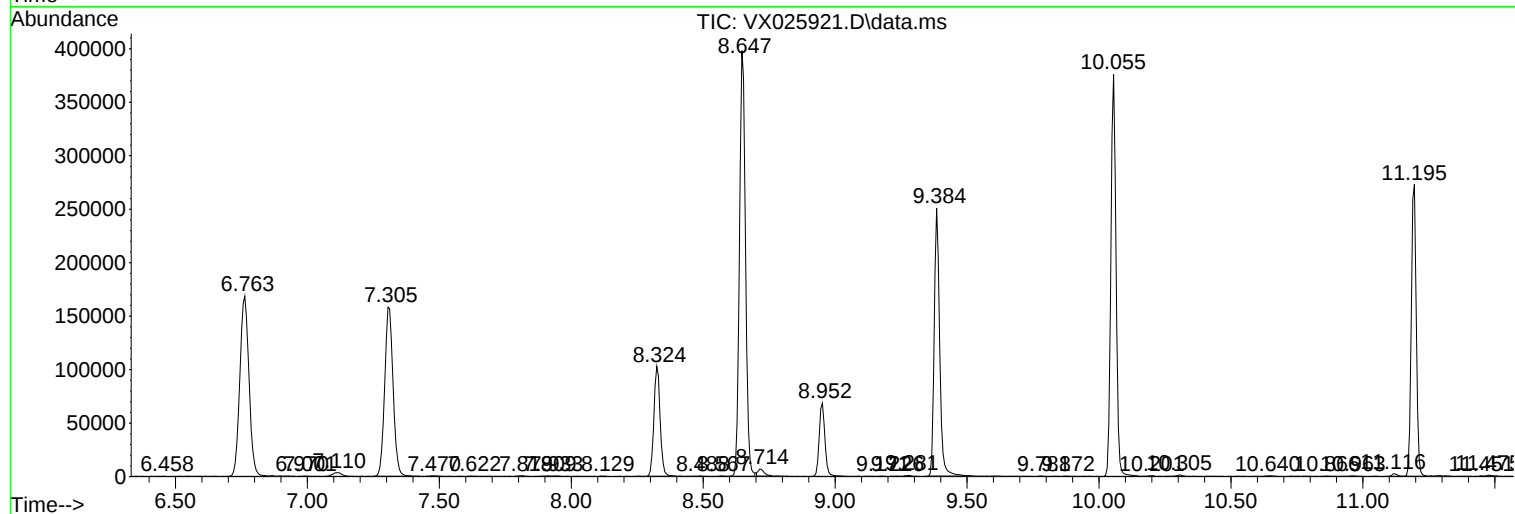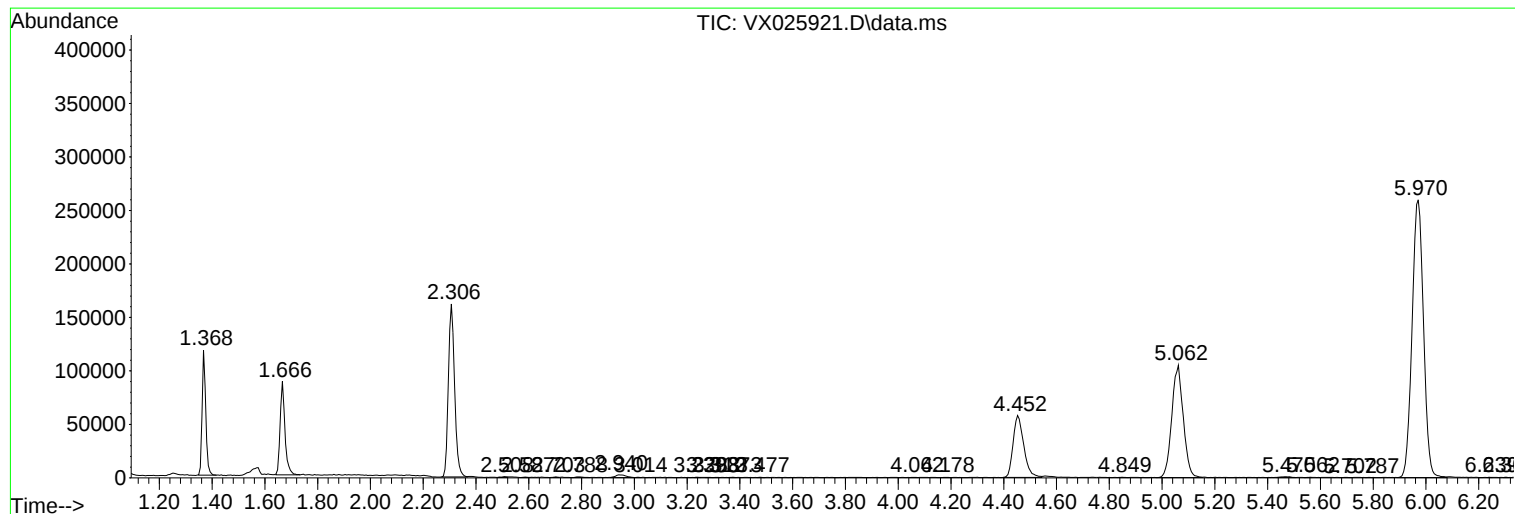

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025921.D
Acq On : 20 Dec 2021 18:05
Operator : JC/MD
Sample : M5150-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBT9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025921.D
Acq On : 20 Dec 2021 18:05
Operator : JC/MD
Sample : M5150-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBT9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc