

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025922.D
 Acq On : 20 Dec 2021 18:28
 Operator : JC/MD
 Sample : M5150-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025922.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	56	rVB	105171	106794	14.37%	1.958%
2	1.666	91	95	105	rVB	84586	109851	14.78%	2.014%
3	2.306	194	200	211	rBV	152386	249559	33.58%	4.574%
4	2.514	230	234	238	rBV4	602	1176	0.16%	0.022%
5	2.794	276	280	283	rVB3	458	665	0.09%	0.012%
6	2.953	298	306	315	rVB4	2404	6491	0.87%	0.119%
7	3.288	358	361	364	rBV2	179	282	0.04%	0.005%
8	3.757	436	438	441	rVB3	286	276	0.04%	0.005%
9	3.812	445	447	451	rBV2	171	263	0.04%	0.005%
10	4.044	483	485	487	rBV3	270	291	0.04%	0.005%
11	4.245	516	518	522	rVB2	363	401	0.05%	0.007%
12	4.452	543	552	570	rBV	56837	164010	22.07%	3.006%
13	4.904	623	626	629	rBV2	322	394	0.05%	0.007%
14	5.056	638	651	667	rBV	100425	304431	40.97%	5.580%
15	5.202	673	675	680	rVB2	313	297	0.04%	0.005%
16	5.281	685	688	689	rBV2	231	243	0.03%	0.004%
17	5.379	701	704	706	rVV2	199	262	0.04%	0.005%
18	5.470	710	719	728	rBV6	2869	9433	1.27%	0.173%
19	5.568	733	735	739	rVB3	480	488	0.07%	0.009%
20	5.970	790	801	817	rVV2	245648	743121	100.00%	13.621%
21	6.397	869	871	875	rVV2	258	342	0.05%	0.006%
22	6.495	886	887	890	rBV2	201	219	0.03%	0.004%
23	6.763	922	931	945	rBV	165922	396281	53.33%	7.264%
24	7.110	982	988	999	rVB6	3614	8322	1.12%	0.153%
25	7.312	1012	1021	1034	rBV	154142	337306	45.39%	6.183%
26	7.458	1041	1045	1046	rBV	288	342	0.05%	0.006%
27	7.482	1046	1049	1053	rVV3	409	568	0.08%	0.010%
28	7.744	1090	1092	1094	rBV2	238	204	0.03%	0.004%
29	7.799	1097	1101	1102	rBV2	355	447	0.06%	0.008%
30	7.903	1114	1118	1121	rBV3	416	635	0.09%	0.012%
31	8.324	1181	1187	1196	rBV	94278	155034	20.86%	2.842%
32	8.476	1209	1212	1213	rBV	180	223	0.03%	0.004%
33	8.653	1234	1241	1248	rBV	374452	597665	80.43%	10.955%
34	8.787	1262	1263	1268	rVB3	500	406	0.05%	0.007%
35	8.952	1284	1290	1297	rBV	66155	94275	12.69%	1.728%
36	9.275	1339	1343	1349	rBV4	1360	1649	0.22%	0.030%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025922.D
 Acq On : 20 Dec 2021 18:28
 Operator : JC/MD
 Sample : M5150-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

37	9.384	1356	1361	1379	rBV	244785	360394	48.50%	6.606%
38	9.738	1418	1419	1421	rVB	306	203	0.03%	0.004%
39	9.756	1421	1422	1424	rBV2	274	226	0.03%	0.004%
40	9.829	1432	1434	1436	rVB	334	257	0.03%	0.005%
41	9.884	1441	1443	1446	rBV3	270	278	0.04%	0.005%
42	10.055	1465	1471	1486	rBV	364337	497512	66.95%	9.119%
43	10.305	1508	1512	1515	rVB3	812	1085	0.15%	0.020%
44	10.396	1525	1527	1530	rBV2	176	207	0.03%	0.004%
45	10.744	1579	1584	1588	rBV3	110	239	0.03%	0.004%
46	10.811	1592	1595	1596	rBV	375	297	0.04%	0.005%
47	10.902	1608	1610	1613	rVB2	234	277	0.04%	0.005%
48	11.043	1630	1633	1638	rVB2	352	401	0.05%	0.007%
49	11.122	1642	1646	1650	rVB	2394	2687	0.36%	0.049%
50	11.195	1652	1658	1667	rBV	273198	346711	46.66%	6.355%
51	11.378	1687	1688	1691	rBV3	217	244	0.03%	0.004%
52	11.457	1694	1701	1702	rBV4	281	482	0.06%	0.009%
53	11.482	1702	1705	1707	rBV3	602	656	0.09%	0.012%
54	11.671	1732	1736	1737	rVV2	261	217	0.03%	0.004%
55	11.750	1745	1749	1754	rVB3	2238	2889	0.39%	0.053%
56	11.847	1761	1765	1769	rVV	437	519	0.07%	0.010%
57	11.933	1776	1779	1783	rVB2	1286	1192	0.16%	0.022%
58	11.969	1783	1785	1789	rBV2	404	464	0.06%	0.009%
59	12.024	1789	1794	1805	rVB	356375	448270	60.32%	8.217%
60	12.152	1812	1815	1818	rVB3	1674	1981	0.27%	0.036%
61	12.219	1823	1826	1829	rVV	362	501	0.07%	0.009%
62	12.323	1835	1843	1853	rBV	372226	482685	64.95%	8.848%
63	12.475	1867	1868	1873	rBV3	470	547	0.07%	0.010%
64	12.658	1896	1898	1902	rVB3	447	479	0.06%	0.009%
65	12.695	1902	1904	1906	rVB2	316	219	0.03%	0.004%
66	12.786	1917	1919	1924	rBV2	214	370	0.05%	0.007%
67	13.061	1960	1964	1965	rBV2	359	430	0.06%	0.008%
68	13.115	1971	1973	1975	rBV	350	322	0.04%	0.006%
69	13.268	1995	1998	1999	rBV2	165	208	0.03%	0.004%
70	13.408	2019	2021	2023	rBV	260	201	0.03%	0.004%
71	13.518	2037	2039	2042	rVB	266	249	0.03%	0.005%
72	13.554	2042	2045	2049	rBV2	254	406	0.05%	0.007%
73	13.591	2049	2051	2054	rVV2	408	388	0.05%	0.007%
74	13.670	2062	2064	2068	rBV	227	318	0.04%	0.006%
75	13.902	2095	2102	2104	rBV2	273	416	0.06%	0.008%
76	14.134	2135	2140	2141	rBV3	248	327	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025922.D
 Acq On : 20 Dec 2021 18:28
 Operator : JC/MD
 Sample : M5150-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

77	14.426	2185	2188	2189	rBV	265	240	0.03%	0.004%
78	14.499	2197	2200	2201	rBV2	264	214	0.03%	0.004%
79	14.670	2226	2228	2233	rVB2	229	233	0.03%	0.004%
80	14.816	2250	2252	2254	rBV2	221	217	0.03%	0.004%
81	14.847	2254	2257	2258	rVB2	307	245	0.03%	0.004%
82	14.871	2258	2261	2263	rBV	242	245	0.03%	0.004%
83	14.896	2263	2265	2267	rBV2	285	241	0.03%	0.004%
84	14.993	2277	2281	2284	rVV3	287	483	0.06%	0.009%
85	15.048	2286	2290	2294	rVB2	193	329	0.04%	0.006%
86	15.115	2296	2301	2306	rBV2	272	577	0.08%	0.011%
87	15.213	2316	2317	2320	rVB	391	201	0.03%	0.004%
88	15.469	2357	2359	2360	rBV	287	254	0.03%	0.005%
89	15.536	2366	2370	2371	rBV2	258	315	0.04%	0.006%
90	15.786	2410	2411	2414	rBV2	267	240	0.03%	0.004%
91	15.847	2419	2421	2427	rVB2	308	366	0.05%	0.007%
92	15.902	2427	2430	2431	rBV2	264	272	0.04%	0.005%
93	16.017	2447	2449	2452	rBV2	231	281	0.04%	0.005%
94	16.097	2460	2462	2466	rBV2	283	350	0.05%	0.006%
95	16.212	2479	2481	2482	rVB2	343	202	0.03%	0.004%
96	16.231	2482	2484	2486	rBV2	258	309	0.04%	0.006%
97	16.420	2512	2515	2516	rBV2	365	409	0.06%	0.007%
98	16.536	2531	2534	2536	rVB2	378	404	0.05%	0.007%
99	16.584	2540	2542	2543	rBV	277	247	0.03%	0.005%
100	16.725	2562	2565	2567	rVB2	292	267	0.04%	0.005%




Sum of corrected areas: 5455541

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025922.D
Acq On : 20 Dec 2021 18:28
Operator : JC/MD
Sample : M5150-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

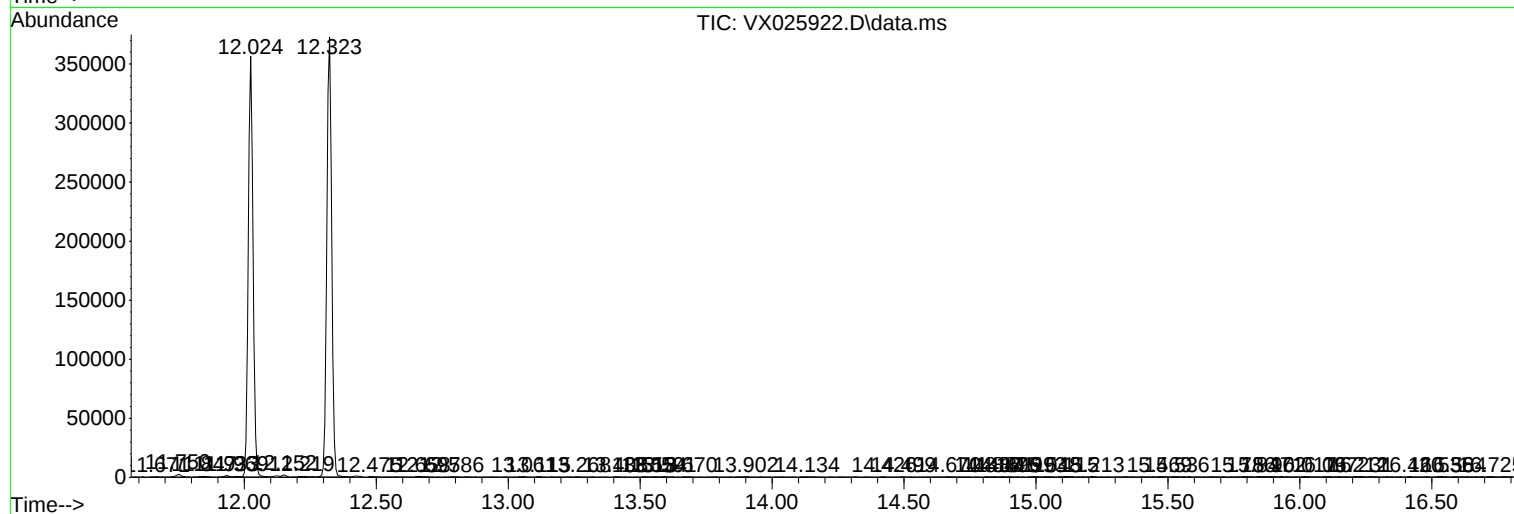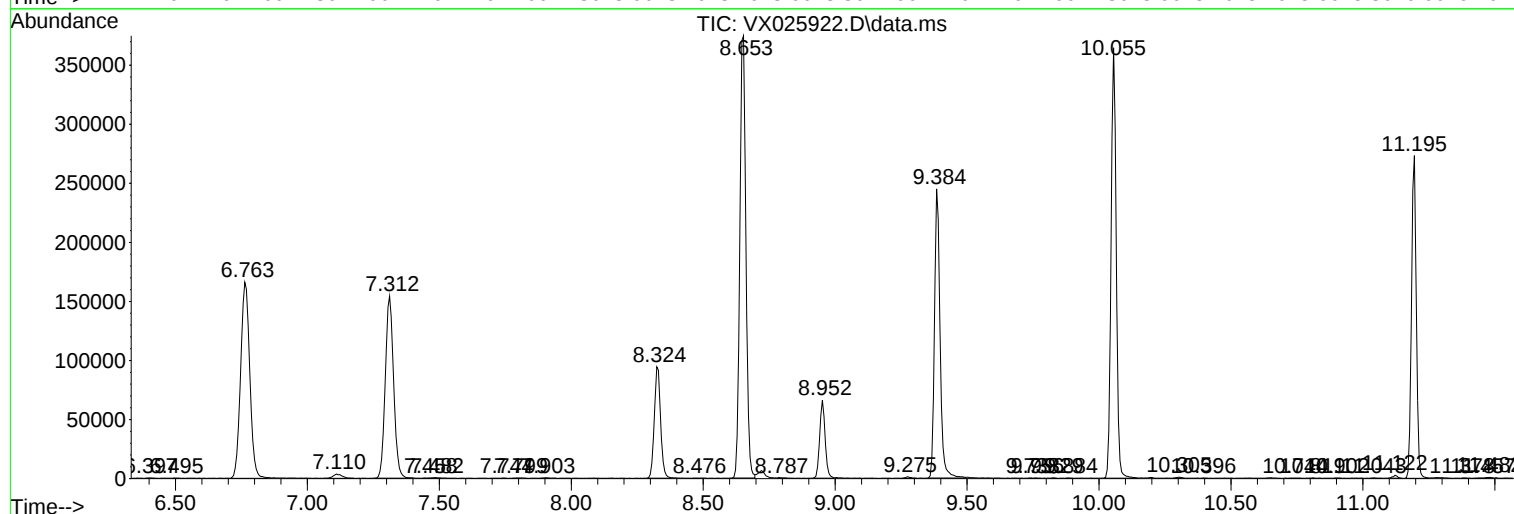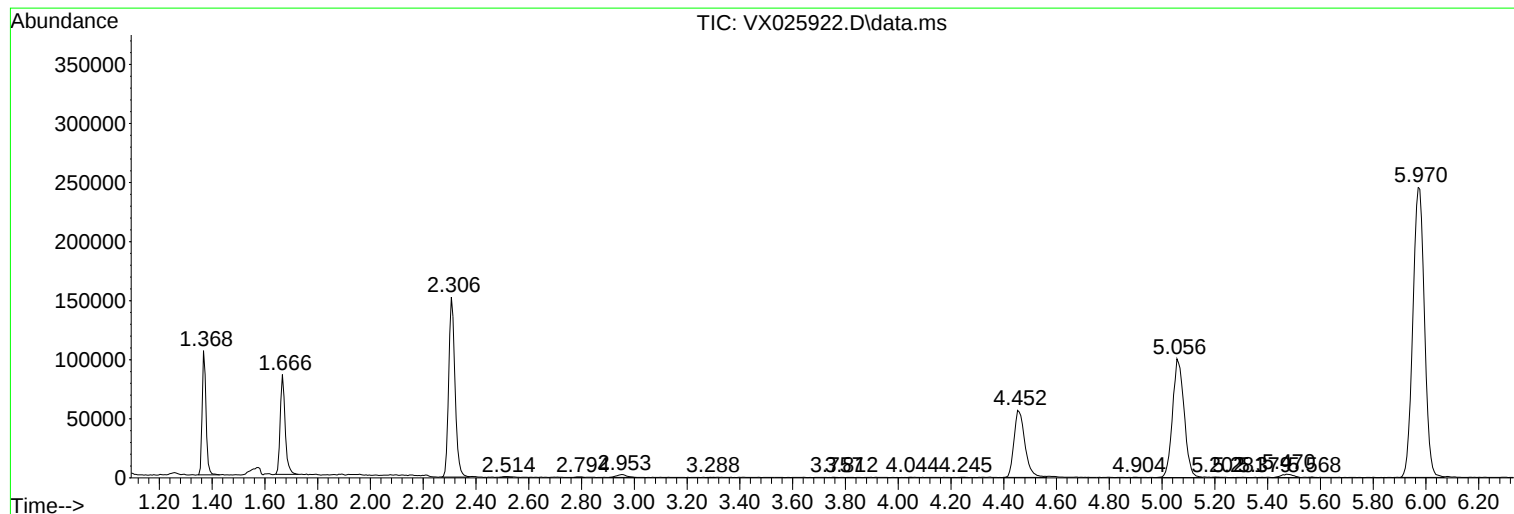

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025922.D
Acq On : 20 Dec 2021 18:28
Operator : JC/MD
Sample : M5150-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025922.D
Acq On : 20 Dec 2021 18:28
Operator : JC/MD
Sample : M5150-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc