

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025923.D
 Acq On : 20 Dec 2021 18:51
 Operator : JC/MD
 Sample : M5150-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025923.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	55	rVB	101115	104158	14.21%	1.934%
2	1.666	91	95	105	rVB	83533	107473	14.66%	1.996%
3	2.306	193	200	208	rBV	149361	249267	34.01%	4.629%
4	2.379	208	212	222	rVB	13610	22978	3.13%	0.427%
5	2.538	234	238	245	rVB2	2852	5318	0.73%	0.099%
6	2.636	253	254	256	rVB	407	284	0.04%	0.005%
7	2.703	261	265	266	rBV2	543	583	0.08%	0.011%
8	2.757	270	274	275	rBV2	192	213	0.03%	0.004%
9	2.794	277	280	283	rVV3	686	839	0.11%	0.016%
10	2.849	286	289	291	rBV2	317	331	0.05%	0.006%
11	2.946	298	305	306	rBV2	1891	3073	0.42%	0.057%
12	3.172	337	342	343	rBV2	279	260	0.04%	0.005%
13	3.580	403	409	415	rVV5	541	1245	0.17%	0.023%
14	4.056	484	487	490	rVB2	189	219	0.03%	0.004%
15	4.202	507	511	512	rBV2	182	202	0.03%	0.004%
16	4.263	518	521	522	rBV2	164	195	0.03%	0.004%
17	4.312	527	529	532	rBV	184	178	0.02%	0.003%
18	4.458	543	553	566	rBV	58797	162316	22.14%	3.014%
19	5.062	640	652	665	rBV2	101417	299859	40.91%	5.568%
20	5.355	698	700	704	rVB2	243	202	0.03%	0.004%
21	5.483	712	721	729	rVB5	1729	5298	0.72%	0.098%
22	5.684	752	754	759	rBV2	210	304	0.04%	0.006%
23	5.976	789	802	817	rBV2	244035	732971	100.00%	13.611%
24	6.318	855	858	859	rBV	272	191	0.03%	0.004%
25	6.336	859	861	863	rVV2	277	225	0.03%	0.004%
26	6.549	893	896	898	rBV2	317	301	0.04%	0.006%
27	6.671	913	916	917	rBV2	242	222	0.03%	0.004%
28	6.763	921	931	943	rBV	160079	379386	51.76%	7.045%
29	7.110	981	988	996	rVV4	2246	4893	0.67%	0.091%
30	7.171	996	998	999	rVV2	312	221	0.03%	0.004%
31	7.312	1012	1021	1039	rVB	150197	333922	45.56%	6.201%
32	7.482	1044	1049	1052	rVV2	400	687	0.09%	0.013%
33	7.750	1091	1093	1096	rVV	207	222	0.03%	0.004%
34	7.811	1096	1103	1108	rVV3	371	976	0.13%	0.018%
35	7.982	1129	1131	1134	rBV	293	217	0.03%	0.004%
36	8.226	1169	1171	1174	rVB2	354	309	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025923.D
 Acq On : 20 Dec 2021 18:51
 Operator : JC/MD
 Sample : M5150-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

37	8.324	1181	1187	1197	rBV	93055	155434	21.21%	2.886%
38	8.464	1209	1210	1211	rBV	360	207	0.03%	0.004%
39	8.482	1211	1213	1216	rVB2	356	238	0.03%	0.004%
40	8.543	1220	1223	1225	rBV2	125	188	0.03%	0.003%
41	8.653	1234	1241	1248	rBV	368864	585004	79.81%	10.863%
42	8.842	1271	1272	1276	rVB2	176	197	0.03%	0.004%
43	8.951	1281	1290	1303	rBV	65035	95134	12.98%	1.767%
44	9.214	1332	1333	1336	rBV2	172	206	0.03%	0.004%
45	9.268	1340	1342	1348	rVB3	725	1096	0.15%	0.020%
46	9.384	1356	1361	1372	rBV	236398	351037	47.89%	6.518%
47	9.622	1397	1400	1402	rVV3	300	385	0.05%	0.007%
48	9.732	1417	1418	1421	rBV2	355	284	0.04%	0.005%
49	9.872	1439	1441	1445	rVV2	261	207	0.03%	0.004%
50	9.945	1451	1453	1456	rVB2	276	235	0.03%	0.004%
51	9.976	1456	1458	1460	rBV2	271	299	0.04%	0.006%
52	10.055	1465	1471	1487	rBV	363497	484732	66.13%	9.001%
53	10.238	1499	1501	1504	rVB2	269	213	0.03%	0.004%
54	10.305	1508	1512	1518	rVB4	1278	1462	0.20%	0.027%
55	10.415	1524	1530	1532	rBV2	175	306	0.04%	0.006%
56	10.652	1565	1569	1570	rBV3	380	424	0.06%	0.008%
57	10.732	1579	1582	1584	rVB2	195	192	0.03%	0.004%
58	10.756	1584	1586	1588	rBV	423	273	0.04%	0.005%
59	10.817	1595	1596	1600	rBV2	204	261	0.04%	0.005%
60	10.963	1619	1620	1623	rVB	405	301	0.04%	0.006%
61	11.036	1630	1632	1635	rBV2	421	401	0.05%	0.007%
62	11.122	1642	1646	1652	rBV2	1803	2560	0.35%	0.048%
63	11.195	1652	1658	1665	rBV	270045	347464	47.40%	6.452%
64	11.286	1669	1673	1674	rBV3	530	671	0.09%	0.012%
65	11.439	1695	1698	1699	rBV	260	252	0.03%	0.005%
66	11.457	1699	1701	1702	rVV2	328	224	0.03%	0.004%
67	11.475	1702	1704	1707	rBV2	801	913	0.12%	0.017%
68	11.603	1723	1725	1728	rVV	197	183	0.02%	0.003%
69	11.750	1745	1749	1753	rVB3	2098	3044	0.42%	0.057%
70	11.835	1761	1763	1768	rBV3	510	572	0.08%	0.011%
71	11.933	1774	1779	1784	rBV3	1103	1584	0.22%	0.029%
72	11.969	1784	1785	1789	rBV2	427	492	0.07%	0.009%
73	12.024	1789	1794	1801	rBV	355735	435023	59.35%	8.078%
74	12.152	1812	1815	1819	rVB3	1561	2106	0.29%	0.039%
75	12.183	1819	1820	1822	rBV	258	196	0.03%	0.004%
76	12.231	1822	1828	1832	rBV5	504	1190	0.16%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025923.D
 Acq On : 20 Dec 2021 18:51
 Operator : JC/MD
 Sample : M5150-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

77	12.323	1837	1843	1849	rVV	373786	483488	65.96%	8.978%
78	12.426	1856	1860	1865	rBV5	547	871	0.12%	0.016%
79	12.475	1865	1868	1870	rVV	325	448	0.06%	0.008%
80	12.664	1895	1899	1903	rBV	454	790	0.11%	0.015%
81	12.695	1903	1904	1907	rVV	222	210	0.03%	0.004%
82	12.865	1929	1932	1934	rBV2	229	225	0.03%	0.004%
83	13.048	1961	1962	1965	rVV2	287	253	0.03%	0.005%
84	13.085	1966	1968	1971	rVB2	356	367	0.05%	0.007%
85	13.109	1971	1972	1974	rBV2	258	212	0.03%	0.004%
86	13.359	2010	2013	2017	rVB3	197	287	0.04%	0.005%
87	13.664	2060	2063	2067	rBV2	218	297	0.04%	0.006%
88	13.713	2070	2071	2075	rBV	162	213	0.03%	0.004%
89	14.207	2150	2152	2155	rBV	279	184	0.03%	0.003%
90	14.518	2200	2203	2204	rBV	137	178	0.02%	0.003%
91	14.560	2207	2210	2211	rBV3	220	211	0.03%	0.004%
92	14.579	2211	2213	2214	rVB	277	191	0.03%	0.004%
93	14.926	2268	2270	2271	rBV	330	244	0.03%	0.005%
94	15.310	2331	2333	2335	rBV	225	248	0.03%	0.005%
95	15.731	2400	2402	2404	rBV2	223	225	0.03%	0.004%
96	16.090	2458	2461	2462	rBV2	266	232	0.03%	0.004%
97	16.158	2471	2472	2474	rBV2	276	227	0.03%	0.004%
98	16.456	2520	2521	2523	rBV	243	203	0.03%	0.004%
99	16.554	2535	2537	2540	rBV	220	249	0.03%	0.005%
100	16.737	2563	2567	2569	rBV3	384	508	0.07%	0.009%




Sum of corrected areas: 5385289

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025923.D
Acq On : 20 Dec 2021 18:51
Operator : JC/MD
Sample : M5150-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

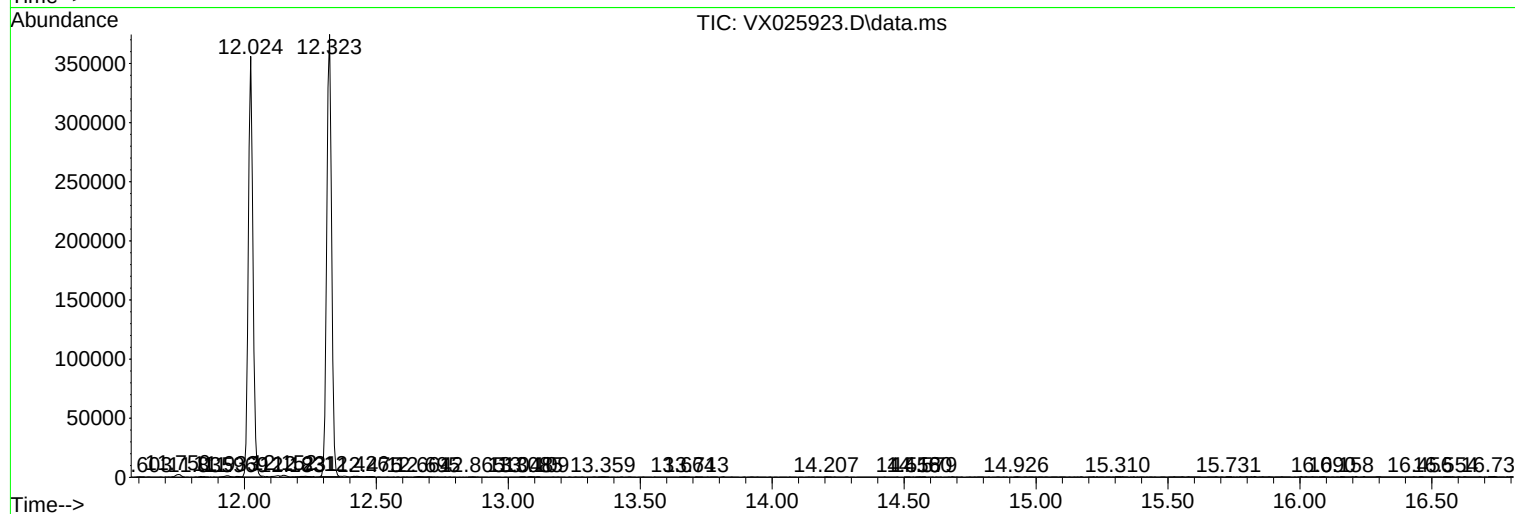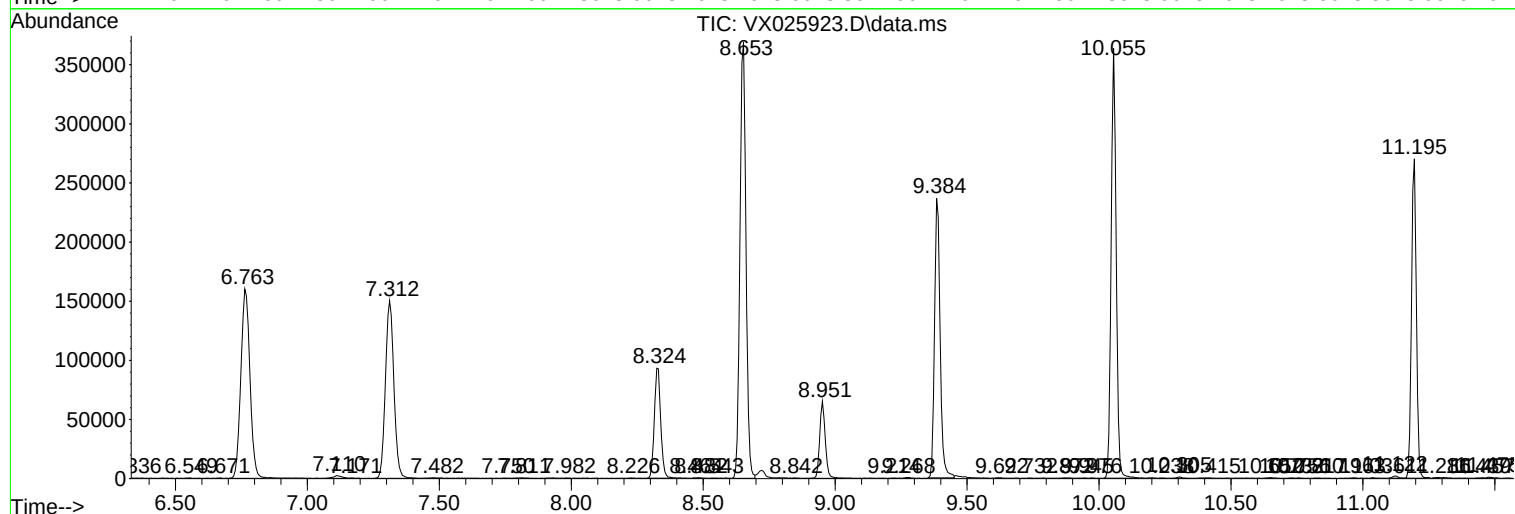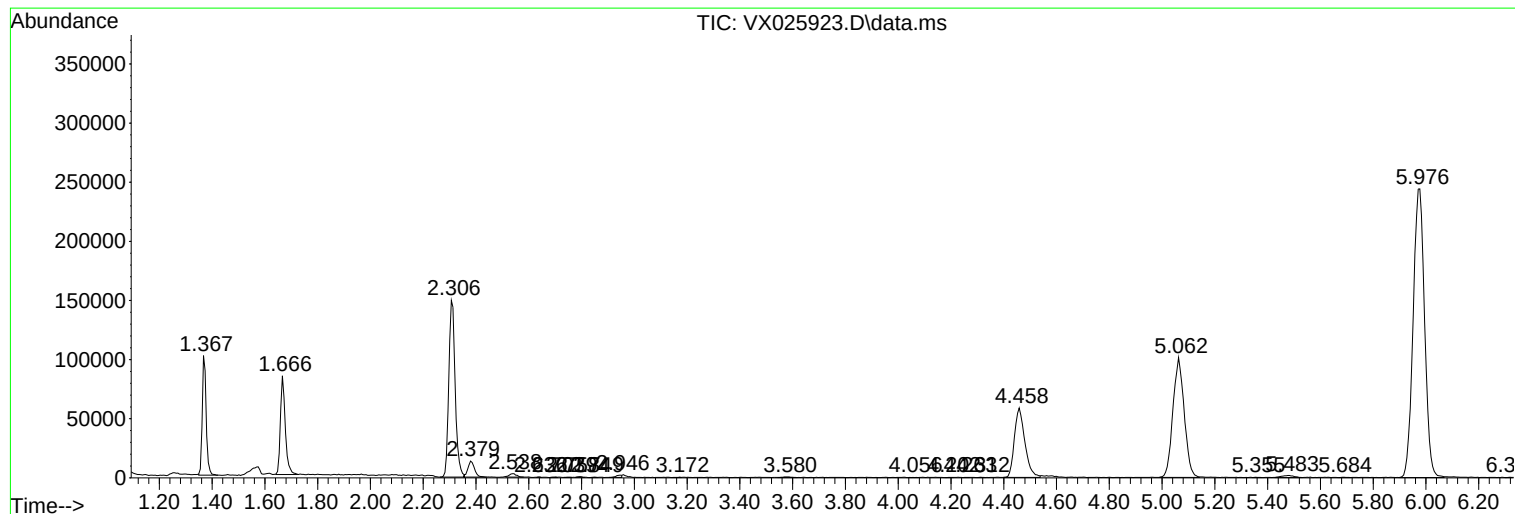

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025923.D
Acq On : 20 Dec 2021 18:51
Operator : JC/MD
Sample : M5150-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025923.D
Acq On : 20 Dec 2021 18:51
Operator : JC/MD
Sample : M5150-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------