

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025925.D
 Acq On : 20 Dec 2021 19:38
 Operator : JC/MD
 Sample : M5150-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M

Title : VOC Analysis

Signal : TIC: VX025925.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	53	rVB	101787	104445	14.09%	1.974%
2	1.666	91	95	102	rVB	85582	106942	14.43%	2.021%
3	2.306	194	200	208	rBV	149141	244448	32.98%	4.619%
4	2.380	208	212	222	rVB	8699	15642	2.11%	0.296%
5	2.544	232	239	244	rBV3	3263	6111	0.82%	0.115%
6	2.623	250	252	253	rBV	325	187	0.03%	0.004%
7	2.782	276	278	279	rBV	446	316	0.04%	0.006%
8	2.880	293	294	297	rBV	298	262	0.04%	0.005%
9	2.947	302	305	314	rVV4	2657	5351	0.72%	0.101%
10	3.008	314	315	318	rVV2	207	215	0.03%	0.004%
11	3.117	330	333	336	rVB2	310	402	0.05%	0.008%
12	3.184	342	344	347	rBV2	323	296	0.04%	0.006%
13	3.556	404	405	406	rBV	522	301	0.04%	0.006%
14	3.843	450	452	455	rBV2	157	218	0.03%	0.004%
15	3.965	470	472	474	rBV	251	261	0.04%	0.005%
16	4.020	479	481	483	rBV2	228	227	0.03%	0.004%
17	4.135	498	500	502	rVB2	185	192	0.03%	0.004%
18	4.458	544	553	567	rBV	55547	161233	21.75%	3.047%
19	4.867	618	620	623	rBV	221	198	0.03%	0.004%
20	5.062	640	652	669	rBV	98507	300107	40.49%	5.671%
21	5.391	704	706	709	rVV2	186	183	0.02%	0.003%
22	5.477	709	720	730	rVV4	2957	8621	1.16%	0.163%
23	5.550	730	732	735	rVB2	302	341	0.05%	0.006%
24	5.970	789	801	819	rBV2	251084	741149	100.00%	14.004%
25	6.263	846	849	852	rBV	176	206	0.03%	0.004%
26	6.324	855	859	861	rBV	304	344	0.05%	0.006%
27	6.635	906	910	913	rBV2	196	250	0.03%	0.005%
28	6.763	921	931	946	rBV	142541	344830	46.53%	6.516%
29	7.117	983	989	995	rVB4	1756	3980	0.54%	0.075%
30	7.171	995	998	1000	rVB3	326	428	0.06%	0.008%
31	7.190	1000	1001	1004	rBV2	256	218	0.03%	0.004%
32	7.312	1012	1021	1038	rBV	155178	335602	45.28%	6.341%
33	7.482	1044	1049	1053	rVB3	471	897	0.12%	0.017%
34	7.562	1059	1062	1063	rBV2	244	207	0.03%	0.004%
35	7.604	1067	1069	1071	rBV	199	184	0.02%	0.003%
36	8.104	1148	1151	1154	rBV2	185	203	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025925.D
 Acq On : 20 Dec 2021 19:38
 Operator : JC/MD
 Sample : M5150-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

37	8.147	1154	1158	1160	rVB2	190	273	0.04%	0.005%
38	8.220	1168	1170	1175	rVB2	195	224	0.03%	0.004%
39	8.324	1181	1187	1200	rBV	93141	153531	20.72%	2.901%
40	8.543	1221	1223	1225	rBV2	219	209	0.03%	0.004%
41	8.574	1225	1228	1231	rBV3	219	359	0.05%	0.007%
42	8.653	1234	1241	1249	rBV	374646	598325	80.73%	11.306%
43	8.952	1284	1290	1297	rBV	65116	92770	12.52%	1.753%
44	9.086	1310	1312	1313	rVV2	297	202	0.03%	0.004%
45	9.122	1316	1318	1322	rBV	172	219	0.03%	0.004%
46	9.275	1340	1343	1346	rVV2	824	856	0.12%	0.016%
47	9.384	1356	1361	1380	rBV	244358	358137	48.32%	6.767%
48	9.604	1395	1397	1398	rBV	335	249	0.03%	0.005%
49	9.909	1444	1447	1450	rBV2	184	248	0.03%	0.005%
50	10.055	1465	1471	1485	rBV	329966	440215	59.40%	8.318%
51	10.201	1491	1495	1498	rBV3	376	482	0.07%	0.009%
52	10.305	1508	1512	1516	rBV2	801	1036	0.14%	0.020%
53	10.476	1538	1540	1543	rVB3	359	345	0.05%	0.007%
54	10.506	1543	1545	1548	rBV2	236	353	0.05%	0.007%
55	10.579	1553	1557	1562	rBV2	161	358	0.05%	0.007%
56	10.640	1564	1567	1569	rBV2	369	387	0.05%	0.007%
57	10.762	1585	1587	1589	rVB	351	258	0.03%	0.005%
58	10.787	1589	1591	1592	rBV2	276	222	0.03%	0.004%
59	10.970	1614	1621	1624	rBV2	405	642	0.09%	0.012%
60	11.024	1628	1630	1632	rBV	352	260	0.04%	0.005%
61	11.043	1632	1633	1637	rVB3	341	288	0.04%	0.005%
62	11.122	1642	1646	1649	rBV2	2076	2714	0.37%	0.051%
63	11.195	1652	1658	1665	rBV	280344	355377	47.95%	6.715%
64	11.384	1687	1689	1692	rBV2	331	460	0.06%	0.009%
65	11.451	1698	1700	1702	rVV	382	376	0.05%	0.007%
66	11.482	1702	1705	1708	rVV2	859	1122	0.15%	0.021%
67	11.628	1727	1729	1734	rBV4	645	877	0.12%	0.017%
68	11.750	1745	1749	1752	rBV3	1562	2290	0.31%	0.043%
69	11.835	1762	1763	1767	rBV2	525	616	0.08%	0.012%
70	11.933	1776	1779	1783	rVB	970	1243	0.17%	0.023%
71	12.024	1789	1794	1807	rVB	311828	393585	53.10%	7.437%
72	12.128	1807	1811	1812	rBV2	891	1172	0.16%	0.022%
73	12.152	1812	1815	1818	rVB3	1820	2025	0.27%	0.038%
74	12.177	1818	1819	1821	rBV	285	241	0.03%	0.005%
75	12.219	1824	1826	1831	rVV3	552	662	0.09%	0.013%
76	12.323	1837	1843	1857	rVB	378447	487032	65.71%	9.203%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025925.D
 Acq On : 20 Dec 2021 19:38
 Operator : JC/MD
 Sample : M5150-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

77	12.420	1857	1859	1862	rBV4	740	815	0.11%	0.015%
78	12.542	1876	1879	1881	rBV	144	202	0.03%	0.004%
79	12.634	1892	1894	1895	rVB2	349	224	0.03%	0.004%
80	12.652	1895	1897	1905	rBV3	386	788	0.11%	0.015%
81	13.000	1952	1954	1956	rVB	245	184	0.02%	0.003%
82	13.048	1960	1962	1966	rVB2	244	238	0.03%	0.004%
83	13.115	1971	1973	1976	rVB2	234	198	0.03%	0.004%
84	13.164	1979	1981	1983	rBV2	187	182	0.02%	0.003%
85	13.268	1994	1998	2001	rBV2	176	272	0.04%	0.005%
86	13.353	2010	2012	2014	rBV	213	185	0.02%	0.003%
87	13.981	2113	2115	2117	rBV2	188	205	0.03%	0.004%
88	14.286	2163	2165	2169	rBV2	228	254	0.03%	0.005%
89	14.426	2184	2188	2189	rBV	189	230	0.03%	0.004%
90	14.481	2195	2197	2200	rVB	258	216	0.03%	0.004%
91	14.694	2230	2232	2235	rBV2	274	329	0.04%	0.006%
92	14.755	2240	2242	2245	rVB3	268	251	0.03%	0.005%
93	14.804	2248	2250	2253	rVB2	225	196	0.03%	0.004%
94	14.853	2257	2258	2260	rBV	257	193	0.03%	0.004%
95	14.951	2270	2274	2275	rBV2	307	394	0.05%	0.007%
96	14.993	2278	2281	2284	rBV2	242	354	0.05%	0.007%
97	15.798	2411	2413	2416	rBV2	320	235	0.03%	0.004%
98	16.115	2463	2465	2466	rBV	272	201	0.03%	0.004%
99	16.231	2482	2484	2486	rVB	316	207	0.03%	0.004%
100	16.383	2505	2509	2512	rBV3	334	531	0.07%	0.010%




Sum of corrected areas: 5292321

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025925.D
Acq On : 20 Dec 2021 19:38
Operator : JC/MD
Sample : M5150-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

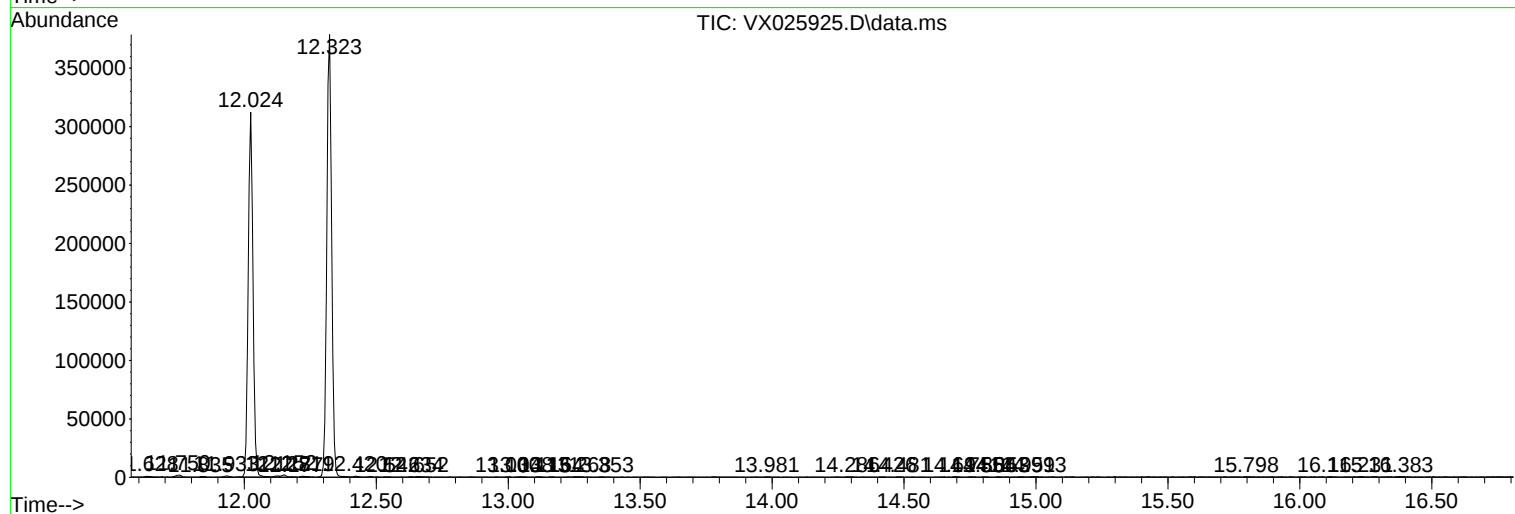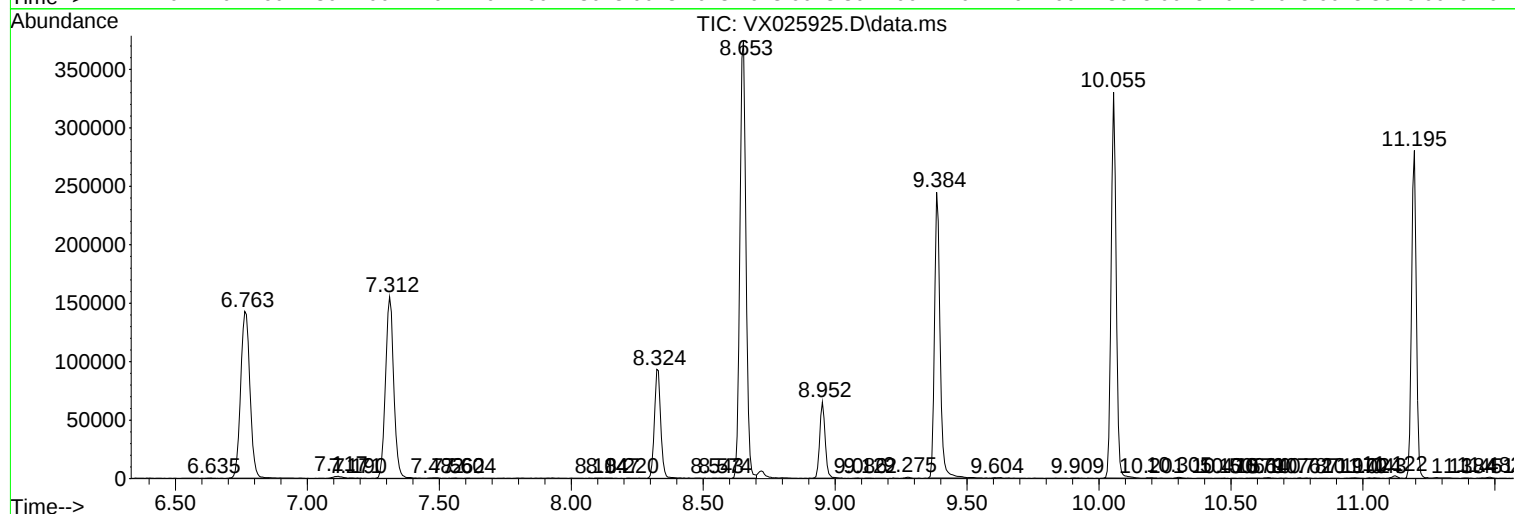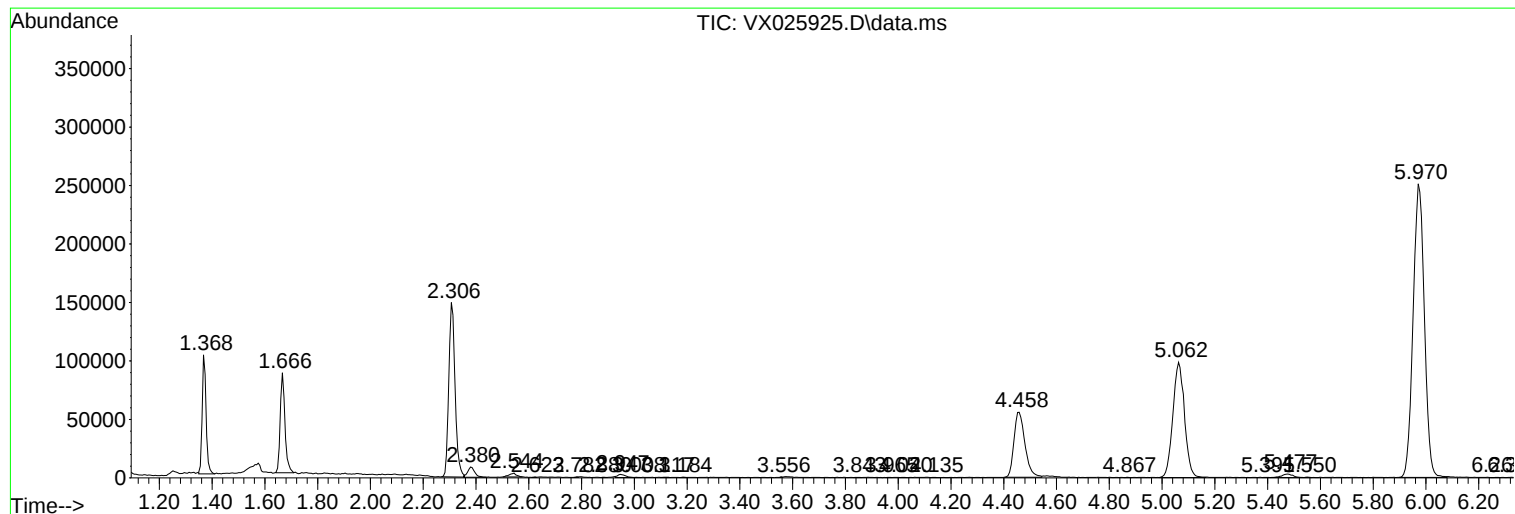

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025925.D
Acq On : 20 Dec 2021 19:38
Operator : JC/MD
Sample : M5150-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025925.D
Acq On : 20 Dec 2021 19:38
Operator : JC/MD
Sample : M5150-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------