

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025926.D
 Acq On : 20 Dec 2021 20:01
 Operator : JC/MD
 Sample : M5150-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025926.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	12	rVB2	2930	2537	0.35%	0.047%
2	1.368	43	46	55	rVB	107660	106481	14.66%	1.985%
3	1.666	91	95	105	rVB	82804	104761	14.42%	1.953%
4	2.307	194	200	208	rBV	144682	241009	33.17%	4.494%
5	2.429	218	220	222	rVB2	446	267	0.04%	0.005%
6	2.538	230	238	246	rBV4	1643	4320	0.59%	0.081%
7	2.794	276	280	284	rVB3	771	906	0.12%	0.017%
8	2.953	298	306	313	rBV	2535	5874	0.81%	0.110%
9	3.093	328	329	331	rVB	301	197	0.03%	0.004%
10	3.459	388	389	392	rVB2	293	193	0.03%	0.004%
11	3.483	392	393	397	rBV2	157	231	0.03%	0.004%
12	3.581	405	409	412	rVB3	487	687	0.09%	0.013%
13	3.751	434	437	439	rVB2	179	225	0.03%	0.004%
14	3.953	467	470	471	rBV	264	196	0.03%	0.004%
15	4.453	543	552	567	rBV	55642	165155	22.73%	3.079%
16	4.800	607	609	612	rBV	194	288	0.04%	0.005%
17	5.062	638	652	667	rBV	94653	294932	40.60%	5.499%
18	5.337	695	697	702	rVB2	281	400	0.06%	0.007%
19	5.465	709	718	719	rBV	4180	6294	0.87%	0.117%
20	5.971	789	801	817	rBV3	241224	726520	100.00%	13.546%
21	6.141	827	829	833	rVB2	313	261	0.04%	0.005%
22	6.306	852	856	859	rBV2	252	307	0.04%	0.006%
23	6.763	922	931	946	rVV	163331	389666	53.63%	7.265%
24	7.129	982	991	999	rVB7	8197	19447	2.68%	0.363%
25	7.202	1001	1003	1007	rBV2	200	180	0.02%	0.003%
26	7.312	1013	1021	1035	rBV	150319	326416	44.93%	6.086%
27	7.476	1044	1048	1049	rBV2	435	526	0.07%	0.010%
28	7.574	1060	1064	1067	rBV2	352	406	0.06%	0.008%
29	7.806	1099	1102	1107	rBV3	299	420	0.06%	0.008%
30	7.909	1117	1119	1120	rBV2	247	214	0.03%	0.004%
31	8.190	1163	1165	1167	rBV2	227	194	0.03%	0.004%
32	8.226	1169	1171	1173	rBV	207	256	0.04%	0.005%
33	8.324	1181	1187	1198	rBV	90132	149149	20.53%	2.781%
34	8.434	1203	1205	1207	rBV	183	195	0.03%	0.004%
35	8.568	1224	1227	1233	rBV2	255	458	0.06%	0.009%
36	8.653	1234	1241	1248	rVV	363372	581497	80.04%	10.842%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025926.D
 Acq On : 20 Dec 2021 20:01
 Operator : JC/MD
 Sample : M5150-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

37	8.720	1249	1252	1258	rVB2	6009	10248	1.41%	0.191%
38	8.885	1277	1279	1282	rVB2	338	264	0.04%	0.005%
39	8.952	1284	1290	1300	rBV	60977	89552	12.33%	1.670%
40	9.110	1315	1316	1319	rVB2	201	189	0.03%	0.004%
41	9.275	1340	1343	1348	rVB4	635	857	0.12%	0.016%
42	9.385	1356	1361	1385	rBV	236479	348155	47.92%	6.491%
43	9.635	1399	1402	1403	rBV2	228	224	0.03%	0.004%
44	10.055	1465	1471	1488	rBV	367287	497716	68.51%	9.280%
45	10.195	1492	1494	1498	rBV	289	373	0.05%	0.007%
46	10.275	1505	1507	1509	rBV2	172	214	0.03%	0.004%
47	10.305	1509	1512	1515	rVV2	1090	1279	0.18%	0.024%
48	10.360	1519	1521	1524	rBV2	241	299	0.04%	0.006%
49	10.647	1564	1568	1570	rVV3	317	463	0.06%	0.009%
50	10.964	1616	1620	1622	rBV2	242	290	0.04%	0.005%
51	11.018	1625	1629	1630	rBV2	211	273	0.04%	0.005%
52	11.037	1630	1632	1635	rBV2	312	357	0.05%	0.007%
53	11.122	1642	1646	1650	rVB3	2157	2502	0.34%	0.047%
54	11.195	1652	1658	1668	rVV	262396	340908	46.92%	6.356%
55	11.275	1668	1671	1675	rBV2	537	736	0.10%	0.014%
56	11.457	1697	1701	1702	rBV3	397	447	0.06%	0.008%
57	11.482	1702	1705	1707	rVV2	828	816	0.11%	0.015%
58	11.549	1713	1716	1717	rBV	250	247	0.03%	0.005%
59	11.604	1721	1725	1726	rBV2	171	180	0.02%	0.003%
60	11.750	1744	1749	1753	rVV2	1727	2482	0.34%	0.046%
61	11.793	1754	1756	1759	rVB2	290	247	0.03%	0.005%
62	11.848	1762	1765	1768	rBV2	374	397	0.05%	0.007%
63	11.896	1770	1773	1774	rVB	262	215	0.03%	0.004%
64	11.933	1777	1779	1783	rVB3	886	956	0.13%	0.018%
65	12.024	1788	1794	1802	rBV	352204	443804	61.09%	8.275%
66	12.122	1806	1810	1812	rBV3	869	1283	0.18%	0.024%
67	12.226	1822	1827	1830	rVV3	708	988	0.14%	0.018%
68	12.323	1836	1843	1851	rBV	365847	475523	65.45%	8.866%
69	12.427	1857	1860	1865	rBV2	684	1119	0.15%	0.021%
70	12.488	1865	1870	1872	rVV2	402	504	0.07%	0.009%
71	12.597	1886	1888	1891	rBV	205	225	0.03%	0.004%
72	12.634	1891	1894	1896	rVB2	210	191	0.03%	0.004%
73	12.665	1896	1899	1901	rBV3	580	567	0.08%	0.011%
74	12.768	1912	1916	1917	rVB2	170	180	0.02%	0.003%
75	12.963	1944	1948	1949	rBV	176	217	0.03%	0.004%
76	13.061	1961	1964	1969	rBV2	302	510	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025926.D
 Acq On : 20 Dec 2021 20:01
 Operator : JC/MD
 Sample : M5150-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

77	13.103	1969	1971	1975	rVB	264	260	0.04%	0.005%
78	13.140	1975	1977	1979	rBV2	212	227	0.03%	0.004%
79	13.195	1983	1986	1987	rBV2	186	189	0.03%	0.004%
80	13.292	2000	2002	2003	rVB	480	220	0.03%	0.004%
81	13.353	2009	2012	2014	rBV2	198	201	0.03%	0.004%
82	13.506	2035	2037	2040	rBV2	210	236	0.03%	0.004%
83	13.634	2056	2058	2060	rBV2	233	239	0.03%	0.004%
84	13.756	2076	2078	2080	rVB2	212	182	0.03%	0.003%
85	13.786	2080	2083	2088	rVB3	235	349	0.05%	0.007%
86	14.518	2201	2203	2208	rVB2	282	335	0.05%	0.006%
87	14.567	2208	2211	2212	rBV2	216	211	0.03%	0.004%
88	14.670	2226	2228	2229	rVV	290	181	0.02%	0.003%
89	14.719	2232	2236	2237	rVB	287	288	0.04%	0.005%
90	14.804	2248	2250	2253	rVB3	238	288	0.04%	0.005%
91	14.878	2260	2262	2266	rBV3	331	362	0.05%	0.007%
92	15.036	2286	2288	2290	rBV2	212	227	0.03%	0.004%
93	15.231	2319	2320	2322	rBV	283	225	0.03%	0.004%
94	15.390	2342	2346	2347	rBV2	314	358	0.05%	0.007%
95	15.493	2361	2363	2365	rBV2	209	203	0.03%	0.004%
96	16.048	2451	2454	2456	rVB2	370	412	0.06%	0.008%
97	16.072	2456	2458	2459	rBV	196	206	0.03%	0.004%
98	16.158	2469	2472	2475	rBV2	327	264	0.04%	0.005%
99	16.237	2483	2485	2487	rBV2	314	317	0.04%	0.006%
100	16.554	2535	2537	2540	rVB2	343	308	0.04%	0.006%




Sum of corrected areas: 5363350

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025926.D
Acq On : 20 Dec 2021 20:01
Operator : JC/MD
Sample : M5150-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

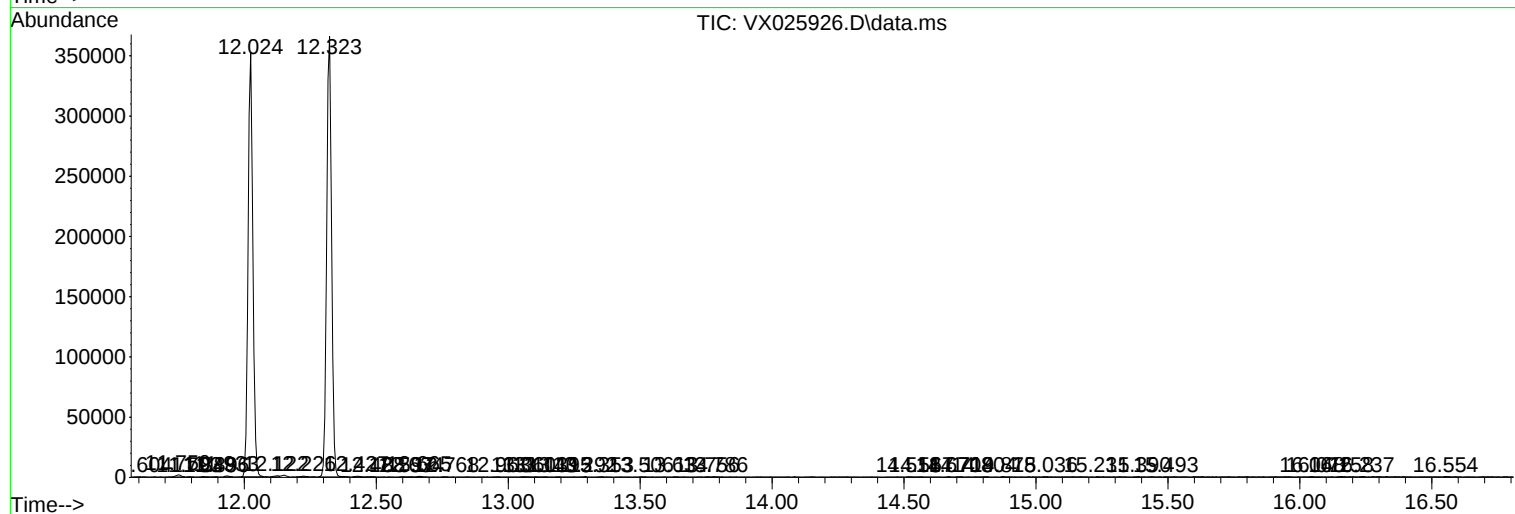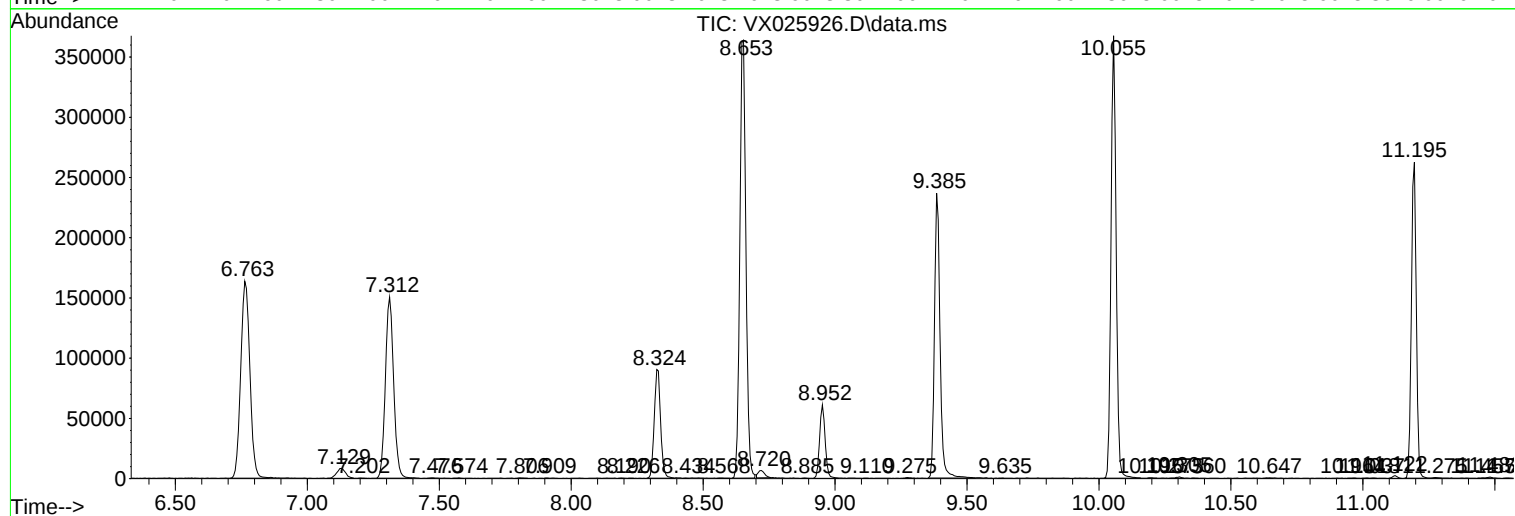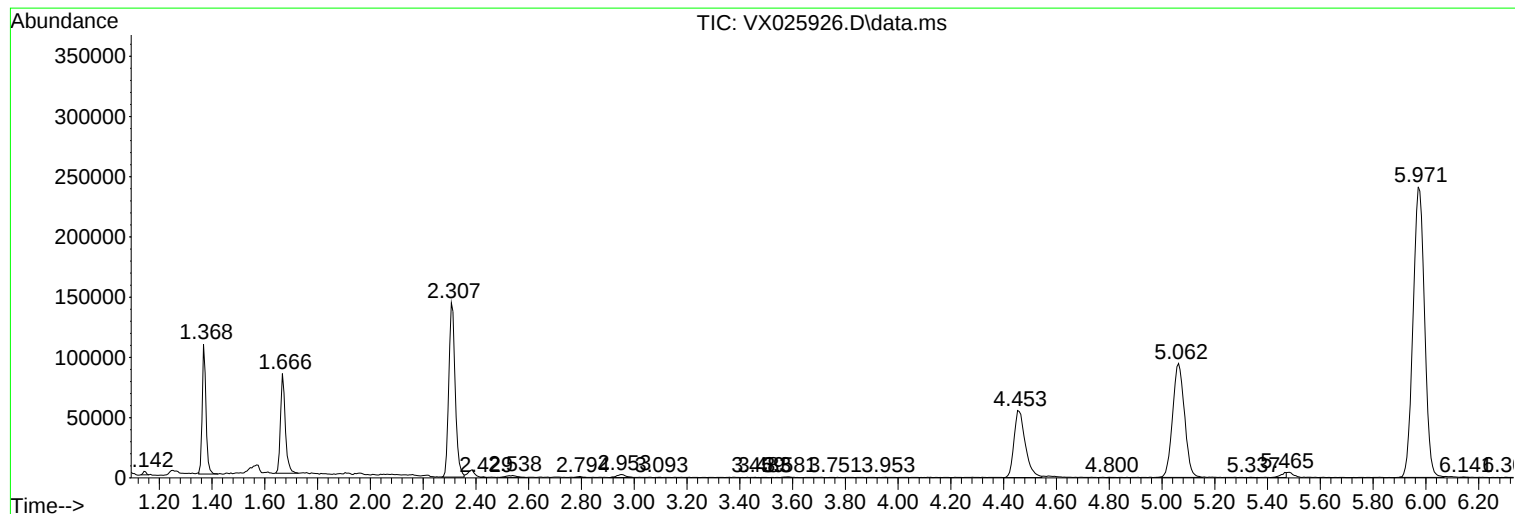

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025926.D
Acq On : 20 Dec 2021 20:01
Operator : JC/MD
Sample : M5150-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025926.D
Acq On : 20 Dec 2021 20:01
Operator : JC/MD
Sample : M5150-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------