

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025927.D
 Acq On : 20 Dec 2021 20:25
 Operator : JC/MD
 Sample : M5150-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025927.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	13	rBV3	2126	2005	0.27%	0.037%
2	1.252	23	27	33	rBV2	5270	10350	1.41%	0.190%
3	1.367	43	46	54	rVB	103510	103547	14.11%	1.902%
4	1.666	91	95	106	rVB	83879	109582	14.93%	2.013%
5	2.306	194	200	208	rBV	146192	244637	33.33%	4.494%
6	2.379	209	212	225	rVB	8503	14523	1.98%	0.267%
7	2.483	225	229	231	rBV2	217	282	0.04%	0.005%
8	2.538	233	238	249	rVB3	3413	6828	0.93%	0.125%
9	2.788	277	279	284	rVB2	559	736	0.10%	0.014%
10	2.825	284	285	288	rVB3	343	299	0.04%	0.005%
11	2.946	297	305	313	rVB2	2851	6803	0.93%	0.125%
12	3.093	327	329	332	rVB	341	210	0.03%	0.004%
13	3.209	347	348	353	rBV2	249	264	0.04%	0.005%
14	3.343	367	370	373	rVB2	332	334	0.05%	0.006%
15	3.580	405	409	411	rVB2	354	330	0.04%	0.006%
16	3.599	411	412	414	rVB2	333	183	0.02%	0.003%
17	3.861	453	455	459	rVB2	195	202	0.03%	0.004%
18	4.044	483	485	490	rVB	169	274	0.04%	0.005%
19	4.093	490	493	496	rBV2	171	196	0.03%	0.004%
20	4.239	513	517	518	rBV2	192	187	0.03%	0.003%
21	4.458	543	553	566	rBV	56449	167511	22.82%	3.077%
22	5.062	639	652	672	rBV	96205	298990	40.74%	5.492%
23	5.483	712	721	728	rVV6	1806	5062	0.69%	0.093%
24	5.556	731	733	735	rBV	413	283	0.04%	0.005%
25	5.604	739	741	744	rVB	238	202	0.03%	0.004%
26	5.806	770	774	779	rVB2	306	510	0.07%	0.009%
27	5.976	789	802	816	rBV2	245798	733978	100.00%	13.482%
28	6.763	922	931	944	rBV	163455	391326	53.32%	7.188%
29	6.921	956	957	959	rBV	257	185	0.03%	0.003%
30	7.055	976	979	983	rBV2	173	346	0.05%	0.006%
31	7.129	983	991	1000	rBV6	9982	24216	3.30%	0.445%
32	7.238	1007	1009	1012	rBV3	263	253	0.03%	0.005%
33	7.312	1012	1021	1032	rBV	152613	332825	45.35%	6.113%
34	7.427	1038	1040	1042	rVB	278	250	0.03%	0.005%
35	7.464	1042	1046	1047	rBV2	189	250	0.03%	0.005%
36	7.488	1047	1050	1054	rVV2	559	746	0.10%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025927.D
 Acq On : 20 Dec 2021 20:25
 Operator : JC/MD
 Sample : M5150-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

37	7.677	1079	1081	1084	rVB	257	180	0.02%	0.003%
38	7.702	1084	1085	1087	rBV2	319	202	0.03%	0.004%
39	7.805	1100	1102	1108	rVB3	347	550	0.07%	0.010%
40	7.921	1119	1121	1122	rBV2	235	193	0.03%	0.004%
41	8.098	1147	1150	1154	rBV2	208	276	0.04%	0.005%
42	8.128	1154	1155	1159	rVB2	182	207	0.03%	0.004%
43	8.165	1159	1161	1164	rBV	184	218	0.03%	0.004%
44	8.324	1181	1187	1197	rBV	89071	151846	20.69%	2.789%
45	8.439	1204	1206	1209	rBV	261	280	0.04%	0.005%
46	8.476	1209	1212	1219	rVB2	293	557	0.08%	0.010%
47	8.653	1234	1241	1248	rBV	374666	592141	80.68%	10.877%
48	8.903	1279	1282	1284	rBV2	192	203	0.03%	0.004%
49	8.951	1284	1290	1299	rBV	62116	92058	12.54%	1.691%
50	9.275	1341	1343	1345	rVB2	575	381	0.05%	0.007%
51	9.384	1356	1361	1377	rBV	239096	350446	47.75%	6.437%
52	9.616	1396	1399	1400	rBV	292	249	0.03%	0.005%
53	9.842	1433	1436	1437	rVB2	252	212	0.03%	0.004%
54	9.860	1437	1439	1441	rBV	217	188	0.03%	0.003%
55	9.902	1443	1446	1449	rBV2	128	173	0.02%	0.003%
56	10.055	1465	1471	1487	rBV	376006	499988	68.12%	9.184%
57	10.195	1492	1494	1498	rVB	404	353	0.05%	0.006%
58	10.256	1503	1504	1507	rBV2	310	283	0.04%	0.005%
59	10.305	1508	1512	1517	rVV3	826	1192	0.16%	0.022%
60	10.646	1565	1568	1573	rVB3	520	573	0.08%	0.011%
61	10.896	1606	1609	1614	rBV2	289	563	0.08%	0.010%
62	10.957	1618	1619	1621	rBV2	314	209	0.03%	0.004%
63	11.122	1641	1646	1649	rBV2	1911	2831	0.39%	0.052%
64	11.195	1652	1658	1668	rBV	265109	347880	47.40%	6.390%
65	11.311	1675	1677	1679	rVV3	396	221	0.03%	0.004%
66	11.555	1714	1717	1718	rBV2	241	258	0.04%	0.005%
67	11.658	1731	1734	1737	rVB2	146	179	0.02%	0.003%
68	11.713	1740	1743	1745	rVV	227	290	0.04%	0.005%
69	11.750	1745	1749	1753	rVB6	2186	2439	0.33%	0.045%
70	11.841	1762	1764	1767	rBV3	353	375	0.05%	0.007%
71	11.933	1776	1779	1784	rVV4	1133	1425	0.19%	0.026%
72	12.024	1789	1794	1805	rVV	358586	443061	60.36%	8.138%
73	12.122	1808	1810	1812	rVV2	877	955	0.13%	0.018%
74	12.152	1812	1815	1820	rVB2	1850	2073	0.28%	0.038%
75	12.225	1823	1827	1831	rBV3	696	1073	0.15%	0.020%
76	12.323	1837	1843	1851	rVB	377832	481562	65.61%	8.846%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025927.D
 Acq On : 20 Dec 2021 20:25
 Operator : JC/MD
 Sample : M5150-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

77	12.426	1856	1860	1865	rBV4	777	1015	0.14%	0.019%
78	12.487	1865	1870	1875	rVB3	371	657	0.09%	0.012%
79	12.536	1875	1878	1880	rBV2	249	373	0.05%	0.007%
80	12.957	1945	1947	1950	rVB	233	190	0.03%	0.003%
81	13.060	1961	1964	1966	rVV2	253	226	0.03%	0.004%
82	13.798	2083	2085	2086	rVB	363	212	0.03%	0.004%
83	13.908	2099	2103	2105	rVB2	177	196	0.03%	0.004%
84	13.963	2111	2112	2116	rBV2	194	213	0.03%	0.004%
85	14.097	2131	2134	2135	rBV	281	307	0.04%	0.006%
86	14.127	2138	2139	2142	rBV2	195	172	0.02%	0.003%
87	14.207	2150	2152	2154	rBV2	237	297	0.04%	0.005%
88	14.292	2165	2166	2170	rVB2	195	237	0.03%	0.004%
89	14.450	2189	2192	2193	rBV2	227	275	0.04%	0.005%
90	14.530	2203	2205	2207	rBV2	281	226	0.03%	0.004%
91	14.932	2269	2271	2273	rBV	217	190	0.03%	0.003%
92	14.969	2275	2277	2279	rBV2	241	198	0.03%	0.004%
93	14.999	2279	2282	2283	rBV2	248	228	0.03%	0.004%
94	15.365	2339	2342	2345	rBV3	312	426	0.06%	0.008%
95	15.651	2388	2389	2393	rBV2	368	341	0.05%	0.006%
96	15.706	2395	2398	2399	rBV2	295	212	0.03%	0.004%
97	15.810	2414	2415	2418	rBV2	213	258	0.04%	0.005%
98	16.609	2544	2546	2547	rBV2	244	184	0.03%	0.003%
99	16.712	2560	2563	2564	rBV2	266	251	0.03%	0.005%
100	16.743	2566	2568	2570	rVV	227	185	0.03%	0.003%




Sum of corrected areas: 5444117

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025927.D
Acq On : 20 Dec 2021 20:25
Operator : JC/MD
Sample : M5150-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

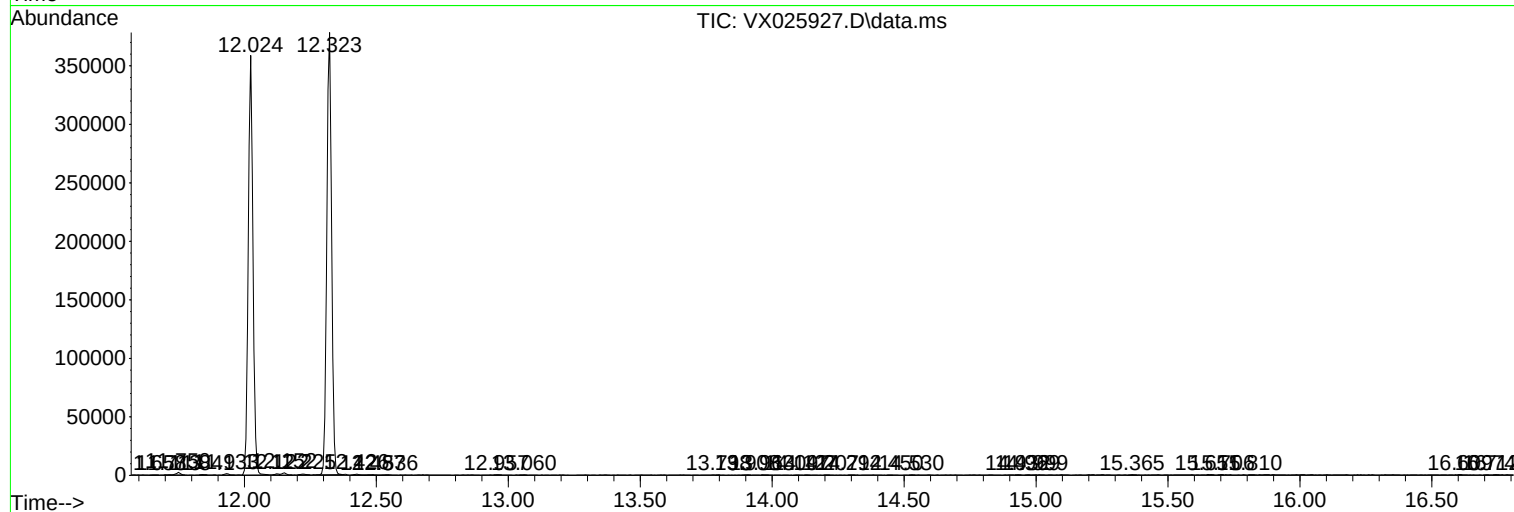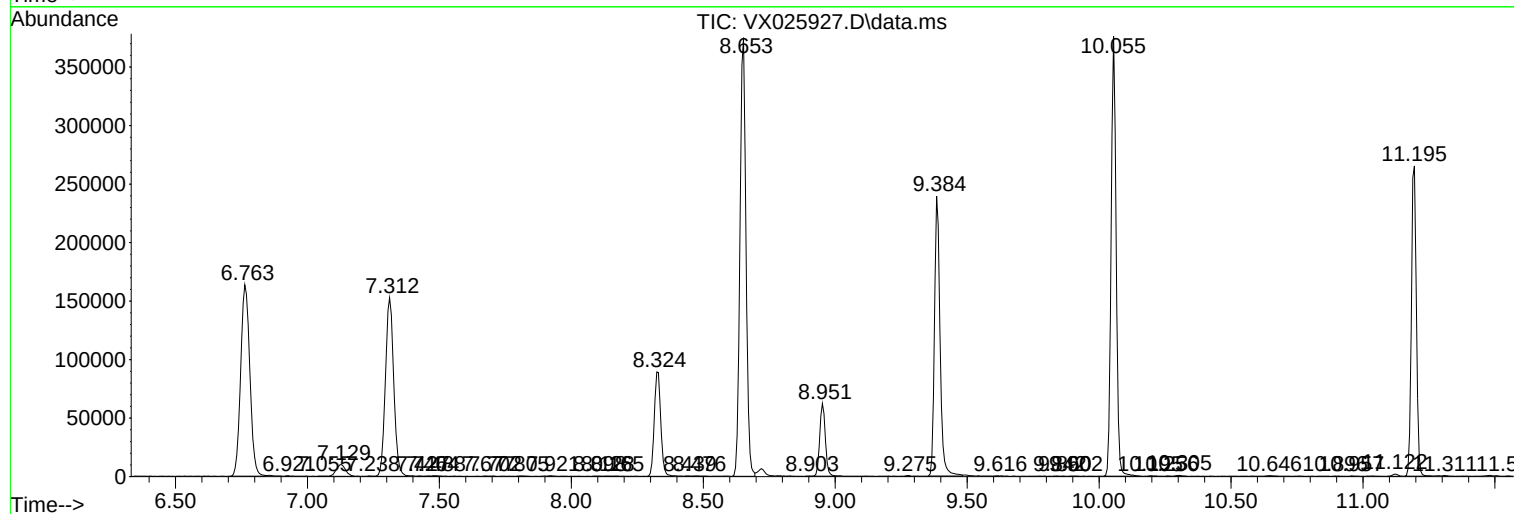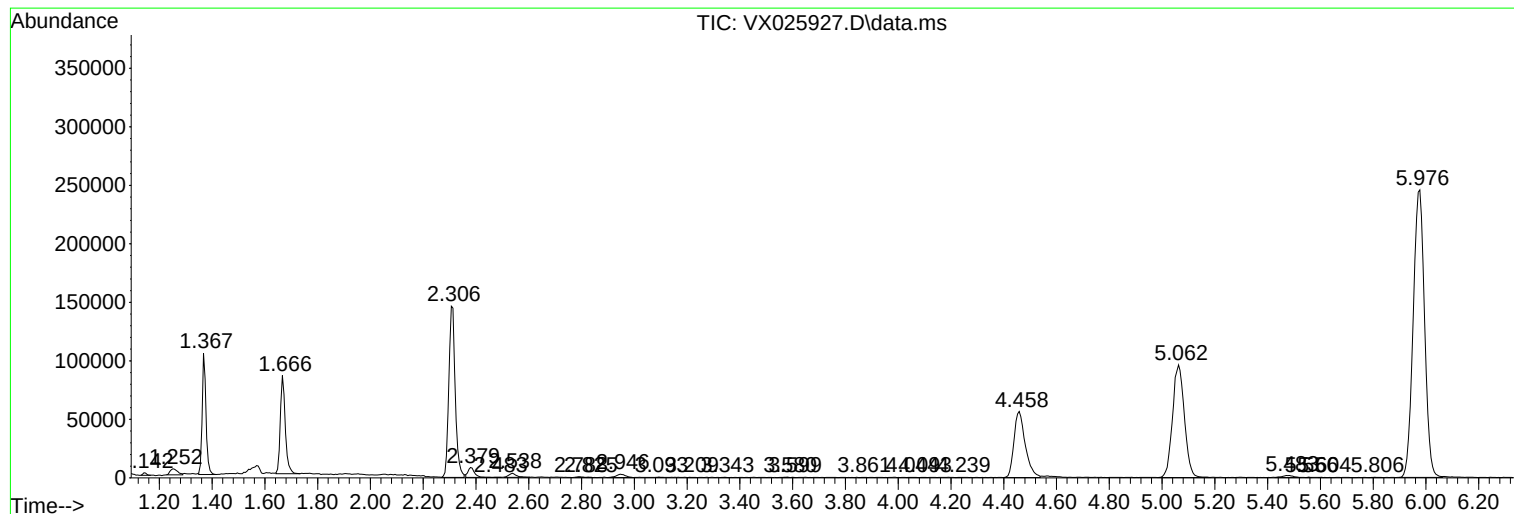

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025927.D
Acq On : 20 Dec 2021 20:25
Operator : JC/MD
Sample : M5150-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025927.D
Acq On : 20 Dec 2021 20:25
Operator : JC/MD
Sample : M5150-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc