

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025932.D
 Acq On : 20 Dec 2021 22:21
 Operator : JC/MD
 Sample : M5150-12DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025932.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	33	rBV2	5433	10568	1.55%	0.210%
2	1.368	43	46	57	rVB	90260	93420	13.71%	1.854%
3	1.666	91	95	105	rVB	78751	96962	14.23%	1.924%
4	2.306	194	200	210	rBV	134433	223253	32.77%	4.431%
5	2.593	244	247	248	rVB2	235	191	0.03%	0.004%
6	2.605	248	249	252	rBV2	298	239	0.04%	0.005%
7	2.636	252	254	257	rBV	303	268	0.04%	0.005%
8	2.697	262	264	265	rBV	296	178	0.03%	0.004%
9	2.788	272	279	283	rBV4	1450	2608	0.38%	0.052%
10	2.892	295	296	299	rBV	297	211	0.03%	0.004%
11	2.947	300	305	309	rBV3	1277	2194	0.32%	0.044%
12	3.008	314	315	320	rVB2	203	174	0.03%	0.003%
13	3.276	357	359	361	rBV2	217	176	0.03%	0.003%
14	3.660	420	422	424	rBV2	163	175	0.03%	0.003%
15	3.684	424	426	431	rVV2	198	347	0.05%	0.007%
16	3.739	433	435	437	rVB2	310	167	0.02%	0.003%
17	3.764	437	439	442	rBV	174	247	0.04%	0.005%
18	3.965	468	472	473	rBV2	255	246	0.04%	0.005%
19	3.983	473	475	477	rVB	246	169	0.02%	0.003%
20	4.257	518	520	524	rBV	308	425	0.06%	0.008%
21	4.459	543	553	568	rVV	52141	149802	21.99%	2.973%
22	4.721	594	596	598	rBV2	226	230	0.03%	0.005%
23	4.788	605	607	610	rVV	182	203	0.03%	0.004%
24	4.812	610	611	613	rVB	306	176	0.03%	0.003%
25	4.879	619	622	625	rVB2	214	245	0.04%	0.005%
26	5.062	640	652	672	rVV	89625	276610	40.60%	5.489%
27	5.196	672	674	675	rVB	318	184	0.03%	0.004%
28	5.556	732	733	737	rVB2	319	207	0.03%	0.004%
29	5.672	749	752	753	rBV	234	214	0.03%	0.004%
30	5.977	789	802	822	rBV2	231350	681306	100.00%	13.521%
31	6.111	822	824	826	rVB2	503	335	0.05%	0.007%
32	6.202	837	839	841	rBV	229	197	0.03%	0.004%
33	6.227	841	843	845	rVB	294	196	0.03%	0.004%
34	6.586	901	902	906	rBV2	149	180	0.03%	0.004%
35	6.763	921	931	943	rBV	153825	372253	54.64%	7.388%
36	6.995	967	969	971	rVB	224	170	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025932.D
 Acq On : 20 Dec 2021 22:21
 Operator : JC/MD
 Sample : M5150-12DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

37	7.068	977	981	982	rBV2	291	349	0.05%	0.007%
38	7.123	982	990	1004	rVB4	24308	57714	8.47%	1.145%
39	7.312	1012	1021	1032	rBV	140723	305955	44.91%	6.072%
40	7.482	1041	1049	1055	rBV4	588	1277	0.19%	0.025%
41	7.696	1083	1084	1086	rVB	292	191	0.03%	0.004%
42	7.812	1101	1103	1106	rVB	307	313	0.05%	0.006%
43	7.927	1120	1122	1124	rBV2	342	353	0.05%	0.007%
44	8.013	1134	1136	1138	rBV2	188	172	0.03%	0.003%
45	8.330	1180	1188	1197	rBV	80626	138285	20.30%	2.744%
46	8.476	1208	1212	1215	rBV2	353	561	0.08%	0.011%
47	8.653	1234	1241	1248	rBV	352354	545619	80.08%	10.828%
48	8.952	1284	1290	1301	rBV	57507	83733	12.29%	1.662%
49	9.384	1356	1361	1375	rBV	215613	319077	46.83%	6.332%
50	9.726	1416	1417	1421	rVB2	352	312	0.05%	0.006%
51	9.866	1438	1440	1442	rVB2	242	203	0.03%	0.004%
52	9.890	1442	1444	1446	rBV2	175	174	0.03%	0.003%
53	10.055	1465	1471	1487	rVV	349814	474576	69.66%	9.418%
54	10.189	1491	1493	1495	rVB2	327	294	0.04%	0.006%
55	10.311	1509	1513	1515	rVV3	502	642	0.09%	0.013%
56	10.354	1518	1520	1522	rBV2	242	200	0.03%	0.004%
57	10.421	1529	1531	1536	rBV	156	203	0.03%	0.004%
58	10.683	1572	1574	1577	rVB2	271	289	0.04%	0.006%
59	10.774	1587	1589	1590	rBV	253	165	0.02%	0.003%
60	10.823	1594	1597	1599	rBV	222	194	0.03%	0.004%
61	10.848	1599	1601	1606	rBV2	212	309	0.05%	0.006%
62	11.049	1632	1634	1638	rBV	148	179	0.03%	0.004%
63	11.122	1643	1646	1652	rVB4	1557	1978	0.29%	0.039%
64	11.195	1652	1658	1666	rBV	245149	319512	46.90%	6.341%
65	11.274	1669	1671	1674	rBV3	355	476	0.07%	0.009%
66	11.366	1684	1686	1691	rBV2	208	403	0.06%	0.008%
67	11.482	1703	1705	1707	rVB3	437	354	0.05%	0.007%
68	11.555	1714	1717	1722	rVB	276	327	0.05%	0.006%
69	11.750	1745	1749	1754	rVB3	1405	1770	0.26%	0.035%
70	11.805	1756	1758	1761	rBV	278	262	0.04%	0.005%
71	11.835	1761	1763	1764	rBV	253	229	0.03%	0.005%
72	11.933	1775	1779	1782	rVB3	766	1073	0.16%	0.021%
73	12.024	1788	1794	1801	rBV	330103	415594	61.00%	8.248%
74	12.146	1812	1814	1820	rVB2	1314	1608	0.24%	0.032%
75	12.323	1837	1843	1852	rVB	344189	441947	64.87%	8.771%
76	12.427	1858	1860	1863	rVB3	527	570	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025932.D
 Acq On : 20 Dec 2021 22:21
 Operator : JC/MD
 Sample : M5150-12DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

77	12.518	1873	1875	1878	rBV	272	301	0.04%	0.006%
78	13.579	2047	2049	2052	rBV2	233	270	0.04%	0.005%
79	13.963	2106	2112	2113	rBV2	210	308	0.05%	0.006%
80	14.018	2120	2121	2126	rVB2	320	367	0.05%	0.007%
81	14.274	2162	2163	2167	rBV2	272	335	0.05%	0.007%
82	14.463	2192	2194	2196	rBV	189	179	0.03%	0.004%
83	14.530	2202	2205	2207	rBV	263	254	0.04%	0.005%
84	14.719	2234	2236	2239	rBV	299	233	0.03%	0.005%
85	14.816	2248	2252	2256	rVB2	309	441	0.06%	0.009%
86	14.932	2268	2271	2273	rBV2	251	338	0.05%	0.007%
87	15.018	2283	2285	2290	rBV2	165	247	0.04%	0.005%
88	15.109	2298	2300	2304	rVV3	242	311	0.05%	0.006%
89	15.170	2308	2310	2312	rBV2	228	259	0.04%	0.005%
90	15.231	2319	2320	2322	rVB	333	184	0.03%	0.004%
91	15.274	2326	2327	2330	rVB	322	225	0.03%	0.004%
92	15.481	2359	2361	2365	rBV3	236	335	0.05%	0.007%
93	15.609	2380	2382	2386	rBV2	245	294	0.04%	0.006%
94	15.883	2425	2427	2429	rBV	254	196	0.03%	0.004%
95	16.152	2470	2471	2475	rBV2	318	360	0.05%	0.007%
96	16.475	2522	2524	2528	rVB2	358	305	0.04%	0.006%
97	16.511	2528	2530	2534	rBV2	270	298	0.04%	0.006%
98	16.621	2546	2548	2550	rBV	261	233	0.03%	0.005%
99	16.658	2553	2554	2558	rBV3	300	330	0.05%	0.007%
100	16.767	2570	2572	2573	rVB	328	168	0.02%	0.003%




Sum of corrected areas: 5038939

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025932.D
Acq On : 20 Dec 2021 22:21
Operator : JC/MD
Sample : M5150-12DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

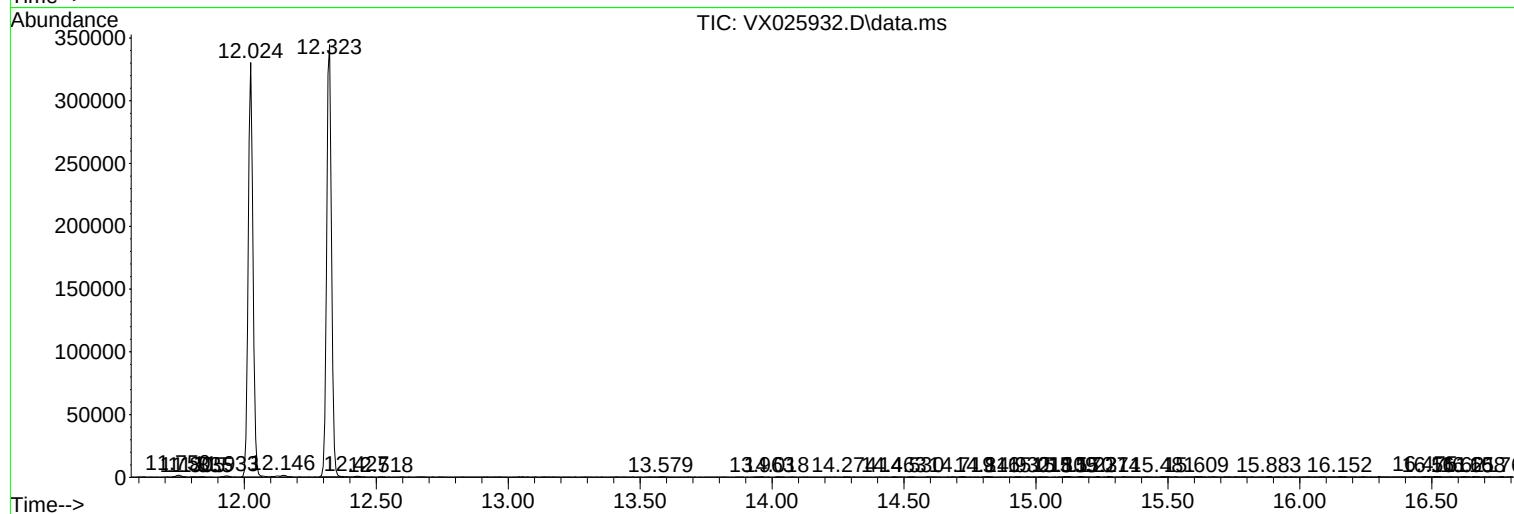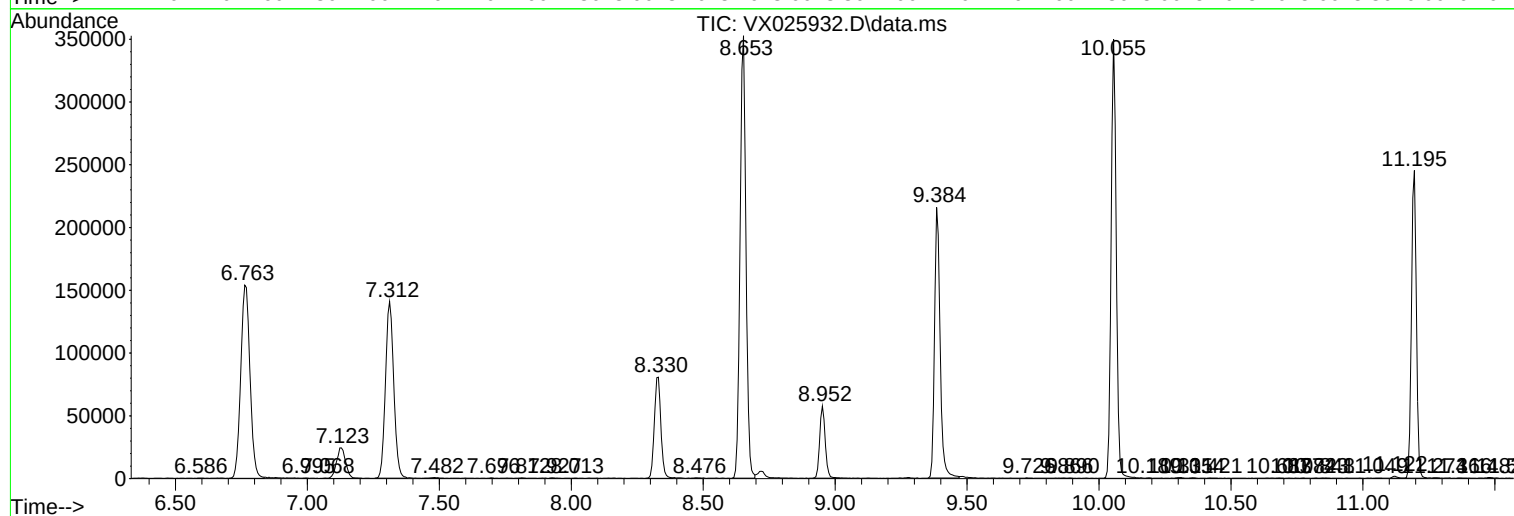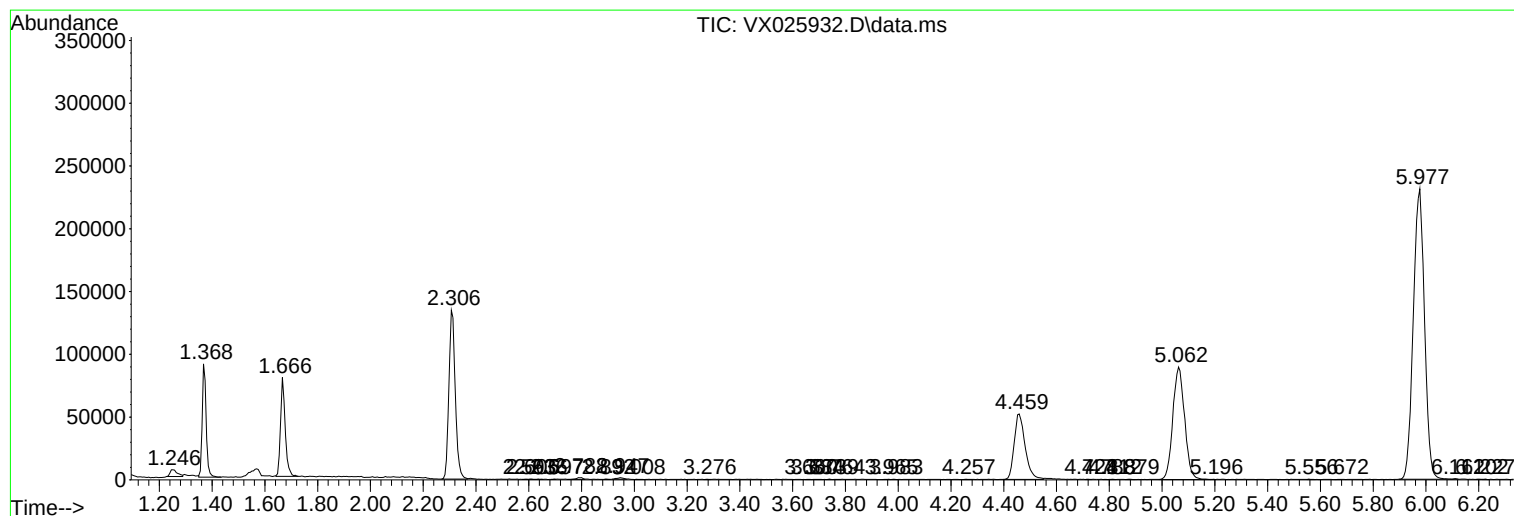

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025932.D
Acq On : 20 Dec 2021 22:21
Operator : JC/MD
Sample : M5150-12DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025932.D
Acq On : 20 Dec 2021 22:21
Operator : JC/MD
Sample : M5150-12DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc