

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025935.D
 Acq On : 20 Dec 2021 23:31
 Operator : JC/MD
 Sample : M5150-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025935.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.251	23	27	31	rBV2	4845	9103	0.17%	0.085%
2	1.367	43	46	53	rVB	93333	98015	1.84%	0.912%
3	1.666	91	95	104	rBV	84279	105602	1.98%	0.982%
4	2.306	194	200	208	rBV	143328	244270	4.57%	2.272%
5	2.379	208	212	225	rVB	14885	25652	0.48%	0.239%
6	2.507	231	233	236	rBV2	317	375	0.01%	0.003%
7	2.696	262	264	266	rBV	390	380	0.01%	0.004%
8	2.794	278	280	284	rVB2	617	632	0.01%	0.006%
9	2.836	285	287	291	rVB2	215	202	0.00%	0.002%
10	2.873	291	293	294	rBV2	249	210	0.00%	0.002%
11	3.007	313	315	318	rBV	245	229	0.00%	0.002%
12	3.342	368	370	373	rVB2	259	241	0.00%	0.002%
13	3.385	376	377	383	rVB2	204	252	0.00%	0.002%
14	3.763	436	439	440	rVB	327	251	0.00%	0.002%
15	3.909	460	463	465	rBV2	193	234	0.00%	0.002%
16	4.354	534	536	539	rVB2	211	208	0.00%	0.002%
17	4.458	543	553	573	rBV	57537	177936	3.33%	1.655%
18	4.976	636	638	640	rBV2	157	196	0.00%	0.002%
19	5.062	640	652	670	rVV	95713	298219	5.58%	2.774%
20	5.470	714	719	721	rBV5	1025	1590	0.03%	0.015%
21	5.708	754	758	760	rVB2	193	268	0.01%	0.002%
22	5.976	788	802	819	rBV2	245960	746383	13.97%	6.943%
23	6.330	858	860	863	rVB2	220	217	0.00%	0.002%
24	6.604	902	905	906	rVV	273	227	0.00%	0.002%
25	6.763	922	931	947	rVV	152026	365931	6.85%	3.404%
26	7.037	974	976	977	rBV	296	200	0.00%	0.002%
27	7.128	981	991	1007	rBV	2471687	5340944	100.00%	49.684%
28	7.311	1013	1021	1035	rVB	153573	334991	6.27%	3.116%
29	7.470	1046	1047	1049	rBV	412	305	0.01%	0.003%
30	7.756	1092	1094	1096	rVB	326	235	0.00%	0.002%
31	7.811	1096	1103	1106	rBV2	530	900	0.02%	0.008%
32	8.323	1181	1187	1197	rBV	93372	155382	2.91%	1.445%
33	8.476	1210	1212	1216	rBV3	453	595	0.01%	0.006%
34	8.579	1228	1229	1234	rVB	253	197	0.00%	0.002%
35	8.652	1234	1241	1248	rBV	382865	607001	11.37%	5.647%
36	8.951	1285	1290	1298	rBV	64454	93180	1.74%	0.867%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025935.D
 Acq On : 20 Dec 2021 23:31
 Operator : JC/MD
 Sample : M5150-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

37	9.055	1305	1307	1309	rVB2	383	256	0.00%	0.002%
38	9.079	1309	1311	1315	rVB2	354	413	0.01%	0.004%
39	9.159	1320	1324	1331	rVB2	837	956	0.02%	0.009%
40	9.219	1331	1334	1336	rBV2	190	209	0.00%	0.002%
41	9.274	1339	1343	1352	rVB2	9617	15026	0.28%	0.140%
42	9.384	1356	1361	1382	rVV	249308	360246	6.74%	3.351%
43	9.536	1385	1386	1388	rBV	392	225	0.00%	0.002%
44	9.610	1397	1398	1400	rBV	248	191	0.00%	0.002%
45	9.665	1405	1407	1410	rBV	187	266	0.00%	0.002%
46	9.750	1418	1421	1423	rBV2	194	222	0.00%	0.002%
47	9.823	1431	1433	1434	rVB	289	189	0.00%	0.002%
48	9.969	1455	1457	1461	rVB3	307	330	0.01%	0.003%
49	10.055	1465	1471	1489	rVB	354546	472403	8.84%	4.395%
50	10.262	1501	1505	1507	rVB2	207	259	0.00%	0.002%
51	10.305	1508	1512	1516	rVV4	830	1298	0.02%	0.012%
52	10.366	1521	1522	1524	rBV	313	198	0.00%	0.002%
53	10.439	1530	1534	1537	rVB2	222	297	0.01%	0.003%
54	10.646	1566	1568	1572	rVB2	447	372	0.01%	0.003%
55	10.689	1572	1575	1576	rBV	268	255	0.00%	0.002%
56	10.914	1611	1612	1616	rVB	196	239	0.00%	0.002%
57	10.975	1620	1622	1623	rVB2	313	206	0.00%	0.002%
58	11.122	1641	1646	1652	rBV4	1710	2217	0.04%	0.021%
59	11.195	1652	1658	1666	rVV	293277	356085	6.67%	3.312%
60	11.481	1698	1705	1707	rBV3	674	1084	0.02%	0.010%
61	11.542	1712	1715	1716	rBV2	176	190	0.00%	0.002%
62	11.707	1740	1742	1744	rBV	266	268	0.01%	0.002%
63	11.750	1744	1749	1754	rVB4	1322	2261	0.04%	0.021%
64	11.835	1759	1763	1768	rBV2	321	587	0.01%	0.005%
65	11.878	1768	1770	1773	rBV2	179	202	0.00%	0.002%
66	11.908	1773	1775	1777	rVB2	252	209	0.00%	0.002%
67	11.932	1777	1779	1785	rBV3	691	960	0.02%	0.009%
68	12.024	1789	1794	1802	rVV	335298	419433	7.85%	3.902%
69	12.121	1808	1810	1812	rBV3	521	646	0.01%	0.006%
70	12.152	1812	1815	1817	rVB3	1300	1413	0.03%	0.013%
71	12.225	1822	1827	1831	rBV3	614	974	0.02%	0.009%
72	12.323	1837	1843	1849	rBV	391658	490474	9.18%	4.563%
73	12.420	1858	1859	1863	rVB2	380	328	0.01%	0.003%
74	12.487	1865	1870	1874	rVB4	406	567	0.01%	0.005%
75	12.554	1880	1881	1884	rBV2	237	295	0.01%	0.003%
76	12.640	1891	1895	1897	rBV2	308	496	0.01%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025935.D
 Acq On : 20 Dec 2021 23:31
 Operator : JC/MD
 Sample : M5150-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

77	13.011	1954	1956	1960	rVB2	260	231	0.00%	0.002%
78	13.164	1980	1981	1985	rBV2	231	216	0.00%	0.002%
79	13.639	2057	2059	2062	rVV2	224	237	0.00%	0.002%
80	13.926	2104	2106	2108	rVV2	258	194	0.00%	0.002%
81	13.975	2110	2114	2117	rBV2	223	276	0.01%	0.003%
82	14.017	2120	2121	2126	rVB	250	214	0.00%	0.002%
83	14.072	2126	2130	2133	rVB	211	237	0.00%	0.002%
84	14.115	2133	2137	2139	rVB2	199	292	0.01%	0.003%
85	14.139	2139	2141	2144	rBV	309	358	0.01%	0.003%
86	14.243	2156	2158	2161	rBV2	205	194	0.00%	0.002%
87	14.456	2192	2193	2197	rBV2	149	188	0.00%	0.002%
88	14.560	2206	2210	2215	rBV2	192	351	0.01%	0.003%
89	14.798	2247	2249	2252	rBV2	216	311	0.01%	0.003%
90	14.944	2271	2273	2276	rBV2	245	232	0.00%	0.002%
91	15.121	2299	2302	2304	rBV2	263	274	0.01%	0.003%
92	15.212	2316	2317	2321	rVB2	274	222	0.00%	0.002%
93	15.334	2333	2337	2338	rBV3	296	365	0.01%	0.003%
94	15.432	2350	2353	2355	rBV2	253	358	0.01%	0.003%
95	15.493	2360	2363	2364	rBV3	312	353	0.01%	0.003%
96	15.755	2405	2406	2408	rBV2	291	197	0.00%	0.002%
97	15.791	2408	2412	2414	rVB2	200	312	0.01%	0.003%
98	16.005	2446	2447	2449	rVB	431	230	0.00%	0.002%
99	16.102	2459	2463	2464	rBV3	193	258	0.00%	0.002%
100	16.267	2488	2490	2491	rBV2	264	231	0.00%	0.002%




Sum of corrected areas: 10749829

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025935.D
Acq On : 20 Dec 2021 23:31
Operator : JC/MD
Sample : M5150-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

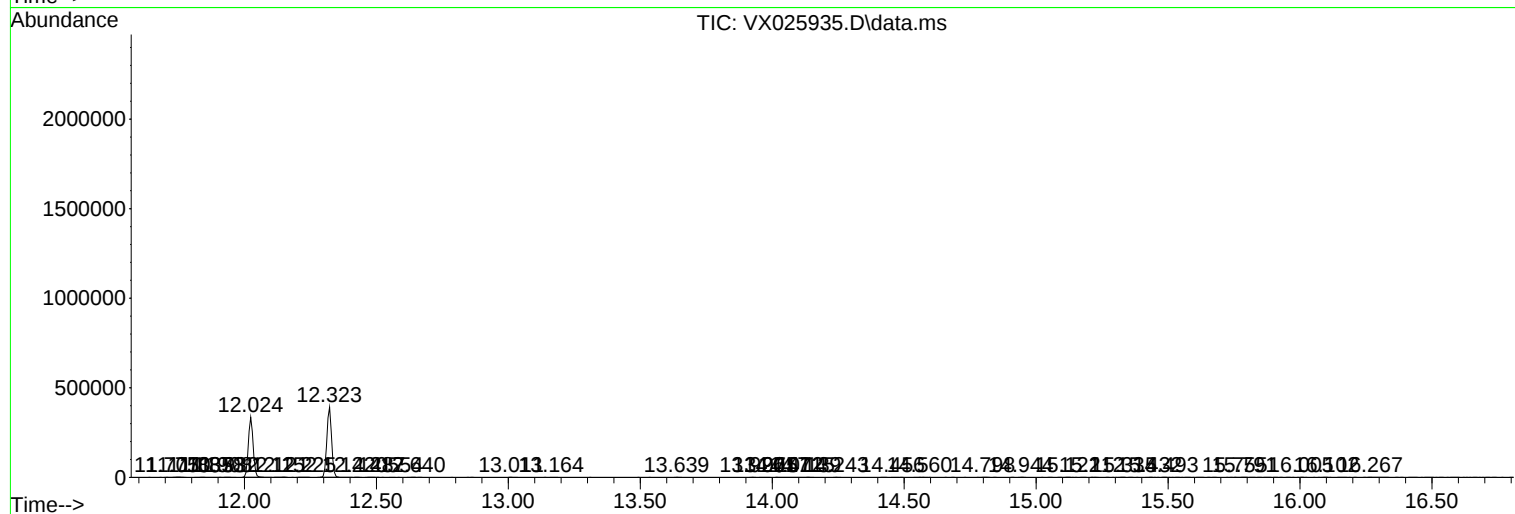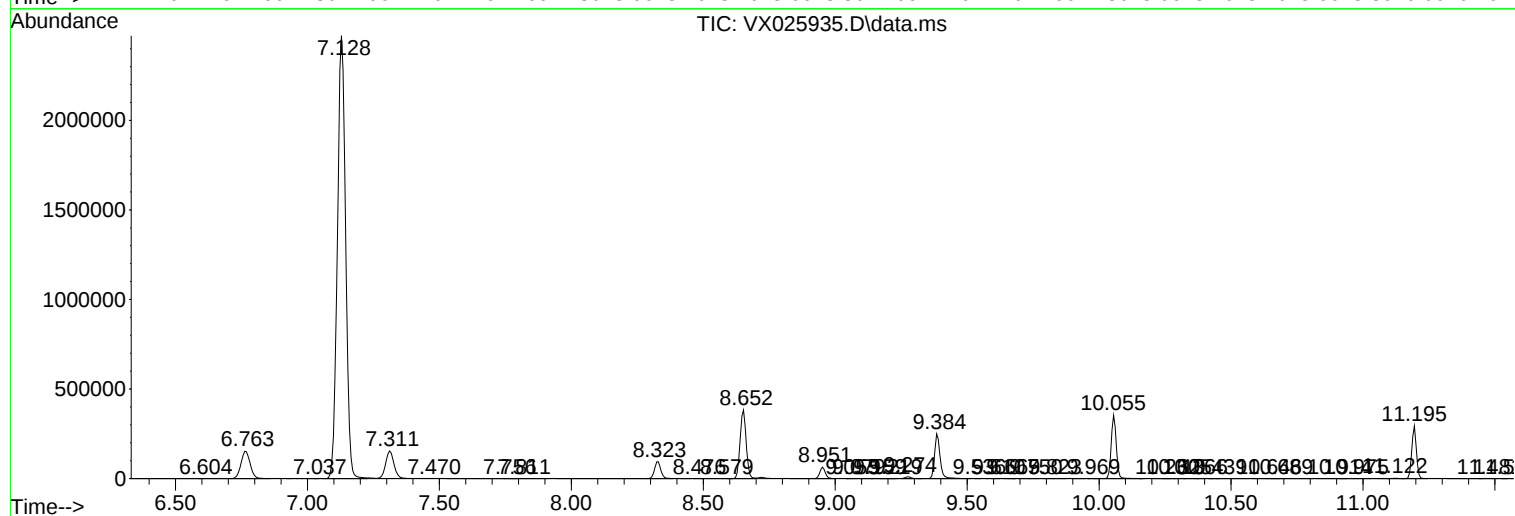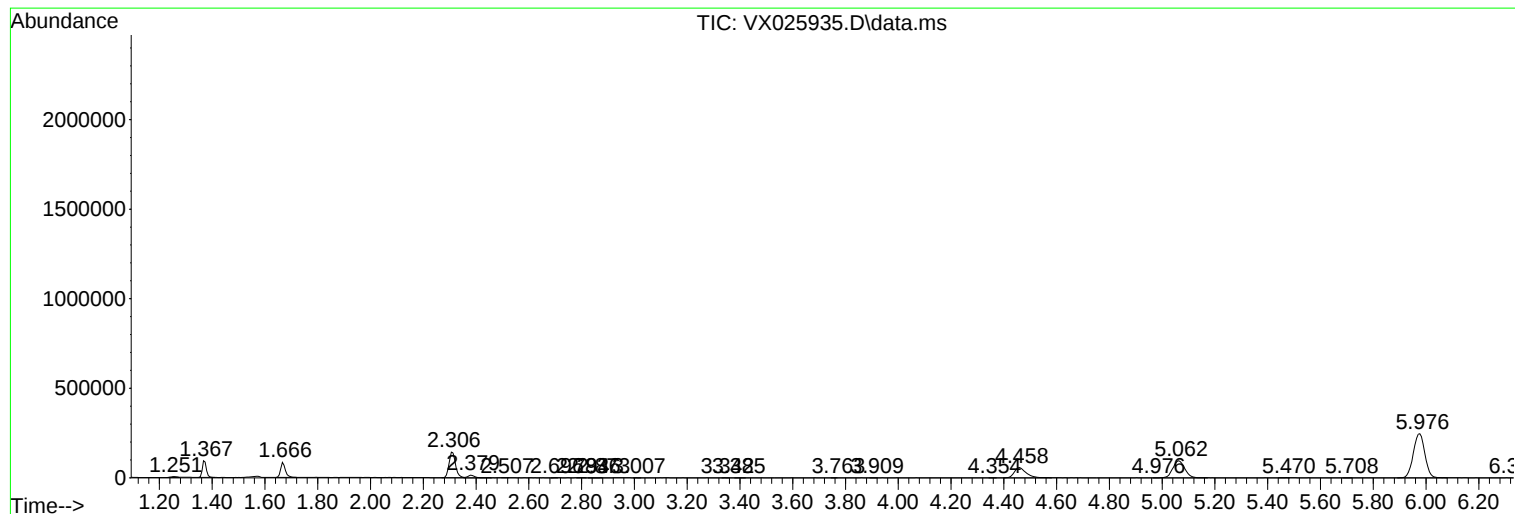

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025935.D
Acq On : 20 Dec 2021 23:31
Operator : JC/MD
Sample : M5150-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025935.D
Acq On : 20 Dec 2021 23:31
Operator : JC/MD
Sample : M5150-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc