

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025938.D
 Acq On : 21 Dec 2021 00:40
 Operator : JC/MD
 Sample : M5150-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025938.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	52	rVB	90323	93401	4.73%	1.323%
2	1.666	91	95	105	rVB	79386	98451	4.98%	1.394%
3	2.313	194	201	208	rBV	137394	229911	11.64%	3.255%
4	3.093	324	329	336	rVB4	1998	3579	0.18%	0.051%
5	3.209	347	348	350	rBV	409	184	0.01%	0.003%
6	3.532	400	401	404	rBV2	227	201	0.01%	0.003%
7	3.611	413	414	416	rBV	274	143	0.01%	0.002%
8	3.629	416	417	421	rVB2	193	155	0.01%	0.002%
9	3.660	421	422	423	rBV	119	65	0.00%	0.001%
10	3.922	463	465	468	rBV2	165	240	0.01%	0.003%
11	4.160	503	504	508	rBV2	146	167	0.01%	0.002%
12	4.330	530	532	537	rBV	343	394	0.02%	0.006%
13	4.465	541	554	556	rBV	60511	150019	7.59%	2.124%
14	4.733	597	598	599	rBV	165	91	0.00%	0.001%
15	4.782	604	606	607	rVB2	163	70	0.00%	0.001%
16	5.062	639	652	666	rBV	98206	287555	14.56%	4.072%
17	5.294	689	690	691	rBV	281	112	0.01%	0.002%
18	5.330	694	696	697	rBV	150	74	0.00%	0.001%
19	5.470	712	719	721	rBV4	1938	3971	0.20%	0.056%
20	5.623	743	744	745	rBV	114	48	0.00%	0.001%
21	5.970	789	801	817	rBV2	232466	704729	35.68%	9.979%
22	6.239	844	845	846	rVB	267	98	0.00%	0.001%
23	6.306	855	856	858	rBV2	208	143	0.01%	0.002%
24	6.324	858	859	861	rBV2	185	132	0.01%	0.002%
25	6.354	862	864	865	rBV	275	149	0.01%	0.002%
26	6.525	891	892	894	rBV	237	206	0.01%	0.003%
27	6.684	916	918	919	rBV	221	129	0.01%	0.002%
28	6.763	922	931	941	rBV	155306	369851	18.72%	5.237%
29	7.129	981	991	1009	rBV	893297	1975282	100.00%	27.969%
30	7.312	1013	1021	1036	rVB	148283	314125	15.90%	4.448%
31	7.482	1045	1049	1056	rBV2	603	1009	0.05%	0.014%
32	7.604	1068	1069	1074	rBV2	272	331	0.02%	0.005%
33	7.818	1099	1104	1105	rBV2	306	408	0.02%	0.006%
34	8.074	1144	1146	1148	rBV2	244	274	0.01%	0.004%
35	8.135	1154	1156	1159	rBV2	113	134	0.01%	0.002%
36	8.159	1159	1160	1161	rVB	242	89	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025938.D
 Acq On : 21 Dec 2021 00:40
 Operator : JC/MD
 Sample : M5150-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

37	8.183	1161	1164	1165	rBV2	216	222	0.01%	0.003%
38	8.324	1181	1187	1197	rBV	84652	142397	7.21%	2.016%
39	8.446	1205	1207	1209	rVB	254	143	0.01%	0.002%
40	8.470	1209	1211	1213	rBV3	269	322	0.02%	0.005%
41	8.568	1225	1227	1228	rBV	257	157	0.01%	0.002%
42	8.653	1234	1241	1249	rBV	348717	564643	28.59%	7.995%
43	8.952	1285	1290	1303	rVB	61857	87068	4.41%	1.233%
44	9.275	1341	1343	1346	rVB	1430	1376	0.07%	0.019%
45	9.384	1356	1361	1379	rBV	226145	337150	17.07%	4.774%
46	9.604	1396	1397	1400	rVB	365	252	0.01%	0.004%
47	9.775	1424	1425	1427	rBV	255	169	0.01%	0.002%
48	9.823	1431	1433	1436	rVV2	268	268	0.01%	0.004%
49	10.055	1465	1471	1488	rBV	344873	474980	24.05%	6.725%
50	10.226	1498	1499	1503	rBV	344	356	0.02%	0.005%
51	10.305	1508	1512	1516	rVB4	727	1003	0.05%	0.014%
52	10.518	1546	1547	1549	rBV2	214	211	0.01%	0.003%
53	10.561	1552	1554	1557	rBV	265	236	0.01%	0.003%
54	10.628	1563	1565	1566	rBV	324	171	0.01%	0.002%
55	10.848	1599	1601	1603	rBV	181	98	0.00%	0.001%
56	11.122	1643	1646	1650	rVB3	1624	2097	0.11%	0.030%
57	11.195	1652	1658	1665	rVV	267631	334599	16.94%	4.738%
58	11.445	1697	1699	1701	rBV	141	127	0.01%	0.002%
59	11.701	1739	1741	1744	rVB2	307	293	0.01%	0.004%
60	11.750	1745	1749	1753	rVB2	1677	2169	0.11%	0.031%
61	12.024	1788	1794	1806	rVB	337921	418072	21.17%	5.920%
62	12.323	1837	1843	1853	rBV	355905	454804	23.02%	6.440%
63	12.914	1937	1940	1943	rBV2	179	214	0.01%	0.003%
64	13.085	1966	1968	1969	rBV	185	136	0.01%	0.002%
65	13.554	2043	2045	2047	rBV2	218	163	0.01%	0.002%
66	13.615	2052	2055	2057	rBV	233	205	0.01%	0.003%
67	13.737	2074	2075	2076	rBV	180	68	0.00%	0.001%
68	13.847	2090	2093	2094	rBV2	215	199	0.01%	0.003%
69	13.908	2102	2103	2104	rBV	212	89	0.00%	0.001%
70	14.042	2124	2125	2131	rBV2	153	229	0.01%	0.003%
71	14.103	2133	2135	2138	rBV2	130	144	0.01%	0.002%
72	14.499	2198	2200	2203	rBV	223	226	0.01%	0.003%
73	14.560	2209	2210	2212	rBV2	218	196	0.01%	0.003%
74	14.859	2258	2259	2261	rBV	224	143	0.01%	0.002%
75	14.963	2275	2276	2279	rBV	309	198	0.01%	0.003%
76	15.018	2284	2285	2287	rBV	372	225	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025938.D
Acq On : 21 Dec 2021 00:40
Operator : JC/MD
Sample : M5150-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Title : VOC Analysis

77	15.548	2370	2372	2374	rBV	358	281	0.01%	0.004%
78	15.664	2389	2391	2393	rBV2	281	214	0.01%	0.003%
79	16.078	2457	2459	2460	rBV	331	159	0.01%	0.002%




Sum of corrected areas: 7062392

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025938.D
Acq On : 21 Dec 2021 00:40
Operator : JC/MD
Sample : M5150-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

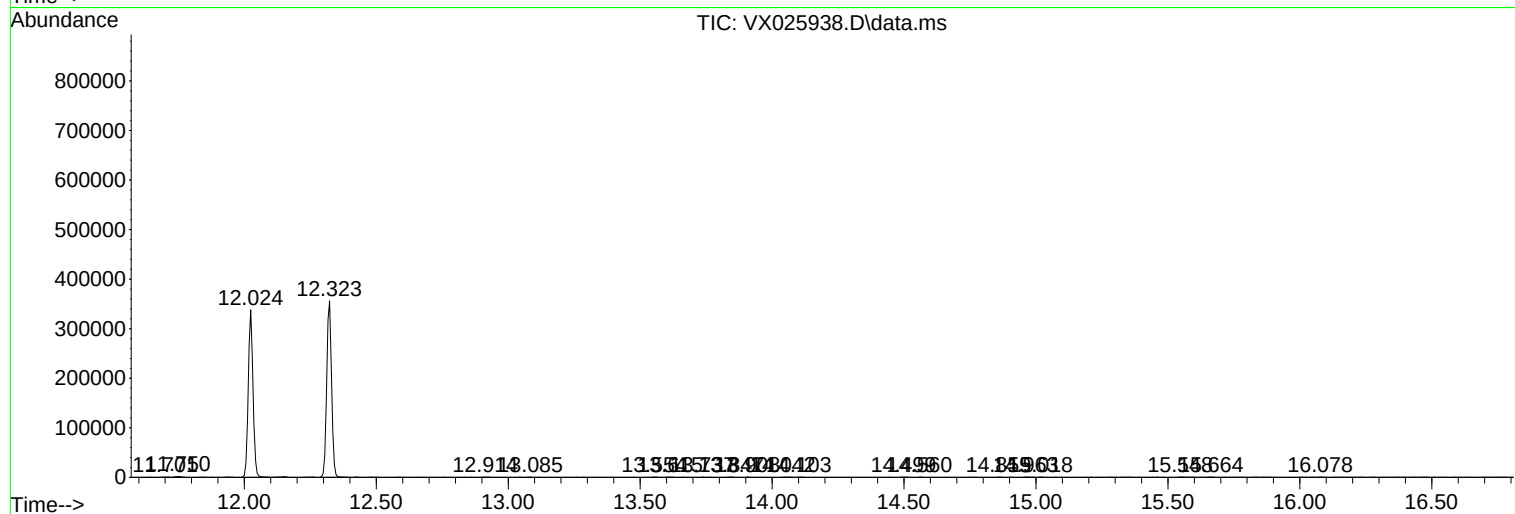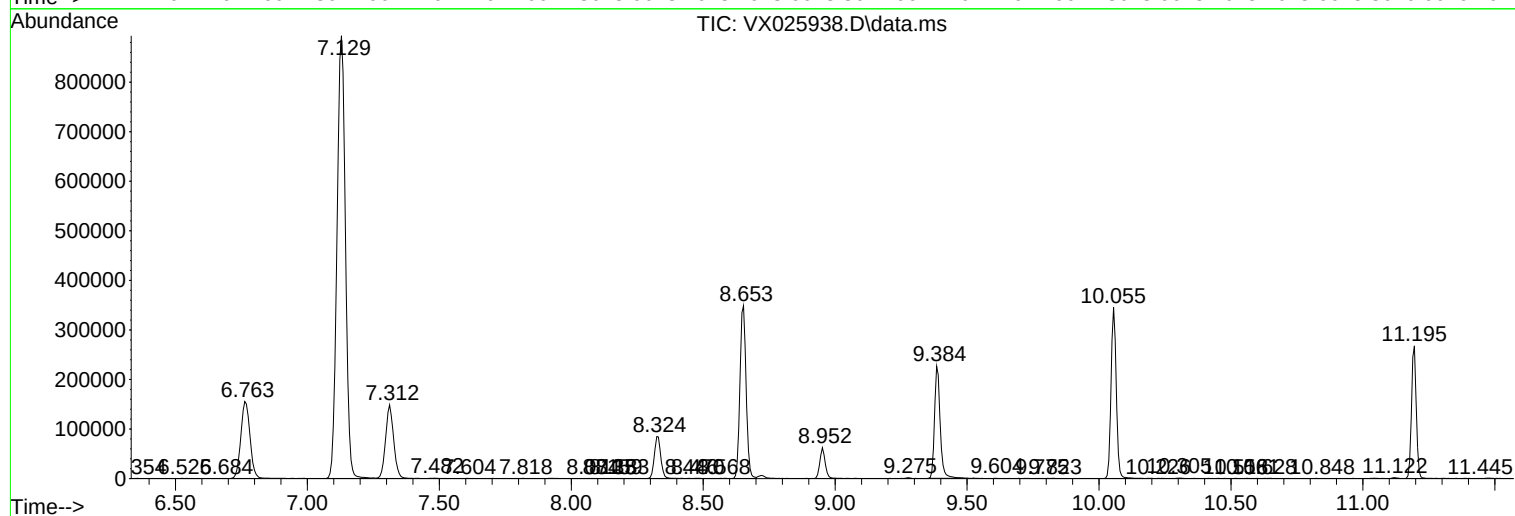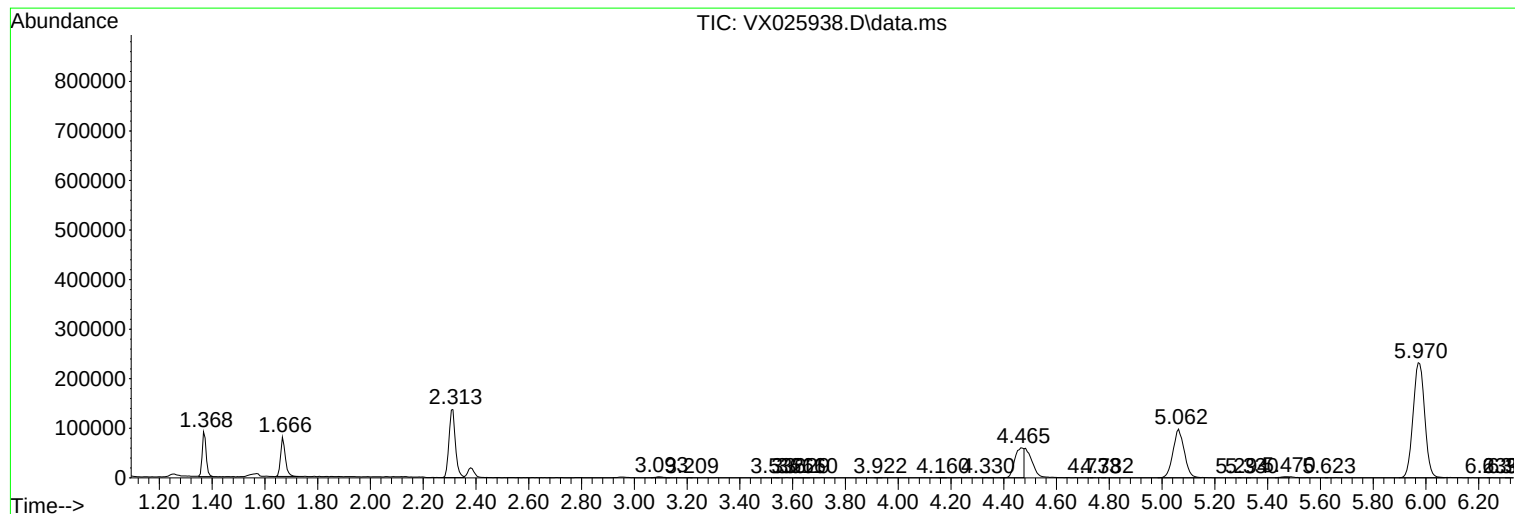

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025938.D
Acq On : 21 Dec 2021 00:40
Operator : JC/MD
Sample : M5150-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025938.D
Acq On : 21 Dec 2021 00:40
Operator : JC/MD
Sample : M5150-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc