

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025939.D
 Acq On : 21 Dec 2021 01:04
 Operator : JC/MD
 Sample : M5150-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025939.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	33	rBV	5508	10733	0.55%	0.152%
2	1.368	43	46	55	rVB	89719	94896	4.82%	1.343%
3	1.666	91	95	106	rBV	77986	100618	5.12%	1.424%
4	2.306	194	200	208	rBV	134184	221323	11.25%	3.133%
5	2.380	208	212	224	rVB	19689	32502	1.65%	0.460%
6	2.508	230	233	234	rBV2	281	283	0.01%	0.004%
7	2.794	278	280	284	rVB3	466	430	0.02%	0.006%
8	2.947	299	305	308	rBV4	1309	2623	0.13%	0.037%
9	3.020	314	317	320	rBV3	269	448	0.02%	0.006%
10	3.099	325	330	336	rBV4	1929	3818	0.19%	0.054%
11	3.434	383	385	388	rVB2	218	192	0.01%	0.003%
12	3.526	398	400	402	rBV2	251	235	0.01%	0.003%
13	3.568	405	407	409	rBV2	325	291	0.01%	0.004%
14	3.635	415	418	420	rVB2	203	251	0.01%	0.004%
15	3.861	453	455	457	rBV2	270	252	0.01%	0.004%
16	3.946	465	469	471	rVB2	202	237	0.01%	0.003%
17	4.135	498	500	503	rBV2	196	230	0.01%	0.003%
18	4.196	508	510	513	rBV2	138	187	0.01%	0.003%
19	4.318	528	530	533	rBV2	259	245	0.01%	0.003%
20	4.465	544	554	556	rBV	59792	145916	7.42%	2.065%
21	4.751	600	601	604	rVB2	231	195	0.01%	0.003%
22	4.800	604	609	610	rBV2	147	236	0.01%	0.003%
23	4.879	618	622	625	rBV	201	222	0.01%	0.003%
24	5.062	640	652	668	rBV	90566	279635	14.22%	3.958%
25	5.477	712	720	729	rVB3	2725	8158	0.41%	0.115%
26	5.684	751	754	756	rBV2	184	222	0.01%	0.003%
27	5.970	788	801	818	rBV3	229470	693379	35.25%	9.815%
28	6.275	848	851	853	rBV2	184	204	0.01%	0.003%
29	6.318	857	858	860	rBV	333	200	0.01%	0.003%
30	6.446	878	879	882	rBV	260	191	0.01%	0.003%
31	6.556	895	897	900	rVB	295	217	0.01%	0.003%
32	6.763	921	931	943	rBV	157905	373370	18.98%	5.285%
33	6.934	957	959	961	rVV	443	285	0.01%	0.004%
34	7.129	980	991	1009	rBV	908056	1966802	100.00%	27.841%
35	7.312	1013	1021	1032	rVB	138178	309720	15.75%	4.384%
36	7.434	1039	1041	1044	rVB	231	251	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025939.D
 Acq On : 21 Dec 2021 01:04
 Operator : JC/MD
 Sample : M5150-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

37	7.476	1044	1048	1050	rBV2	521	759	0.04%	0.011%
38	7.592	1064	1067	1068	rBV	187	208	0.01%	0.003%
39	7.702	1080	1085	1088	rBV2	247	424	0.02%	0.006%
40	7.751	1092	1093	1096	rVB2	259	223	0.01%	0.003%
41	7.909	1116	1119	1120	rBV	223	237	0.01%	0.003%
42	7.964	1125	1128	1131	rVV	262	354	0.02%	0.005%
43	8.330	1181	1188	1197	rBV	82614	140878	7.16%	1.994%
44	8.421	1201	1203	1208	rVB2	340	585	0.03%	0.008%
45	8.470	1208	1211	1215	rBV3	527	728	0.04%	0.010%
46	8.653	1234	1241	1249	rBV	350656	557616	28.35%	7.893%
47	8.775	1259	1261	1262	rVB	497	268	0.01%	0.004%
48	8.878	1277	1278	1282	rVB2	171	210	0.01%	0.003%
49	8.952	1284	1290	1299	rVV	57013	83068	4.22%	1.176%
50	9.147	1319	1322	1323	rBV	184	215	0.01%	0.003%
51	9.220	1333	1334	1337	rBV2	194	222	0.01%	0.003%
52	9.275	1340	1343	1348	rVB2	1104	1445	0.07%	0.020%
53	9.384	1356	1361	1376	rBV	221808	329925	16.77%	4.670%
54	9.537	1384	1386	1387	rVB2	354	185	0.01%	0.003%
55	9.775	1422	1425	1426	rBV2	238	246	0.01%	0.003%
56	9.866	1438	1440	1445	rVV2	193	303	0.02%	0.004%
57	10.055	1465	1471	1492	rBV	359324	479401	24.37%	6.786%
58	10.299	1507	1511	1516	rVV4	734	1359	0.07%	0.019%
59	10.342	1516	1518	1521	rVV2	223	249	0.01%	0.004%
60	10.482	1539	1541	1543	rVB	309	188	0.01%	0.003%
61	10.506	1543	1545	1546	rBV	269	206	0.01%	0.003%
62	10.646	1565	1568	1571	rBV	432	429	0.02%	0.006%
63	10.781	1588	1590	1594	rBV2	261	352	0.02%	0.005%
64	10.835	1595	1599	1600	rBV2	185	256	0.01%	0.004%
65	10.970	1618	1621	1622	rVB	261	234	0.01%	0.003%
66	11.049	1629	1634	1636	rBV4	470	715	0.04%	0.010%
67	11.122	1642	1646	1649	rVB3	1426	1760	0.09%	0.025%
68	11.195	1652	1658	1667	rVV	250286	324256	16.49%	4.590%
69	11.305	1675	1676	1679	rVB2	397	401	0.02%	0.006%
70	11.335	1679	1681	1685	rVB2	204	197	0.01%	0.003%
71	11.750	1746	1749	1754	rVV2	1692	2119	0.11%	0.030%
72	11.811	1756	1759	1761	rBV2	216	275	0.01%	0.004%
73	11.841	1761	1764	1766	rVB3	287	307	0.02%	0.004%
74	11.939	1775	1780	1782	rBV3	517	768	0.04%	0.011%
75	12.024	1789	1794	1803	rVB	333741	427263	21.72%	6.048%
76	12.134	1806	1812	1813	rBV3	719	1157	0.06%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025939.D
 Acq On : 21 Dec 2021 01:04
 Operator : JC/MD
 Sample : M5150-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

77	12.152	1813	1815	1818	rVB	956	900	0.05%	0.013%
78	12.262	1827	1833	1835	rBV2	429	646	0.03%	0.009%
79	12.323	1837	1843	1850	rBV	345191	448519	22.80%	6.349%
80	12.427	1857	1860	1863	rVB3	439	555	0.03%	0.008%
81	12.670	1897	1900	1901	rBV2	443	399	0.02%	0.006%
82	12.866	1930	1932	1935	rBV2	175	178	0.01%	0.003%
83	13.055	1961	1963	1965	rVV	196	196	0.01%	0.003%
84	13.207	1986	1988	1991	rBV	285	290	0.01%	0.004%
85	13.237	1991	1993	1996	rBV	146	181	0.01%	0.003%
86	14.323	2170	2171	2174	rBV	239	287	0.01%	0.004%
87	14.518	2202	2203	2206	rBV2	208	205	0.01%	0.003%
88	14.627	2219	2221	2224	rVB2	286	318	0.02%	0.005%
89	14.987	2278	2280	2282	rVB	285	196	0.01%	0.003%
90	15.048	2289	2290	2292	rBV2	228	203	0.01%	0.003%
91	15.133	2302	2304	2306	rBV	233	243	0.01%	0.003%
92	15.475	2358	2360	2364	rVB	312	327	0.02%	0.005%
93	15.524	2367	2368	2370	rBV	346	217	0.01%	0.003%
94	15.609	2380	2382	2384	rVV3	256	219	0.01%	0.003%
95	15.713	2397	2399	2401	rBV2	219	210	0.01%	0.003%
96	15.914	2431	2432	2435	rVB3	279	230	0.01%	0.003%
97	16.042	2451	2453	2455	rBV2	349	259	0.01%	0.004%
98	16.255	2487	2488	2491	rBV2	310	249	0.01%	0.004%
99	16.530	2531	2533	2536	rBV2	184	191	0.01%	0.003%
100	16.779	2571	2574	2575	rBV2	239	255	0.01%	0.004%




Sum of corrected areas: 7064461

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025939.D
Acq On : 21 Dec 2021 01:04
Operator : JC/MD
Sample : M5150-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

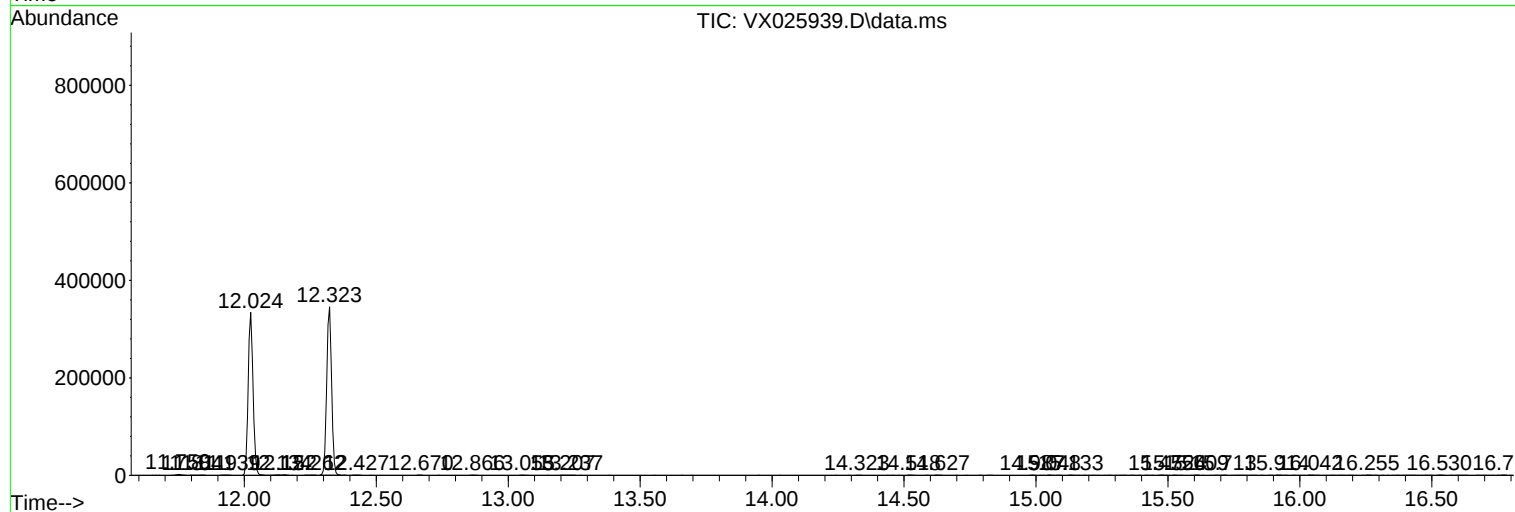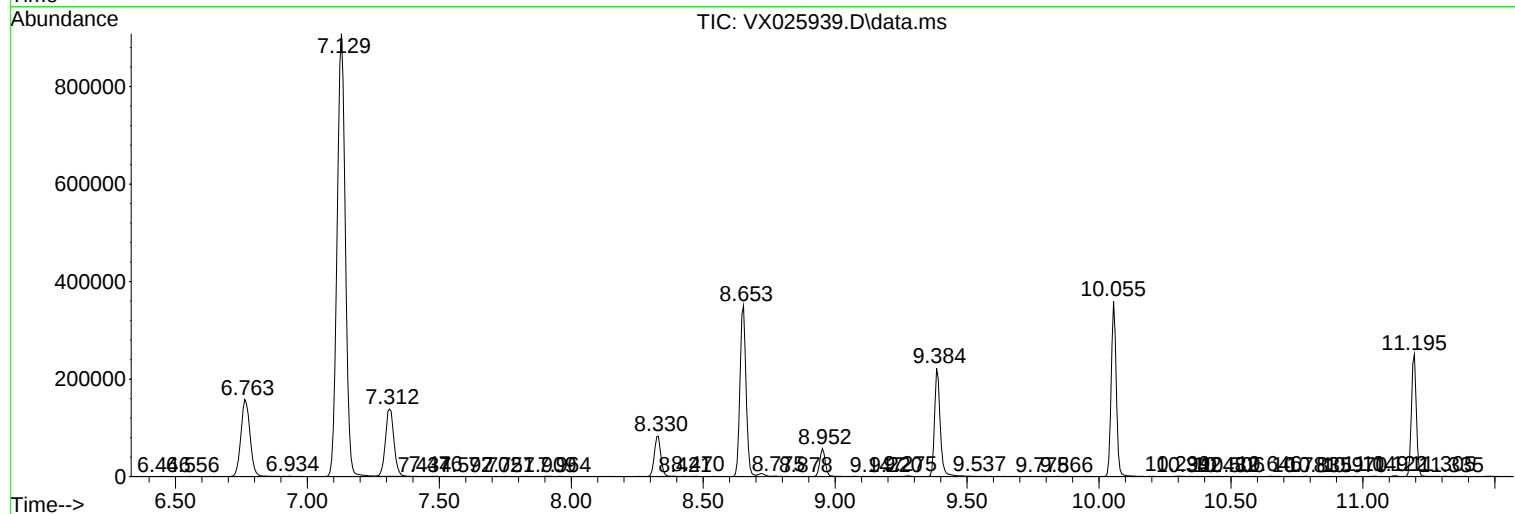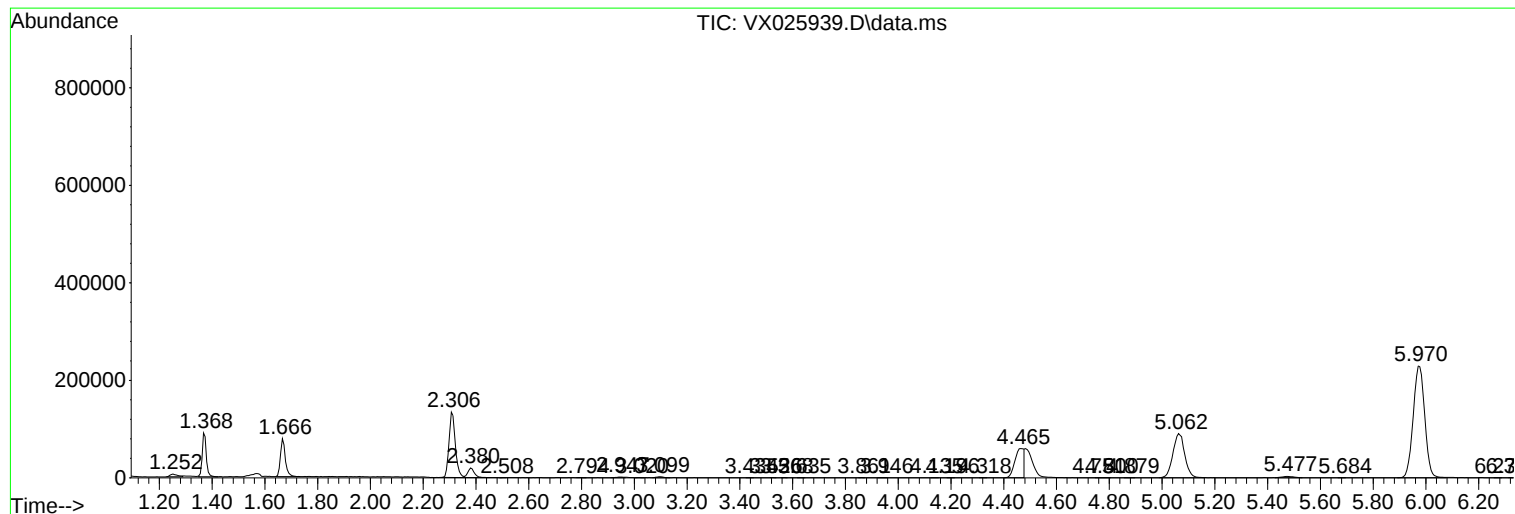

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025939.D
Acq On : 21 Dec 2021 01:04
Operator : JC/MD
Sample : M5150-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025939.D
Acq On : 21 Dec 2021 01:04
Operator : JC/MD
Sample : M5150-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc