

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025940.D
 Acq On : 21 Dec 2021 01:27
 Operator : JC/MD
 Sample : M5150-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025940.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	33	rBV	4933	10040	0.18%	0.094%
2	1.368	43	46	53	rVB	87830	91959	1.68%	0.864%
3	1.666	91	95	106	rVB	71091	93061	1.70%	0.874%
4	2.306	194	200	208	rBV	132924	227340	4.15%	2.135%
5	2.380	208	212	220	rVB	9922	16674	0.30%	0.157%
6	2.703	263	265	268	rBV2	255	294	0.01%	0.003%
7	2.782	276	278	279	rBV	432	296	0.01%	0.003%
8	2.825	283	285	288	rVB2	305	217	0.00%	0.002%
9	2.959	300	307	312	rBV4	1114	2751	0.05%	0.026%
10	3.099	323	330	338	rVV2	2908	5682	0.10%	0.053%
11	4.111	493	496	499	rBV2	239	372	0.01%	0.003%
12	4.227	512	515	516	rBV2	211	247	0.00%	0.002%
13	4.458	544	553	570	rVV2	57066	228782	4.18%	2.148%
14	4.757	601	602	607	rBV2	199	216	0.00%	0.002%
15	4.849	614	617	620	rBV	197	201	0.00%	0.002%
16	4.946	629	633	635	rBV2	204	302	0.01%	0.003%
17	5.056	638	651	666	rBV	91417	279893	5.11%	2.628%
18	5.477	710	720	727	rVV6	2541	7931	0.14%	0.074%
19	5.556	730	733	736	rBV3	228	359	0.01%	0.003%
20	5.617	741	743	746	rBV2	281	260	0.00%	0.002%
21	5.659	748	750	753	rVV2	185	211	0.00%	0.002%
22	5.690	753	755	760	rVB2	272	244	0.00%	0.002%
23	5.751	763	765	769	rBV2	171	201	0.00%	0.002%
24	5.848	778	781	782	rBV2	235	198	0.00%	0.002%
25	5.970	788	801	816	rBV2	227211	688164	12.58%	6.462%
26	6.275	849	851	853	rVB	286	232	0.00%	0.002%
27	6.763	922	931	945	rBV	156982	377575	6.90%	3.546%
28	6.897	951	953	958	rVB	343	249	0.00%	0.002%
29	7.025	971	974	978	rBV2	202	236	0.00%	0.002%
30	7.129	981	991	1012	rBV	2551040	5472235	100.00%	51.387%
31	7.312	1013	1021	1038	rVB2	137765	309580	5.66%	2.907%
32	7.549	1059	1060	1064	rBV	214	209	0.00%	0.002%
33	7.629	1071	1073	1075	rVB2	275	221	0.00%	0.002%
34	7.763	1091	1095	1096	rVB2	230	224	0.00%	0.002%
35	7.805	1100	1102	1104	rVV	319	329	0.01%	0.003%
36	7.854	1108	1110	1113	rVV2	235	280	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025940.D
 Acq On : 21 Dec 2021 01:27
 Operator : JC/MD
 Sample : M5150-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

37	7.891	1114	1116	1118	rVV2	276	278	0.01%	0.003%
38	7.927	1121	1122	1125	rVV2	371	388	0.01%	0.004%
39	7.964	1126	1128	1130	rVB	364	262	0.00%	0.002%
40	7.994	1130	1133	1134	rBV2	265	268	0.00%	0.003%
41	8.330	1181	1188	1198	rVV	84438	140853	2.57%	1.323%
42	8.525	1219	1220	1224	rBV	316	297	0.01%	0.003%
43	8.653	1234	1241	1249	rBV	349825	554943	10.14%	5.211%
44	8.952	1284	1290	1299	rBV	58680	84128	1.54%	0.790%
45	9.037	1303	1304	1310	rVB2	429	398	0.01%	0.004%
46	9.153	1321	1323	1327	rBV3	637	812	0.01%	0.008%
47	9.275	1339	1343	1348	rVB3	5119	7598	0.14%	0.071%
48	9.384	1355	1361	1381	rBV	220302	330166	6.03%	3.100%
49	9.787	1425	1427	1430	rVB2	203	200	0.00%	0.002%
50	9.823	1430	1433	1435	rVB2	327	394	0.01%	0.004%
51	9.951	1451	1454	1456	rBV2	195	225	0.00%	0.002%
52	10.006	1461	1463	1465	rVB2	265	196	0.00%	0.002%
53	10.055	1465	1471	1487	rBV	360575	488470	8.93%	4.587%
54	10.183	1491	1492	1493	rBV	324	195	0.00%	0.002%
55	10.274	1505	1507	1508	rBV	272	197	0.00%	0.002%
56	10.305	1509	1512	1516	rVB2	678	976	0.02%	0.009%
57	10.342	1516	1518	1521	rBV2	174	199	0.00%	0.002%
58	10.549	1550	1552	1555	rBV	278	257	0.00%	0.002%
59	10.616	1559	1563	1564	rVB2	312	285	0.01%	0.003%
60	10.646	1564	1568	1570	rVB2	321	345	0.01%	0.003%
61	11.018	1624	1629	1630	rBV2	302	349	0.01%	0.003%
62	11.116	1642	1645	1650	rVB4	1458	2340	0.04%	0.022%
63	11.195	1652	1658	1666	rVV	248834	324248	5.93%	3.045%
64	11.280	1670	1672	1675	rBV2	575	526	0.01%	0.005%
65	11.451	1698	1700	1702	rVV	352	279	0.01%	0.003%
66	11.475	1702	1704	1707	rBV3	481	660	0.01%	0.006%
67	11.543	1712	1715	1717	rBV2	182	238	0.00%	0.002%
68	11.671	1733	1736	1738	rBV	220	263	0.00%	0.002%
69	11.750	1745	1749	1755	rVB4	1512	2055	0.04%	0.019%
70	11.841	1762	1764	1766	rBV3	195	238	0.00%	0.002%
71	11.933	1776	1779	1783	rBV3	728	901	0.02%	0.008%
72	12.024	1788	1794	1805	rBV	350450	432728	7.91%	4.064%
73	12.122	1807	1810	1812	rBV3	544	681	0.01%	0.006%
74	12.268	1831	1834	1836	rBV	240	222	0.00%	0.002%
75	12.323	1837	1843	1850	rVV	345599	446433	8.16%	4.192%
76	12.427	1858	1860	1862	rVB	528	402	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025940.D
 Acq On : 21 Dec 2021 01:27
 Operator : JC/MD
 Sample : M5150-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

77	12.658	1895	1898	1900	rBV3	284	341	0.01%	0.003%
78	12.780	1915	1918	1924	rBV2	255	438	0.01%	0.004%
79	12.872	1932	1933	1939	rVB3	340	475	0.01%	0.004%
80	13.621	2054	2056	2059	rBV2	221	258	0.00%	0.002%
81	13.780	2079	2082	2086	rVB2	265	365	0.01%	0.003%
82	14.054	2124	2127	2131	rVB2	188	292	0.01%	0.003%
83	14.121	2137	2138	2141	rVV	286	221	0.00%	0.002%
84	14.146	2141	2142	2147	rVV2	223	282	0.01%	0.003%
85	14.274	2161	2163	2169	rVV2	132	196	0.00%	0.002%
86	14.548	2206	2208	2212	rBV2	176	242	0.00%	0.002%
87	14.707	2231	2234	2236	rBV2	280	259	0.00%	0.002%
88	14.761	2241	2243	2246	rVB2	267	216	0.00%	0.002%
89	14.822	2250	2253	2256	rVB3	336	429	0.01%	0.004%
90	14.865	2258	2260	2263	rBV2	195	199	0.00%	0.002%
91	14.944	2271	2273	2276	rVB2	206	203	0.00%	0.002%
92	14.975	2276	2278	2279	rBV	267	238	0.00%	0.002%
93	15.225	2317	2319	2321	rBV2	276	216	0.00%	0.002%
94	15.359	2339	2341	2344	rVB2	207	195	0.00%	0.002%
95	15.755	2404	2406	2410	rBV2	258	457	0.01%	0.004%
96	16.017	2446	2449	2452	rBV2	274	368	0.01%	0.003%
97	16.151	2470	2471	2474	rBV2	230	210	0.00%	0.002%
98	16.188	2474	2477	2479	rBV2	246	336	0.01%	0.003%
99	16.255	2486	2488	2490	rVB2	311	196	0.00%	0.002%
100	16.279	2490	2492	2494	rBV3	237	256	0.00%	0.002%




Sum of corrected areas: 10649046

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025940.D
Acq On : 21 Dec 2021 01:27
Operator : JC/MD
Sample : M5150-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

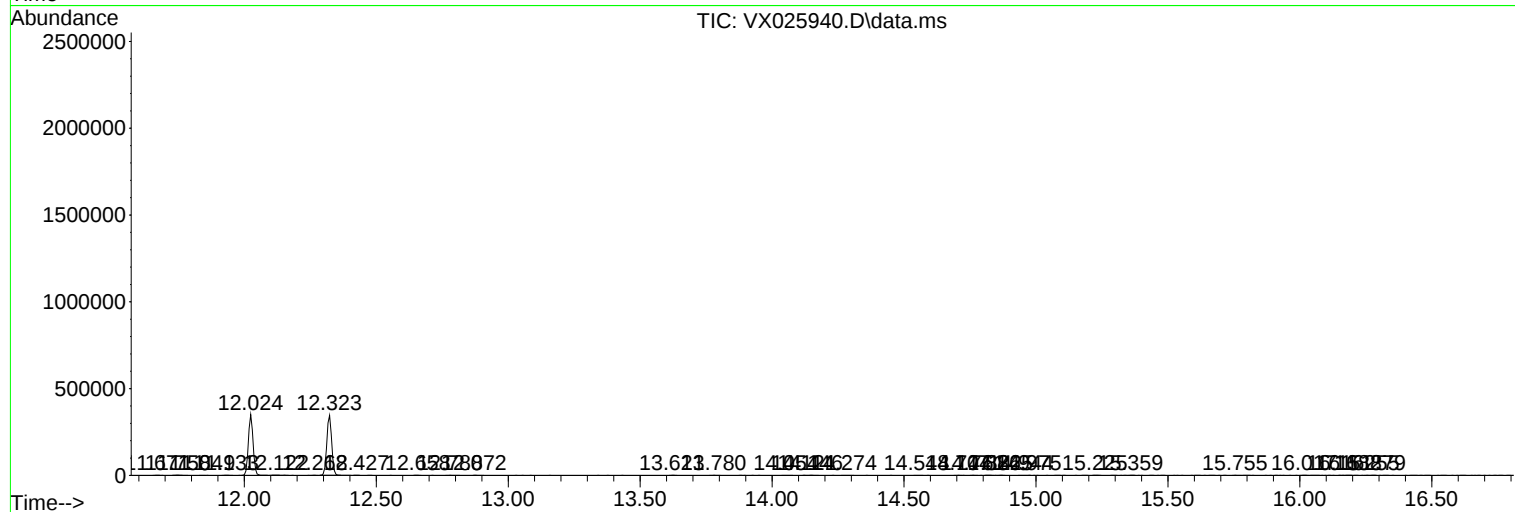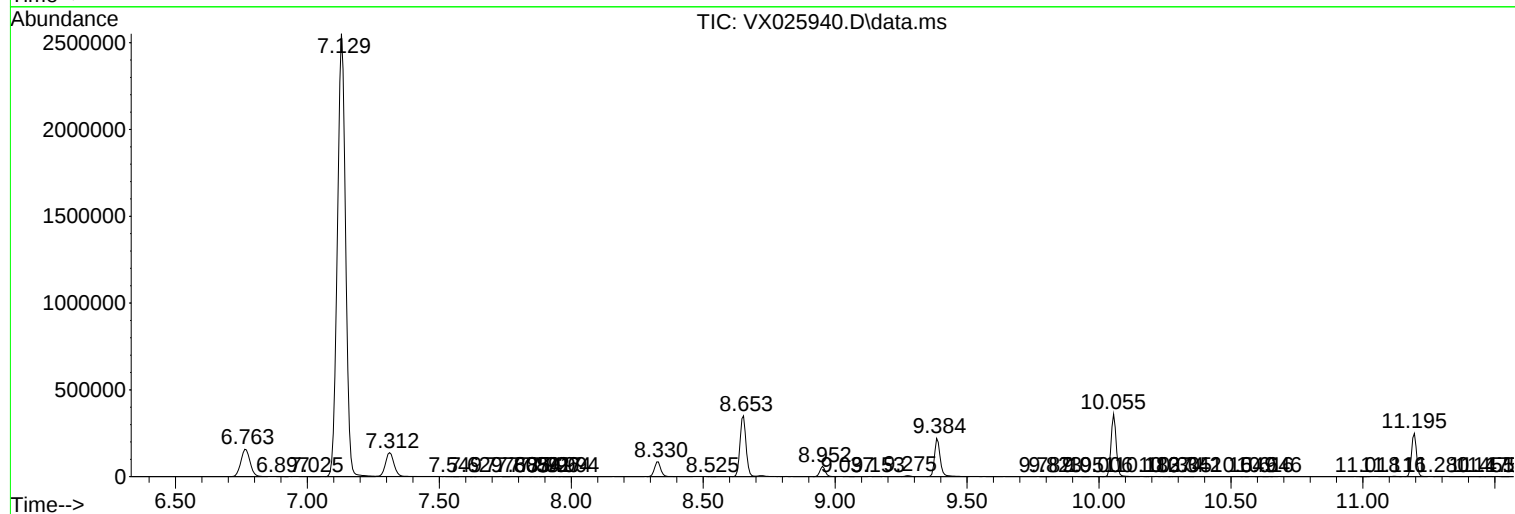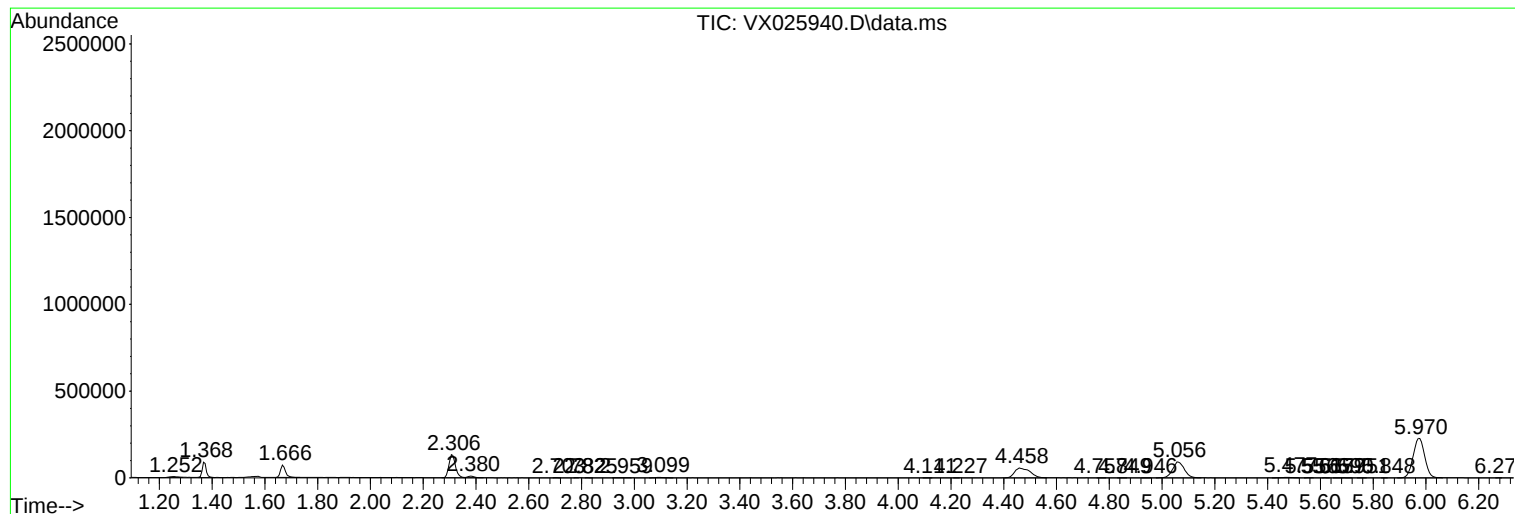

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025940.D
Acq On : 21 Dec 2021 01:27
Operator : JC/MD
Sample : M5150-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025940.D
Acq On : 21 Dec 2021 01:27
Operator : JC/MD
Sample : M5150-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------