

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025941.D
 Acq On : 21 Dec 2021 01:50
 Operator : JC/MD
 Sample : M5126-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025941.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	57	rVB	88388	92868	13.54%	1.849%
2	1.666	91	95	105	rBV	76776	95816	13.97%	1.908%
3	2.306	194	200	209	rBV	131102	215911	31.48%	4.299%
4	2.508	230	233	235	rBV2	310	453	0.07%	0.009%
5	2.703	263	265	266	rBV	364	177	0.03%	0.004%
6	2.788	276	279	283	rBV2	550	667	0.10%	0.013%
7	2.947	300	305	309	rVV2	922	2047	0.30%	0.041%
8	3.105	327	331	333	rVB2	264	322	0.05%	0.006%
9	3.142	333	337	338	rBV2	238	254	0.04%	0.005%
10	3.270	356	358	360	rBV2	276	243	0.04%	0.005%
11	3.507	394	397	400	rBV	237	391	0.06%	0.008%
12	3.751	435	437	439	rBV	165	169	0.02%	0.003%
13	3.855	450	454	455	rBV2	165	187	0.03%	0.004%
14	4.038	482	484	487	rVV	143	201	0.03%	0.004%
15	4.087	489	492	495	rBV2	252	267	0.04%	0.005%
16	4.221	512	514	518	rBV2	179	248	0.04%	0.005%
17	4.324	529	531	534	rVB2	240	188	0.03%	0.004%
18	4.458	542	553	567	rBV2	50818	151517	22.09%	3.017%
19	4.708	592	594	596	rVB2	294	180	0.03%	0.004%
20	4.757	599	602	603	rBV	263	229	0.03%	0.005%
21	4.855	616	618	621	rVB2	227	181	0.03%	0.004%
22	5.068	639	653	667	rBV	92802	277469	40.45%	5.525%
23	5.300	689	691	694	rVV2	191	170	0.02%	0.003%
24	5.385	698	705	714	rVB6	1664	4106	0.60%	0.082%
25	5.544	730	731	735	rVB2	245	240	0.03%	0.005%
26	5.605	739	741	744	rBV	221	196	0.03%	0.004%
27	5.970	789	801	816	rBV2	226882	685940	100.00%	13.659%
28	6.153	830	831	834	rVB	291	201	0.03%	0.004%
29	6.208	836	840	842	rBV	228	316	0.05%	0.006%
30	6.367	864	866	870	rVB	176	217	0.03%	0.004%
31	6.671	913	916	919	rBV	289	389	0.06%	0.008%
32	6.763	922	931	947	rBV	152618	365200	53.24%	7.272%
33	6.915	954	956	958	rVB3	286	173	0.03%	0.003%
34	7.129	982	991	1000	rVV5	23030	52922	7.72%	1.054%
35	7.312	1012	1021	1034	rBV	141801	309989	45.19%	6.173%
36	7.464	1045	1046	1048	rBV2	316	287	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025941.D
 Acq On : 21 Dec 2021 01:50
 Operator : JC/MD
 Sample : M5126-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

37	7.708	1084	1086	1089	rBV2	232	252	0.04%	0.005%
38	7.799	1099	1101	1104	rBV2	175	211	0.03%	0.004%
39	7.933	1120	1123	1126	rBV3	266	318	0.05%	0.006%
40	8.129	1153	1155	1160	rVV2	190	227	0.03%	0.005%
41	8.324	1181	1187	1199	rBV	82370	136972	19.97%	2.727%
42	8.421	1201	1203	1205	rVB	220	177	0.03%	0.004%
43	8.604	1230	1233	1234	rBV2	219	238	0.03%	0.005%
44	8.653	1234	1241	1248	rBV	339165	543865	79.29%	10.830%
45	8.842	1270	1272	1277	rBV2	312	378	0.06%	0.008%
46	8.952	1284	1290	1299	rBV	56692	82189	11.98%	1.637%
47	9.092	1311	1313	1316	rBV2	169	194	0.03%	0.004%
48	9.116	1316	1317	1322	rVV2	160	243	0.04%	0.005%
49	9.275	1338	1343	1350	rBV2	15606	23478	3.42%	0.468%
50	9.384	1356	1361	1381	rBV	217382	322606	47.03%	6.424%
51	9.683	1407	1410	1413	rBV2	227	308	0.04%	0.006%
52	9.860	1436	1439	1443	rVB2	233	450	0.07%	0.009%
53	9.903	1443	1446	1448	rBV	344	309	0.05%	0.006%
54	10.055	1465	1471	1485	rBV	344099	460915	67.19%	9.178%
55	10.195	1492	1494	1498	rVB2	430	386	0.06%	0.008%
56	10.244	1498	1502	1505	rBV2	681	834	0.12%	0.017%
57	10.305	1508	1512	1517	rVB3	540	873	0.13%	0.017%
58	10.396	1524	1527	1529	rVB2	270	233	0.03%	0.005%
59	10.640	1565	1567	1571	rVB3	265	279	0.04%	0.006%
60	10.793	1590	1592	1594	rVV2	189	197	0.03%	0.004%
61	11.043	1628	1633	1635	rBV2	223	404	0.06%	0.008%
62	11.122	1642	1646	1650	rVB2	1351	1752	0.26%	0.035%
63	11.195	1652	1658	1668	rVV	257900	320756	46.76%	6.387%
64	11.457	1698	1701	1702	rBV2	342	303	0.04%	0.006%
65	11.591	1721	1723	1726	rBV2	255	197	0.03%	0.004%
66	11.750	1745	1749	1754	rVB4	1212	1887	0.28%	0.038%
67	11.835	1761	1763	1768	rBV3	214	444	0.06%	0.009%
68	11.927	1775	1778	1783	rBV5	698	1067	0.16%	0.021%
69	12.024	1789	1794	1803	rBV	323763	408214	59.51%	8.129%
70	12.128	1809	1811	1812	rBV	447	352	0.05%	0.007%
71	12.225	1824	1827	1830	rVB2	612	717	0.10%	0.014%
72	12.323	1837	1843	1852	rBV	332497	441130	64.31%	8.784%
73	12.427	1858	1860	1863	rVB	729	614	0.09%	0.012%
74	12.451	1863	1864	1867	rVB	203	189	0.03%	0.004%
75	12.481	1867	1869	1873	rBV2	455	486	0.07%	0.010%
76	12.536	1875	1878	1879	rVB2	226	177	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025941.D
 Acq On : 21 Dec 2021 01:50
 Operator : JC/MD
 Sample : M5126-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

77	12.609	1888	1890	1893	rVV2	247	273	0.04%	0.005%
78	12.664	1896	1899	1903	rVB2	300	338	0.05%	0.007%
79	12.731	1908	1910	1915	rVV	202	284	0.04%	0.006%
80	12.945	1940	1945	1948	rVB2	195	296	0.04%	0.006%
81	13.298	2002	2003	2006	rBV2	248	233	0.03%	0.005%
82	13.329	2006	2008	2010	rVV2	251	284	0.04%	0.006%
83	13.530	2040	2041	2044	rBV	238	313	0.05%	0.006%
84	13.798	2084	2085	2089	rBV2	288	354	0.05%	0.007%
85	13.926	2104	2106	2109	rVB2	298	268	0.04%	0.005%
86	14.134	2136	2140	2141	rBV2	270	280	0.04%	0.006%
87	14.377	2178	2180	2183	rBV	225	184	0.03%	0.004%
88	14.652	2223	2225	2227	rVB	358	186	0.03%	0.004%
89	14.798	2246	2249	2250	rBV	195	184	0.03%	0.004%
90	15.176	2309	2311	2314	rBV3	340	478	0.07%	0.010%
91	15.225	2318	2319	2323	rVV2	245	288	0.04%	0.006%
92	15.341	2336	2338	2343	rVV3	241	308	0.04%	0.006%
93	15.499	2361	2364	2367	rBV3	216	359	0.05%	0.007%
94	15.609	2381	2382	2384	rBV2	265	204	0.03%	0.004%
95	15.639	2384	2387	2390	rVV3	282	287	0.04%	0.006%
96	15.725	2400	2401	2403	rBV2	249	185	0.03%	0.004%
97	15.774	2408	2409	2412	rVB2	326	202	0.03%	0.004%
98	15.981	2439	2443	2444	rBV3	343	398	0.06%	0.008%
99	16.078	2456	2459	2460	rBV	230	214	0.03%	0.004%
100	16.389	2508	2510	2515	rVB2	393	369	0.05%	0.007%




Sum of corrected areas: 5021921

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025941.D
Acq On : 21 Dec 2021 01:50
Operator : JC/MD
Sample : M5126-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

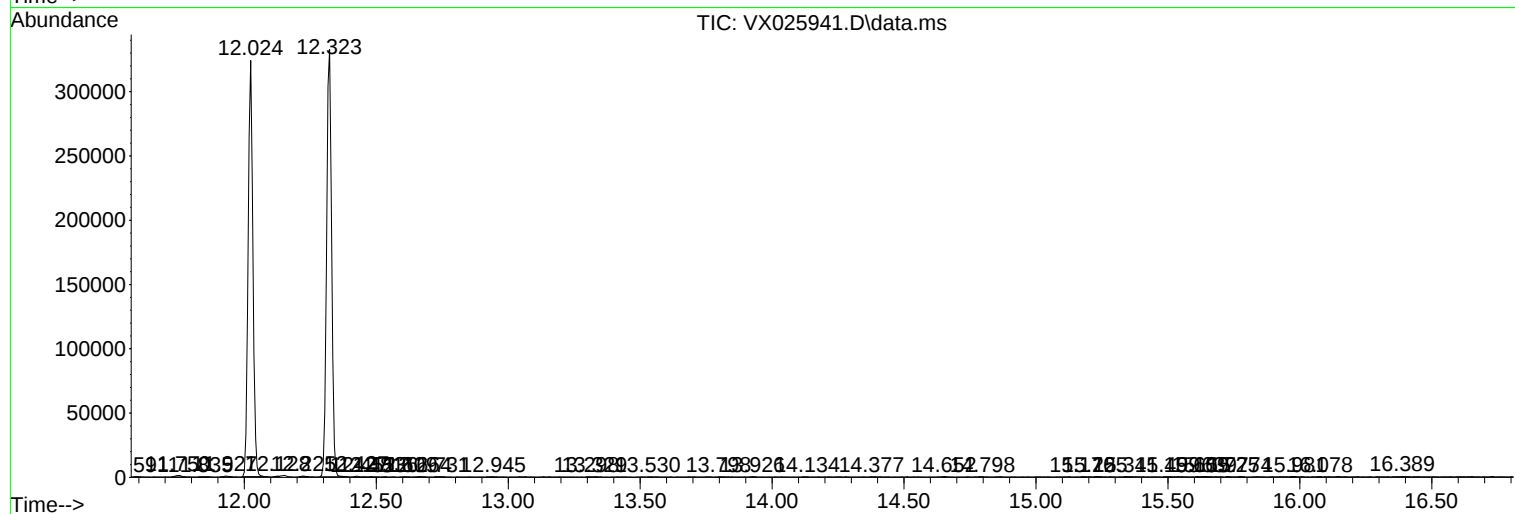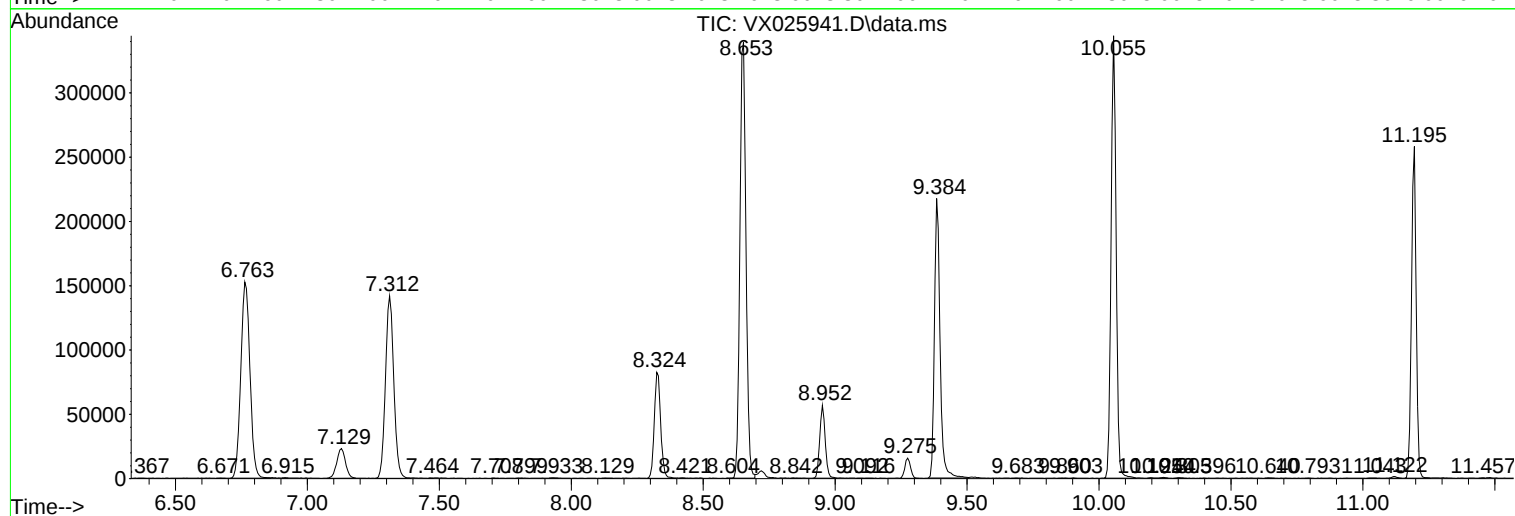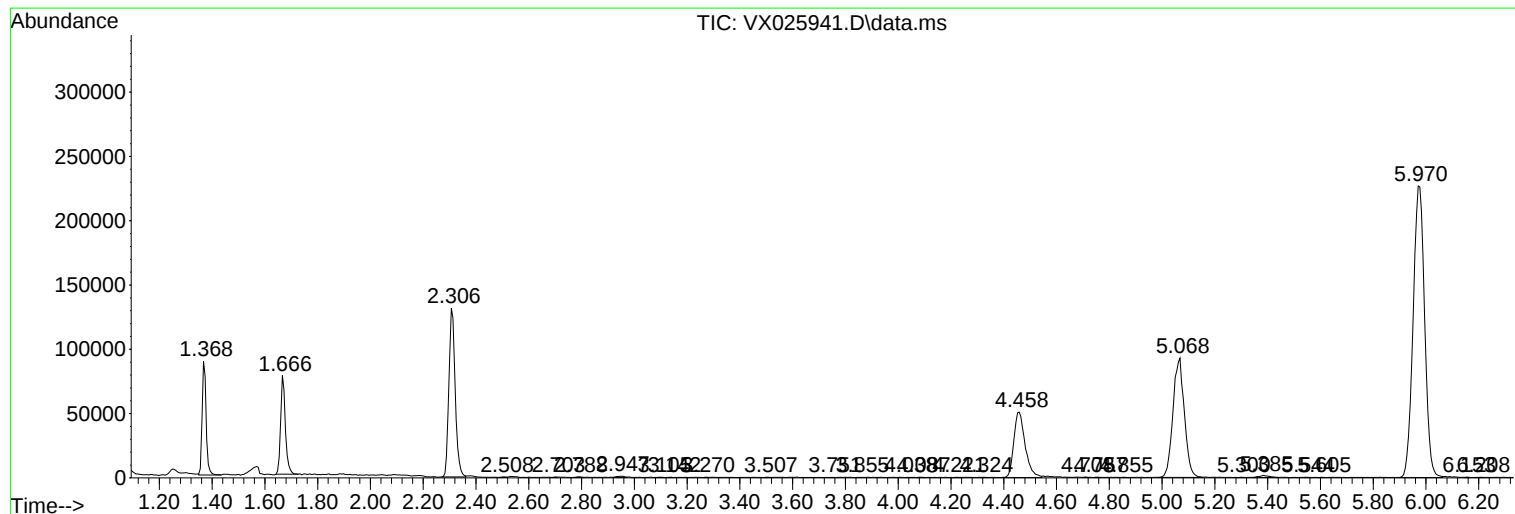

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025941.D
Acq On : 21 Dec 2021 01:50
Operator : JC/MD
Sample : M5126-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
Data File : VX025941.D
Acq On : 21 Dec 2021 01:50
Operator : JC/MD
Sample : M5126-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc