


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122021\
 Data File : VX025908.D
 Acq On : 20 Dec 2021 09:40
 Operator : JC/MD
 Sample : BFB625
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB625

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis
 Last Update : Wed Dec 22 05:35:20 2021

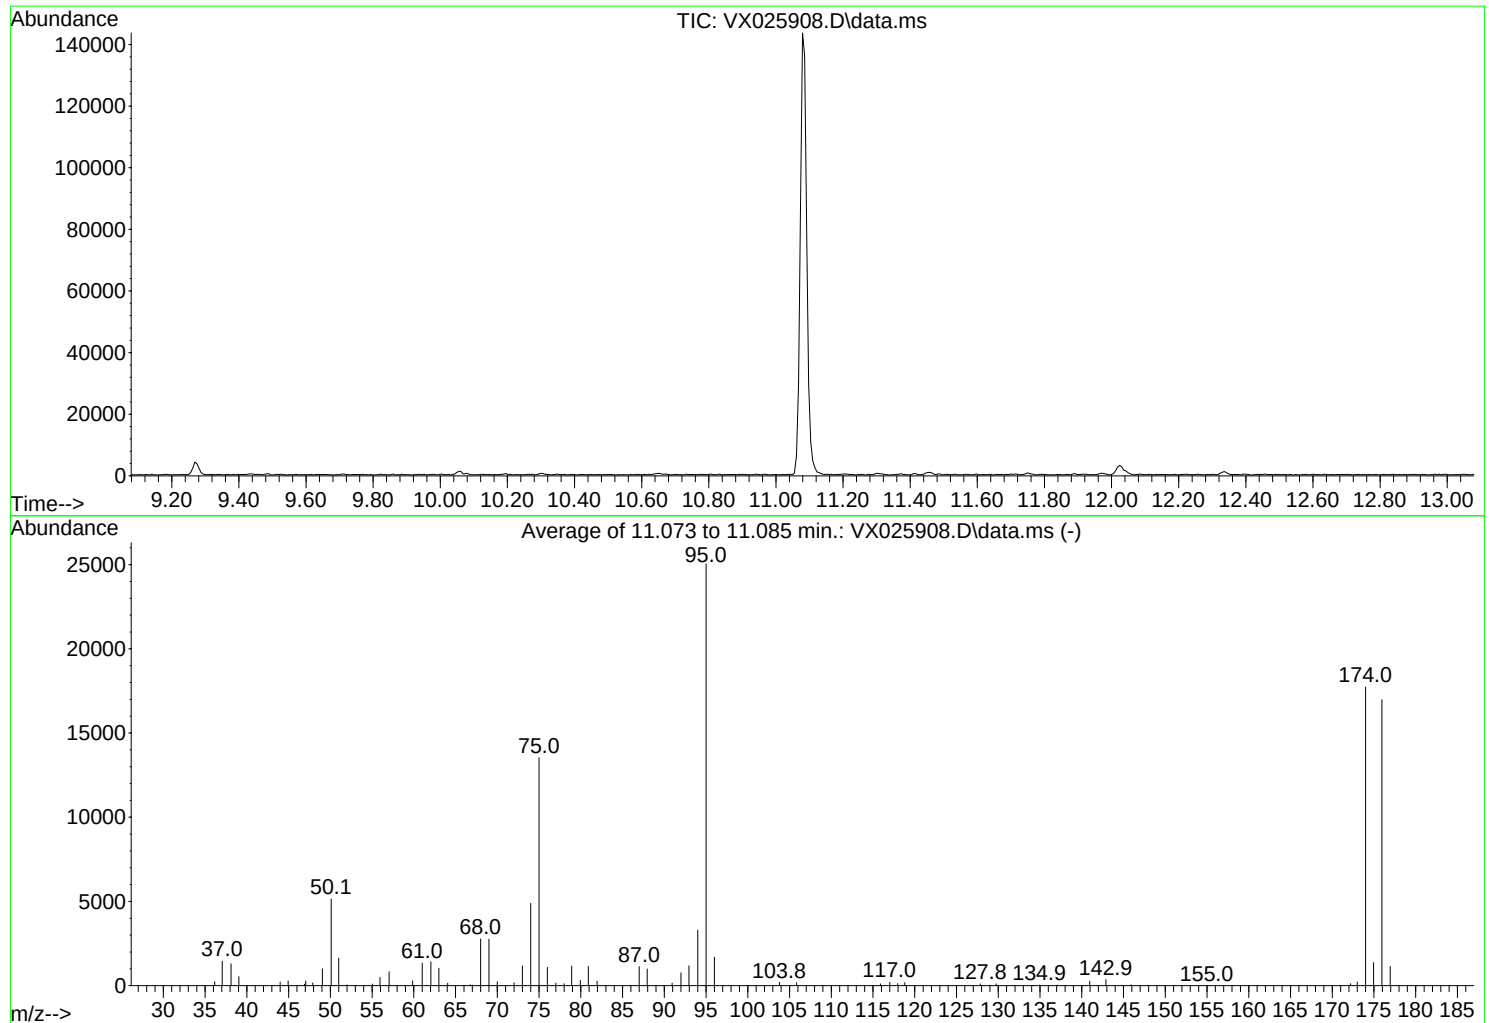

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	5136	PASS
75	95	30	80	54.1	13540	PASS
95	95	100	100	100.0	25045	PASS
96	95	5	9	6.8	1694	PASS
173	174	0.00	2	1.2	221	PASS
174	95	50	120	70.8	17731	PASS
175	174	5	9	7.7	1369	PASS
176	174	95	101	95.8	16981	PASS
177	176	5	9	6.7	1144	PASS

m/z	Abundance
40.00	341.0
44.00	167.0

Instrument :
MSVOA_X
ClientSampleId :
BFB625

m/z	Abundance
36.20	148.0
37.00	1113.0
38.10	1093.0
39.10	461.0
40.10	206.0
44.10	302.0
45.00	266.0
46.90	247.0
47.90	143.0
49.00	727.0
50.10	4203.0
51.00	1419.0
52.00	98.0
55.10	81.0
55.90	378.0
57.00	757.0
59.80	222.0
61.10	1126.0
62.00	1360.0
63.00	771.0
64.10	78.0
66.80	102.0
68.00	1914.0
69.00	1989.0
70.00	209.0
72.00	150.0
73.00	848.0
74.00	3769.0
75.00	10415.0
76.00	797.0
76.90	109.0
78.10	57.0
78.90	864.0
80.00	182.0
80.90	831.0
81.90	186.0
87.00	977.0
88.00	792.0
90.90	108.0
92.10	676.0
92.90	811.0
94.00	2320.0
95.00	18512.0
96.00	1306.0
103.80	134.0
105.80	125.0
115.90	62.0
117.00	160.0
117.90	100.0
118.90	116.0
127.80	71.0
129.80	67.0
140.90	173.0
142.90	336.0
147.80	62.0
172.40	51.0
173.00	81.0
174.00	10728.0
174.90	1015.0
176.00	9360.0
176.90	749.0

Instrument :
MSVOA_X
ClientSampleId :
BFB625

m/z	Abundance
36.10	287.0
37.10	1802.0
38.10	1478.0
39.00	543.0
39.90	223.0
43.90	390.0
44.90	274.0
47.10	403.0
47.90	211.0
49.00	1190.0
50.10	6198.0
51.00	1894.0
52.00	85.0
55.10	95.0
56.00	614.0
57.10	995.0
59.90	290.0
61.00	1537.0
62.10	1427.0
63.00	1263.0
64.00	190.0
66.70	74.0
67.10	66.0
68.00	3562.0
69.00	3322.0
70.00	310.0
72.00	217.0
73.00	1432.0
74.00	5507.0
75.00	15745.0
76.00	1338.0
77.00	228.0
78.00	151.0
78.90	1315.0
79.90	395.0
80.90	1357.0
81.90	321.0
87.00	1249.0
88.00	1116.0
90.90	172.0
92.00	870.0
93.00	1499.0
94.00	3979.0
95.00	28640.0
96.00	2024.0
103.90	230.0
105.90	176.0
116.00	125.0
117.00	146.0
117.90	123.0
118.90	227.0
127.90	95.0
128.90	80.0
129.80	131.0
135.00	53.0
137.00	68.0
140.90	382.0
141.80	65.0
142.90	431.0
144.80	77.0
145.90	100.0
172.20	95.0
173.00	301.0
174.00	20560.0
175.00	1643.0
176.00	20944.0
177.00	1378.0

Instrument :
MSVOA_X
ClientSampleId :
BFB625

m/z	Abundance
36.10	259.0
37.10	1421.0
38.10	1311.0
39.00	605.0
40.00	272.0
44.10	439.0
45.00	291.0
47.00	423.0
47.90	142.0
49.10	1084.0
50.10	5007.0
51.00	1585.0
55.00	121.0
56.00	474.0
57.10	724.0
59.90	351.0
60.90	1350.0
62.10	1473.0
63.00	1079.0
64.00	165.0
67.00	57.0
68.00	2829.0
69.00	2953.0
70.00	188.0
72.00	157.0
73.00	1218.0
74.00	5377.0
75.00	14459.0
76.00	1108.0
77.10	131.0
77.90	150.0
78.90	1288.0
79.90	370.0
80.90	1225.0
82.00	305.0
87.00	1162.0
87.90	1049.0
91.00	166.0
91.90	721.0
93.00	1224.0
94.00	3592.0
95.00	27984.0
96.00	1751.0
103.70	207.0
105.00	55.0
105.90	206.0
115.80	134.0
117.00	294.0
118.00	140.0
118.70	210.0
127.90	161.0
129.70	124.0
134.90	77.0
137.10	60.0
141.00	243.0
142.90	311.0
145.90	76.0
155.00	53.0
172.20	198.0
173.00	280.0
174.00	21904.0
175.00	1449.0
175.90	20640.0
177.00	1306.0

Instrument :
MSVOA_X
ClientSampleId :
BFB625