

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122022\
Data File : VX033499.D
Acq On : 20 Dec 2022 11:32
Operator : JC/MD
Sample : VX1220WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1220WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M

Title : SW846 8260

Signal : TIC: VX033499.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	693	705	720	rBV	50226	146093	27.17%	5.349%
2	5.550	721	732	748	rVB	136635	389074	72.36%	14.247%
3	5.952	788	798	813	rBV	37212	100335	18.66%	3.674%
4	6.757	920	930	950	rBV	197901	471762	87.74%	17.274%
5	8.647	1234	1240	1250	rBV	147119	228722	42.54%	8.375%
6	10.055	1465	1471	1484	rBV	391673	537710	100.00%	19.689%
7	11.079	1634	1639	1657	rBV	273292	341089	63.43%	12.489%
8	12.024	1788	1794	1802	rBV	403083	510758	94.99%	18.702%
9	13.725	2069	2073	2078	rBV2	4593	5464	1.02%	0.200%




Sum of corrected areas: 2731007

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122022\
Data File : VX033499.D
Acq On : 20 Dec 2022 11:32
Operator : JC/MD
Sample : VX1220WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1220WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

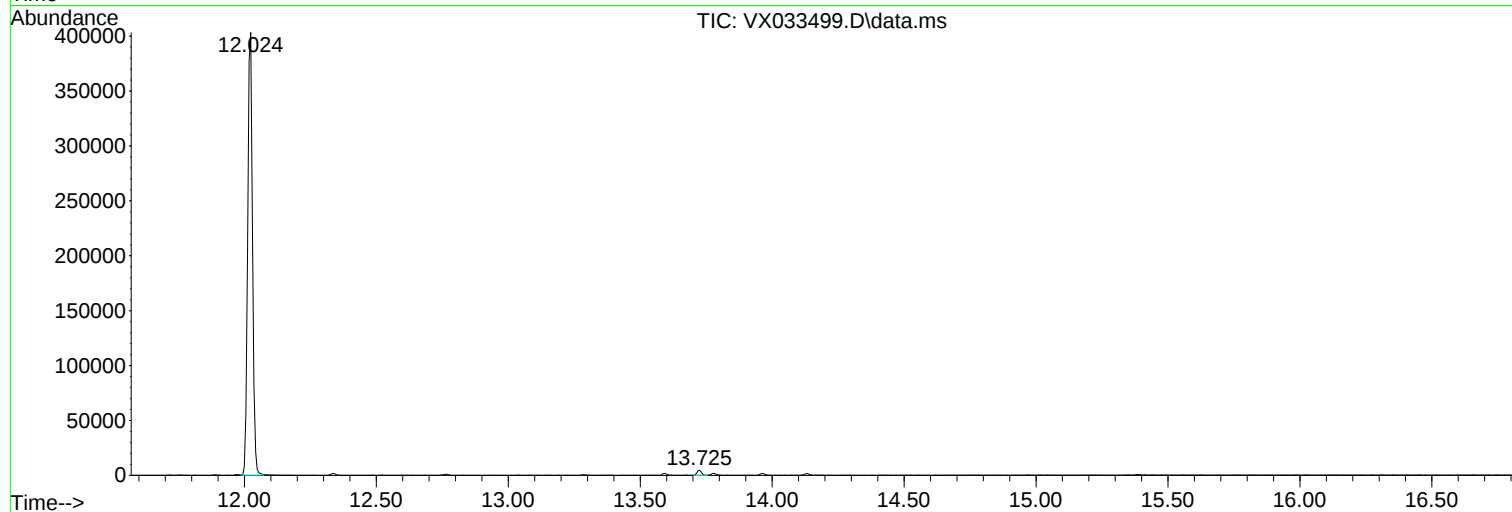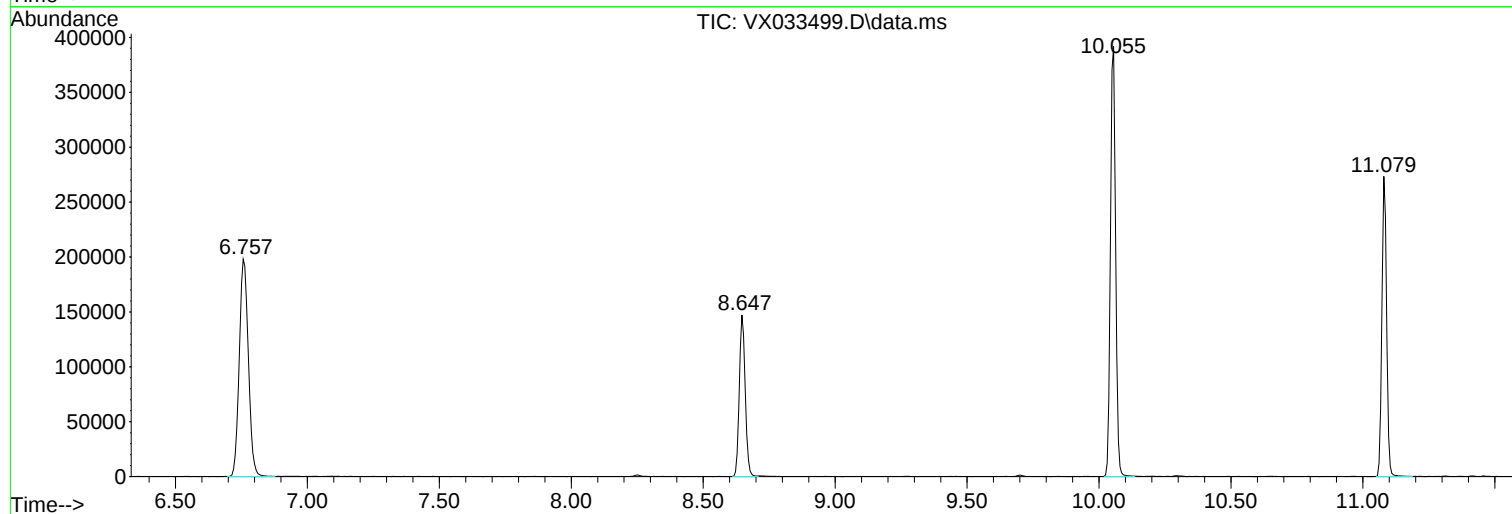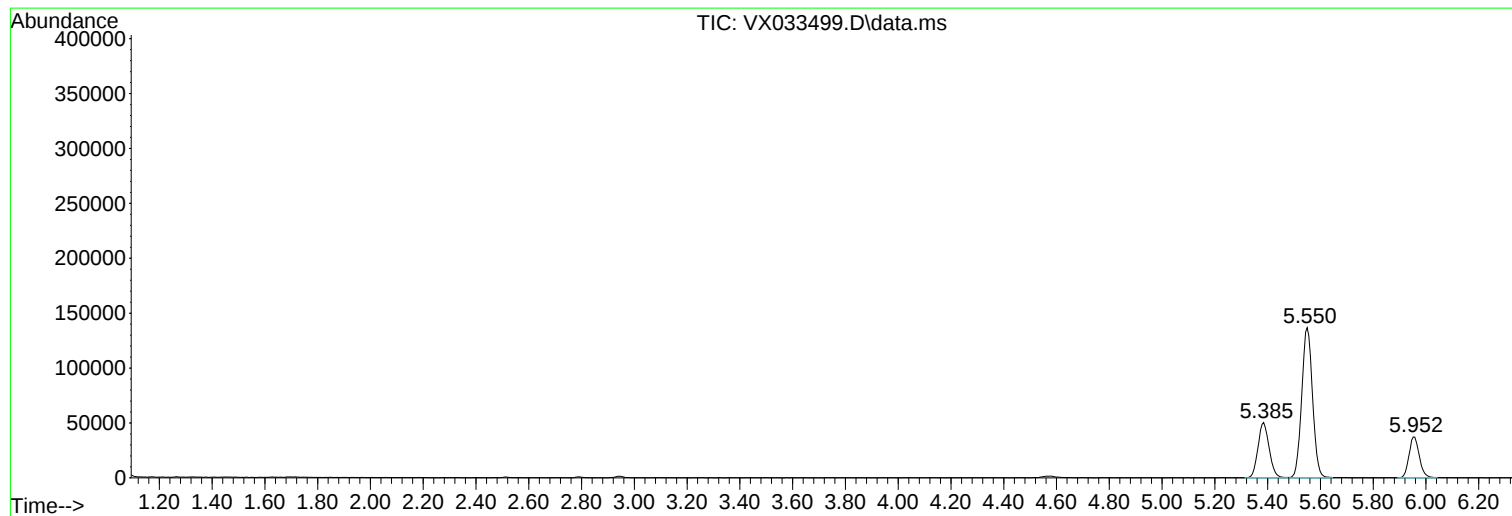

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122022\
Data File : VX033499.D
Acq On : 20 Dec 2022 11:32
Operator : JC/MD
Sample : VX1220WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1220WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122022\
Data File : VX033499.D
Acq On : 20 Dec 2022 11:32
Operator : JC/MD
Sample : VX1220WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1220WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc