

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039387.D
 Acq On : 20 Dec 2023 09:23
 Operator : JC/MD
 Sample : VX1220MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK654

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039387.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	57	rVB	103801	117912	13.29%	1.725%
2	1.672	91	96	112	rBV	68798	107485	12.12%	1.573%
3	2.306	194	200	211	rBV	192953	301774	34.02%	4.415%
4	2.550	238	240	242	rBV2	215	188	0.02%	0.003%
5	2.697	263	264	265	rBV	327	177	0.02%	0.003%
6	2.715	265	267	269	rVV	389	277	0.03%	0.004%
7	2.782	273	278	284	rBV3	1552	3037	0.34%	0.044%
8	2.940	295	304	311	rBV4	2287	5357	0.60%	0.078%
9	3.014	314	316	319	rBV2	168	202	0.02%	0.003%
10	3.093	323	329	334	rBV4	518	1250	0.14%	0.018%
11	3.172	340	342	344	rBV2	224	214	0.02%	0.003%
12	3.422	380	383	386	rBV2	122	189	0.02%	0.003%
13	3.532	398	401	402	rBV2	200	183	0.02%	0.003%
14	3.568	405	407	410	rVB2	255	192	0.02%	0.003%
15	3.922	462	465	467	rBV2	176	249	0.03%	0.004%
16	4.050	481	486	487	rBV2	207	308	0.03%	0.005%
17	4.440	542	550	565	rBV	74757	215274	24.27%	3.150%
18	5.050	638	650	667	rBV	108516	353704	39.87%	5.175%
19	5.214	675	677	679	rVB	352	225	0.03%	0.003%
20	5.300	687	691	693	rBV2	199	298	0.03%	0.004%
21	5.434	710	713	716	rVB2	181	258	0.03%	0.004%
22	5.464	716	718	720	rBV2	300	248	0.03%	0.004%
23	5.964	787	800	819	rBV2	290164	887100	100.00%	12.979%
24	6.385	866	869	871	rBV2	212	277	0.03%	0.004%
25	6.543	892	895	899	rBV3	183	223	0.03%	0.003%
26	6.757	921	930	944	rBV	211230	500176	56.38%	7.318%
27	7.117	983	989	994	rBV5	1192	3059	0.34%	0.045%
28	7.306	1010	1020	1035	rBV	180308	406943	45.87%	5.954%
29	7.470	1045	1047	1048	rBV	313	169	0.02%	0.002%
30	7.488	1048	1050	1054	rVV2	465	480	0.05%	0.007%
31	7.519	1054	1055	1059	rVB2	351	205	0.02%	0.003%
32	7.623	1069	1072	1073	rBV2	190	231	0.03%	0.003%
33	7.799	1099	1101	1105	rBV2	182	267	0.03%	0.004%
34	7.946	1123	1125	1129	rBV	393	536	0.06%	0.008%
35	8.324	1181	1187	1205	rBV	127945	212212	23.92%	3.105%
36	8.574	1225	1228	1233	rVB4	571	856	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039387.D
 Acq On : 20 Dec 2023 09:23
 Operator : JC/MD
 Sample : VX1220MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK654

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	8.647	1233	1240	1258	rBV	427092	695080	78.35%	10.169%
38	8.897	1279	1281	1284	rBV2	179	189	0.02%	0.003%
39	8.946	1284	1289	1305	rVV	93775	143466	16.17%	2.099%
40	9.128	1316	1319	1322	rBV2	199	234	0.03%	0.003%
41	9.275	1339	1343	1345	rBV2	433	660	0.07%	0.010%
42	9.378	1355	1360	1375	rBV	356726	512593	57.78%	7.499%
43	9.604	1395	1397	1400	rVB3	416	297	0.03%	0.004%
44	9.854	1435	1438	1441	rVB2	368	378	0.04%	0.006%
45	9.890	1441	1444	1445	rBV2	298	243	0.03%	0.004%
46	10.049	1465	1470	1482	rBV	446240	626716	70.65%	9.169%
47	10.195	1491	1494	1499	rVB3	901	1436	0.16%	0.021%
48	10.238	1499	1501	1503	rBV	185	206	0.02%	0.003%
49	10.281	1505	1508	1509	rBV2	212	223	0.03%	0.003%
50	10.305	1509	1512	1515	rBV2	478	659	0.07%	0.010%
51	10.372	1521	1523	1526	rBV2	252	242	0.03%	0.004%
52	10.396	1526	1527	1531	rVB2	229	175	0.02%	0.003%
53	10.646	1565	1568	1570	rBV3	723	874	0.10%	0.013%
54	10.805	1590	1594	1597	rVB2	225	260	0.03%	0.004%
55	10.957	1617	1619	1624	rVB3	643	916	0.10%	0.013%
56	11.189	1652	1657	1668	rBV	344024	433505	48.87%	6.342%
57	11.311	1673	1677	1682	rBV3	1019	1483	0.17%	0.022%
58	11.457	1697	1701	1704	rBV2	784	928	0.10%	0.014%
59	11.524	1711	1712	1716	rVB2	238	264	0.03%	0.004%
60	11.585	1716	1722	1724	rBV	325	578	0.07%	0.008%
61	11.677	1734	1737	1740	rVB	205	239	0.03%	0.003%
62	11.707	1740	1742	1744	rBV	312	309	0.03%	0.005%
63	11.756	1747	1750	1754	rVB3	807	1038	0.12%	0.015%
64	11.969	1781	1785	1788	rBV2	1012	1380	0.16%	0.020%
65	12.018	1788	1793	1806	rVV	496004	641970	72.37%	9.392%
66	12.317	1837	1842	1852	rBV	489331	617099	69.56%	9.028%
67	12.451	1862	1864	1866	rVB2	316	309	0.03%	0.005%
68	12.591	1884	1887	1889	rVB2	183	213	0.02%	0.003%
69	12.622	1889	1892	1893	rBV	311	249	0.03%	0.004%
70	12.762	1906	1915	1924	rVB2	3412	5191	0.59%	0.076%
71	12.823	1924	1925	1928	rBV2	219	270	0.03%	0.004%
72	12.933	1941	1943	1945	rBV	332	324	0.04%	0.005%
73	13.055	1961	1963	1965	rVB2	251	183	0.02%	0.003%
74	13.109	1970	1972	1977	rVV3	1016	1371	0.15%	0.020%
75	13.341	2006	2010	2011	rBV2	162	213	0.02%	0.003%
76	13.481	2029	2033	2034	rBV2	222	235	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039387.D
 Acq On : 20 Dec 2023 09:23
 Operator : JC/MD
 Sample : VX1220MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK654

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.591	2048	2051	2055	rBV3	2006	2315	0.26%	0.034%
78	13.780	2077	2082	2088	rBV2	2906	4146	0.47%	0.061%
79	13.853	2091	2094	2097	rVB	242	296	0.03%	0.004%
80	13.920	2103	2105	2108	rBV2	183	228	0.03%	0.003%
81	13.963	2108	2112	2115	rVV2	2106	2496	0.28%	0.037%
82	14.128	2135	2139	2144	rVB	4576	5833	0.66%	0.085%
83	14.213	2152	2153	2156	rVB	272	227	0.03%	0.003%
84	14.438	2188	2190	2194	rBV	128	191	0.02%	0.003%
85	14.566	2208	2211	2212	rBV2	188	185	0.02%	0.003%
86	14.902	2262	2266	2268	rBV3	238	382	0.04%	0.006%
87	14.926	2268	2270	2272	rBV	327	238	0.03%	0.003%
88	15.298	2329	2331	2336	rBV2	260	370	0.04%	0.005%
89	15.335	2336	2337	2339	rVV	193	171	0.02%	0.003%
90	15.383	2342	2345	2351	rBV6	742	1372	0.15%	0.020%
91	15.469	2358	2359	2360	rBV	371	175	0.02%	0.003%
92	15.487	2360	2362	2365	rVV3	272	247	0.03%	0.004%
93	15.548	2370	2372	2376	rBV2	329	497	0.06%	0.007%
94	15.627	2383	2385	2386	rBV	310	167	0.02%	0.002%
95	15.780	2408	2410	2411	rBV	277	180	0.02%	0.003%
96	15.956	2437	2439	2442	rVB2	298	297	0.03%	0.004%
97	16.194	2476	2478	2482	rVB3	289	291	0.03%	0.004%
98	16.347	2502	2503	2505	rVB	386	197	0.02%	0.003%
99	16.383	2507	2509	2514	rBV3	335	433	0.05%	0.006%
100	16.597	2543	2544	2547	rBV2	251	234	0.03%	0.003%

Sum of corrected areas: 6835101




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039387.D
Acq On : 20 Dec 2023 09:23
Operator : JC/MD
Sample : VX1220MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK654

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

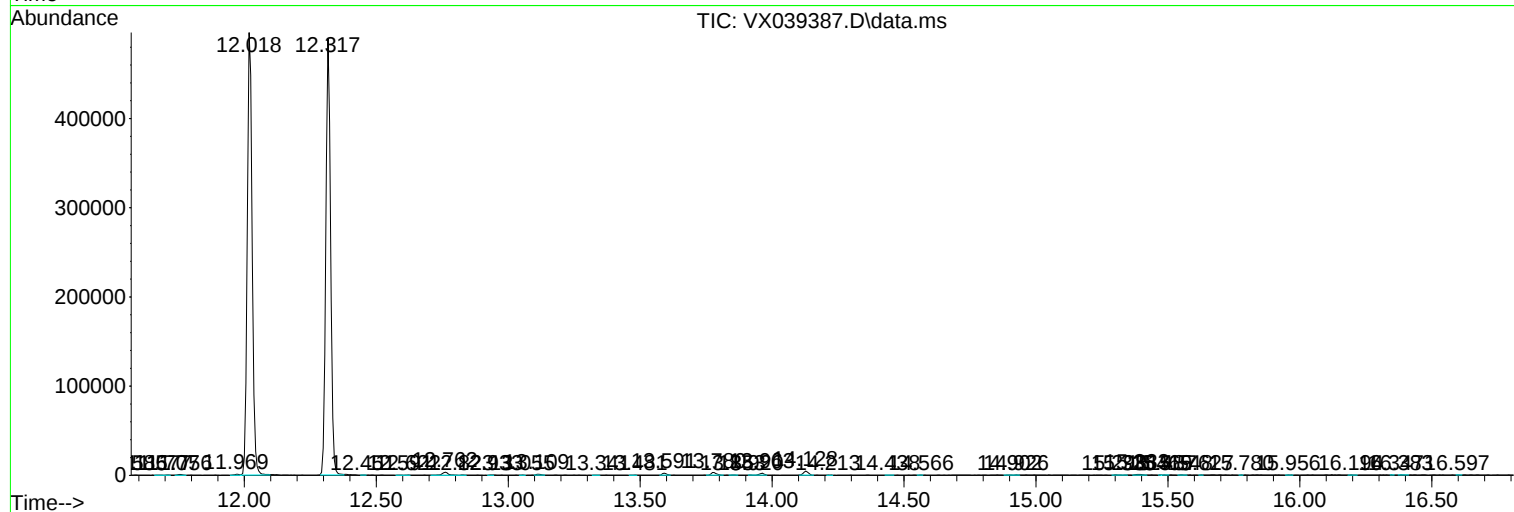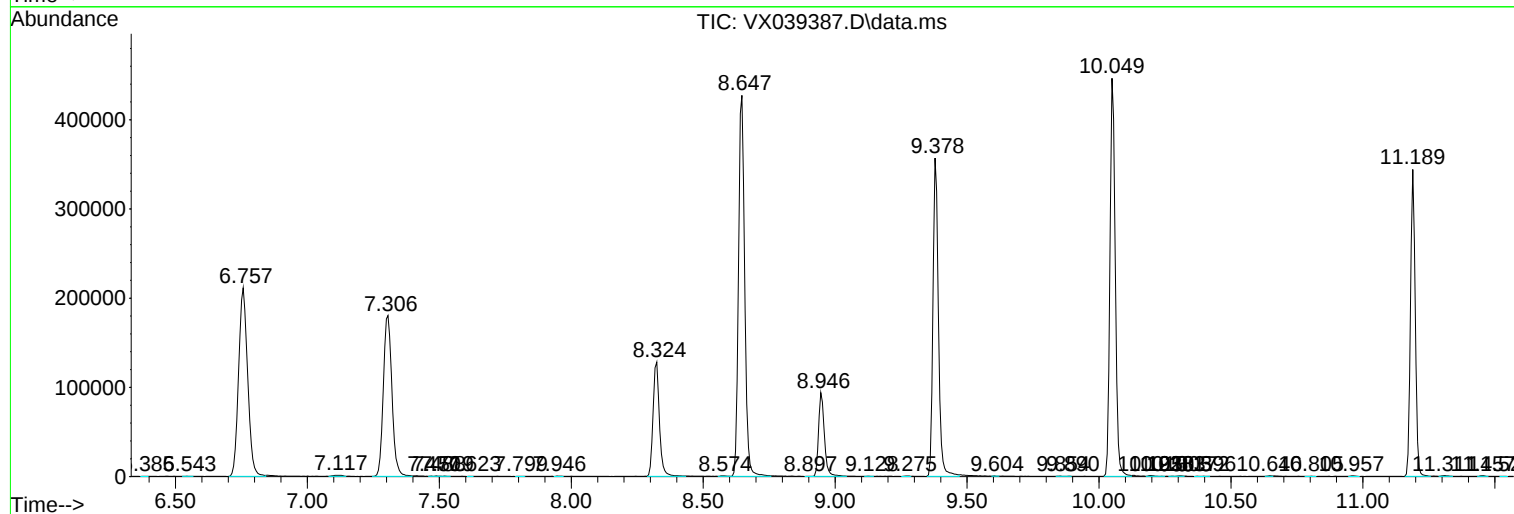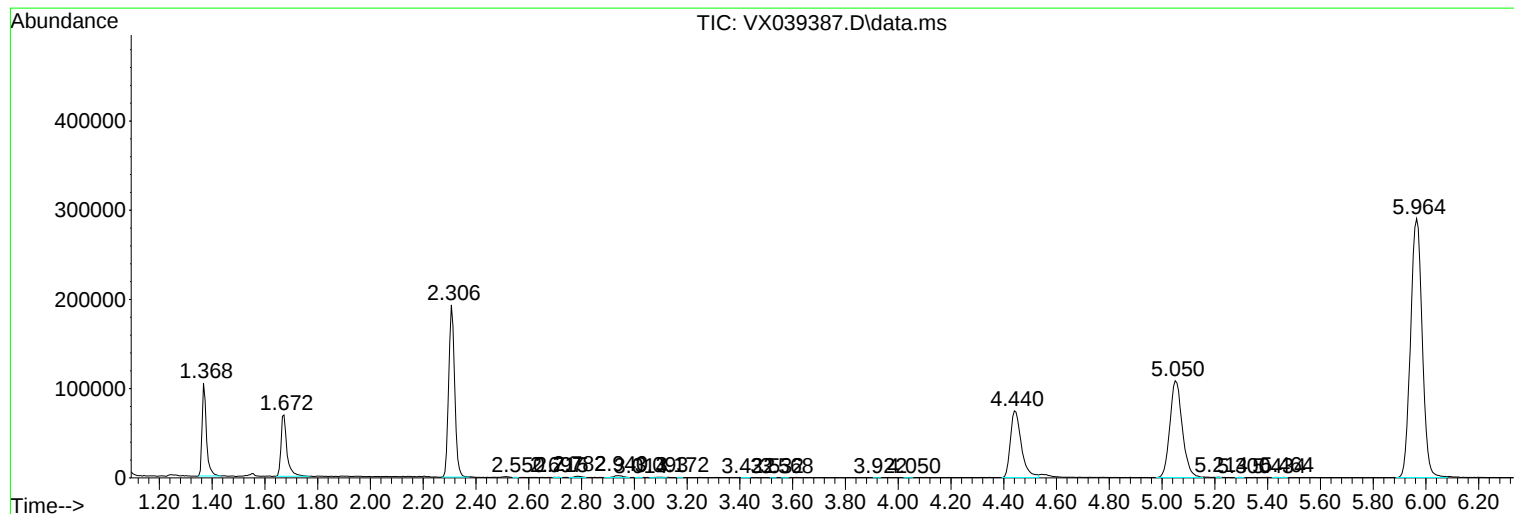

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039387.D
Acq On : 20 Dec 2023 09:23
Operator : JC/MD
Sample : VX1220MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK654

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039387.D
Acq On : 20 Dec 2023 09:23
Operator : JC/MD
Sample : VX1220MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK654

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc