

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039388.D
 Acq On : 20 Dec 2023 09:46
 Operator : JC/MD
 Sample : VX1220WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK655

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039388.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	27	rBV	1899	1854	0.22%	0.028%
2	1.368	43	46	60	rVB	99350	112485	13.19%	1.704%
3	1.550	72	76	80	rBV2	2889	4083	0.48%	0.062%
4	1.672	91	96	107	rBV	70591	104272	12.23%	1.580%
5	2.306	194	200	212	rBV	180002	288052	33.78%	4.364%
6	2.514	229	234	241	rBV3	1007	1900	0.22%	0.029%
7	2.581	241	245	246	rBV	279	273	0.03%	0.004%
8	2.599	246	248	250	rVB	409	234	0.03%	0.004%
9	2.623	250	252	255	rVB	279	275	0.03%	0.004%
10	2.678	260	261	263	rBV	257	196	0.02%	0.003%
11	2.794	275	280	285	rBV3	1126	1937	0.23%	0.029%
12	2.940	295	304	311	rBV2	2828	6292	0.74%	0.095%
13	3.093	326	329	330	rBV2	215	223	0.03%	0.003%
14	3.251	350	355	356	rBV2	214	248	0.03%	0.004%
15	3.721	428	432	435	rVB2	192	219	0.03%	0.003%
16	3.904	460	462	467	rVB2	225	304	0.04%	0.005%
17	3.952	467	470	471	rBV	285	214	0.03%	0.003%
18	4.038	482	484	487	rBV2	165	218	0.03%	0.003%
19	4.190	507	509	512	rBV2	220	170	0.02%	0.003%
20	4.446	542	551	564	rBV	76243	220330	25.84%	3.338%
21	5.056	637	651	671	rBV2	102126	339739	39.84%	5.148%
22	5.373	701	703	704	rBV	658	471	0.06%	0.007%
23	5.446	711	715	718	rBV2	235	419	0.05%	0.006%
24	5.544	727	731	733	rBV3	421	521	0.06%	0.008%
25	5.964	789	800	823	rBV2	279482	852822	100.00%	12.922%
26	6.269	847	850	851	rBV	185	228	0.03%	0.003%
27	6.757	921	930	947	rBV	198692	480153	56.30%	7.275%
28	7.043	976	977	980	rBV2	284	285	0.03%	0.004%
29	7.110	984	988	991	rVV4	1297	2265	0.27%	0.034%
30	7.306	1011	1020	1037	rBV	177855	395504	46.38%	5.993%
31	7.476	1046	1048	1050	rBV2	330	285	0.03%	0.004%
32	7.580	1063	1065	1067	rBV2	164	181	0.02%	0.003%
33	7.610	1067	1070	1074	rVB2	213	257	0.03%	0.004%
34	7.744	1089	1092	1095	rBV	214	239	0.03%	0.004%
35	7.903	1116	1118	1121	rBV2	183	241	0.03%	0.004%
36	8.110	1150	1152	1154	rBV2	205	214	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039388.D
 Acq On : 20 Dec 2023 09:46
 Operator : JC/MD
 Sample : VX1220WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK655

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	8.177	1159	1163	1166	rVB2	179	260	0.03%	0.004%
38	8.324	1181	1187	1199	rBV	126023	204769	24.01%	3.103%
39	8.470	1209	1211	1213	rBV2	229	275	0.03%	0.004%
40	8.574	1224	1228	1233	rVB3	601	769	0.09%	0.012%
41	8.647	1233	1240	1256	rBV	424353	660316	77.43%	10.005%
42	8.945	1284	1289	1304	rBV	85455	134268	15.74%	2.034%
43	9.275	1339	1343	1345	rBV2	386	489	0.06%	0.007%
44	9.323	1349	1351	1355	rBV2	134	197	0.02%	0.003%
45	9.378	1355	1360	1376	rBV	347174	513650	60.23%	7.783%
46	9.701	1410	1413	1414	rVV	342	304	0.04%	0.005%
47	9.829	1432	1434	1436	rBV	205	187	0.02%	0.003%
48	10.049	1465	1470	1487	rBV	411873	599477	70.29%	9.083%
49	10.232	1498	1500	1502	rVB	183	172	0.02%	0.003%
50	10.250	1502	1503	1506	rBV2	212	184	0.02%	0.003%
51	10.305	1509	1512	1516	rBV3	737	1021	0.12%	0.015%
52	10.378	1523	1524	1526	rBV	218	202	0.02%	0.003%
53	10.646	1564	1568	1572	rBV4	513	904	0.11%	0.014%
54	10.768	1586	1588	1590	rVB	240	204	0.02%	0.003%
55	10.823	1596	1597	1602	rVB	279	208	0.02%	0.003%
56	10.963	1617	1620	1625	rVB2	529	638	0.07%	0.010%
57	11.098	1636	1642	1647	rVB3	213	465	0.05%	0.007%
58	11.146	1647	1650	1652	rBV	175	192	0.02%	0.003%
59	11.189	1652	1657	1670	rVB	332512	426591	50.02%	6.464%
60	11.311	1675	1677	1682	rVB3	977	1000	0.12%	0.015%
61	11.451	1696	1700	1704	rBV3	622	933	0.11%	0.014%
62	11.512	1707	1710	1715	rBV2	160	253	0.03%	0.004%
63	11.689	1738	1739	1742	rBV	259	266	0.03%	0.004%
64	11.756	1746	1750	1755	rBV3	655	883	0.10%	0.013%
65	11.975	1782	1786	1788	rVB3	947	1124	0.13%	0.017%
66	12.018	1788	1793	1804	rBV	462900	612526	71.82%	9.281%
67	12.140	1812	1813	1815	rVB	464	231	0.03%	0.004%
68	12.213	1822	1825	1826	rBV2	221	198	0.02%	0.003%
69	12.317	1837	1842	1854	rBV	470541	597155	70.02%	9.048%
70	12.701	1900	1905	1907	rVV2	185	297	0.03%	0.005%
71	12.737	1907	1911	1912	rVV2	413	486	0.06%	0.007%
72	12.762	1912	1915	1920	rVV2	3320	4298	0.50%	0.065%
73	12.823	1923	1925	1928	rBV2	173	168	0.02%	0.003%
74	12.890	1933	1936	1937	rVB2	273	217	0.03%	0.003%
75	12.914	1937	1940	1941	rBV2	181	229	0.03%	0.003%
76	13.048	1961	1962	1964	rBV	274	191	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039388.D
 Acq On : 20 Dec 2023 09:46
 Operator : JC/MD
 Sample : VX1220WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK655

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.085	1966	1968	1970	rBV	190	172	0.02%	0.003%
78	13.122	1970	1974	1977	rVB3	440	648	0.08%	0.010%
79	13.591	2047	2051	2055	rVB2	1178	1535	0.18%	0.023%
80	13.628	2055	2057	2060	rBV	221	275	0.03%	0.004%
81	13.737	2073	2075	2077	rBV	261	213	0.02%	0.003%
82	13.780	2080	2082	2090	rVB3	1181	1750	0.21%	0.027%
83	13.841	2090	2092	2094	rBV2	247	251	0.03%	0.004%
84	13.920	2103	2105	2107	rBV	189	178	0.02%	0.003%
85	13.957	2109	2111	2116	rVV3	672	967	0.11%	0.015%
86	14.036	2123	2124	2127	rVB	318	188	0.02%	0.003%
87	14.073	2127	2130	2134	rBV2	322	470	0.06%	0.007%
88	14.127	2135	2139	2144	rVV	3943	4958	0.58%	0.075%
89	14.182	2147	2148	2151	rBV2	309	297	0.03%	0.005%
90	14.274	2161	2163	2166	rVB	234	184	0.02%	0.003%
91	14.457	2191	2193	2197	rVB2	312	226	0.03%	0.003%
92	14.835	2252	2255	2259	rBV2	203	296	0.03%	0.004%
93	14.926	2267	2270	2272	rBV2	292	368	0.04%	0.006%
94	15.383	2342	2345	2351	rBV3	922	1614	0.19%	0.024%
95	15.463	2357	2358	2363	rVB2	365	329	0.04%	0.005%
96	15.621	2383	2384	2386	rBV	282	179	0.02%	0.003%
97	15.908	2428	2431	2433	rBV2	296	408	0.05%	0.006%
98	15.963	2438	2440	2442	rVB2	258	185	0.02%	0.003%
99	16.060	2454	2456	2458	rBV2	237	212	0.02%	0.003%
100	16.182	2475	2476	2478	rBV	261	224	0.03%	0.003%


Sum of corrected areas: 6599927

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039388.D
Acq On : 20 Dec 2023 09:46
Operator : JC/MD
Sample : VX1220WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK655

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

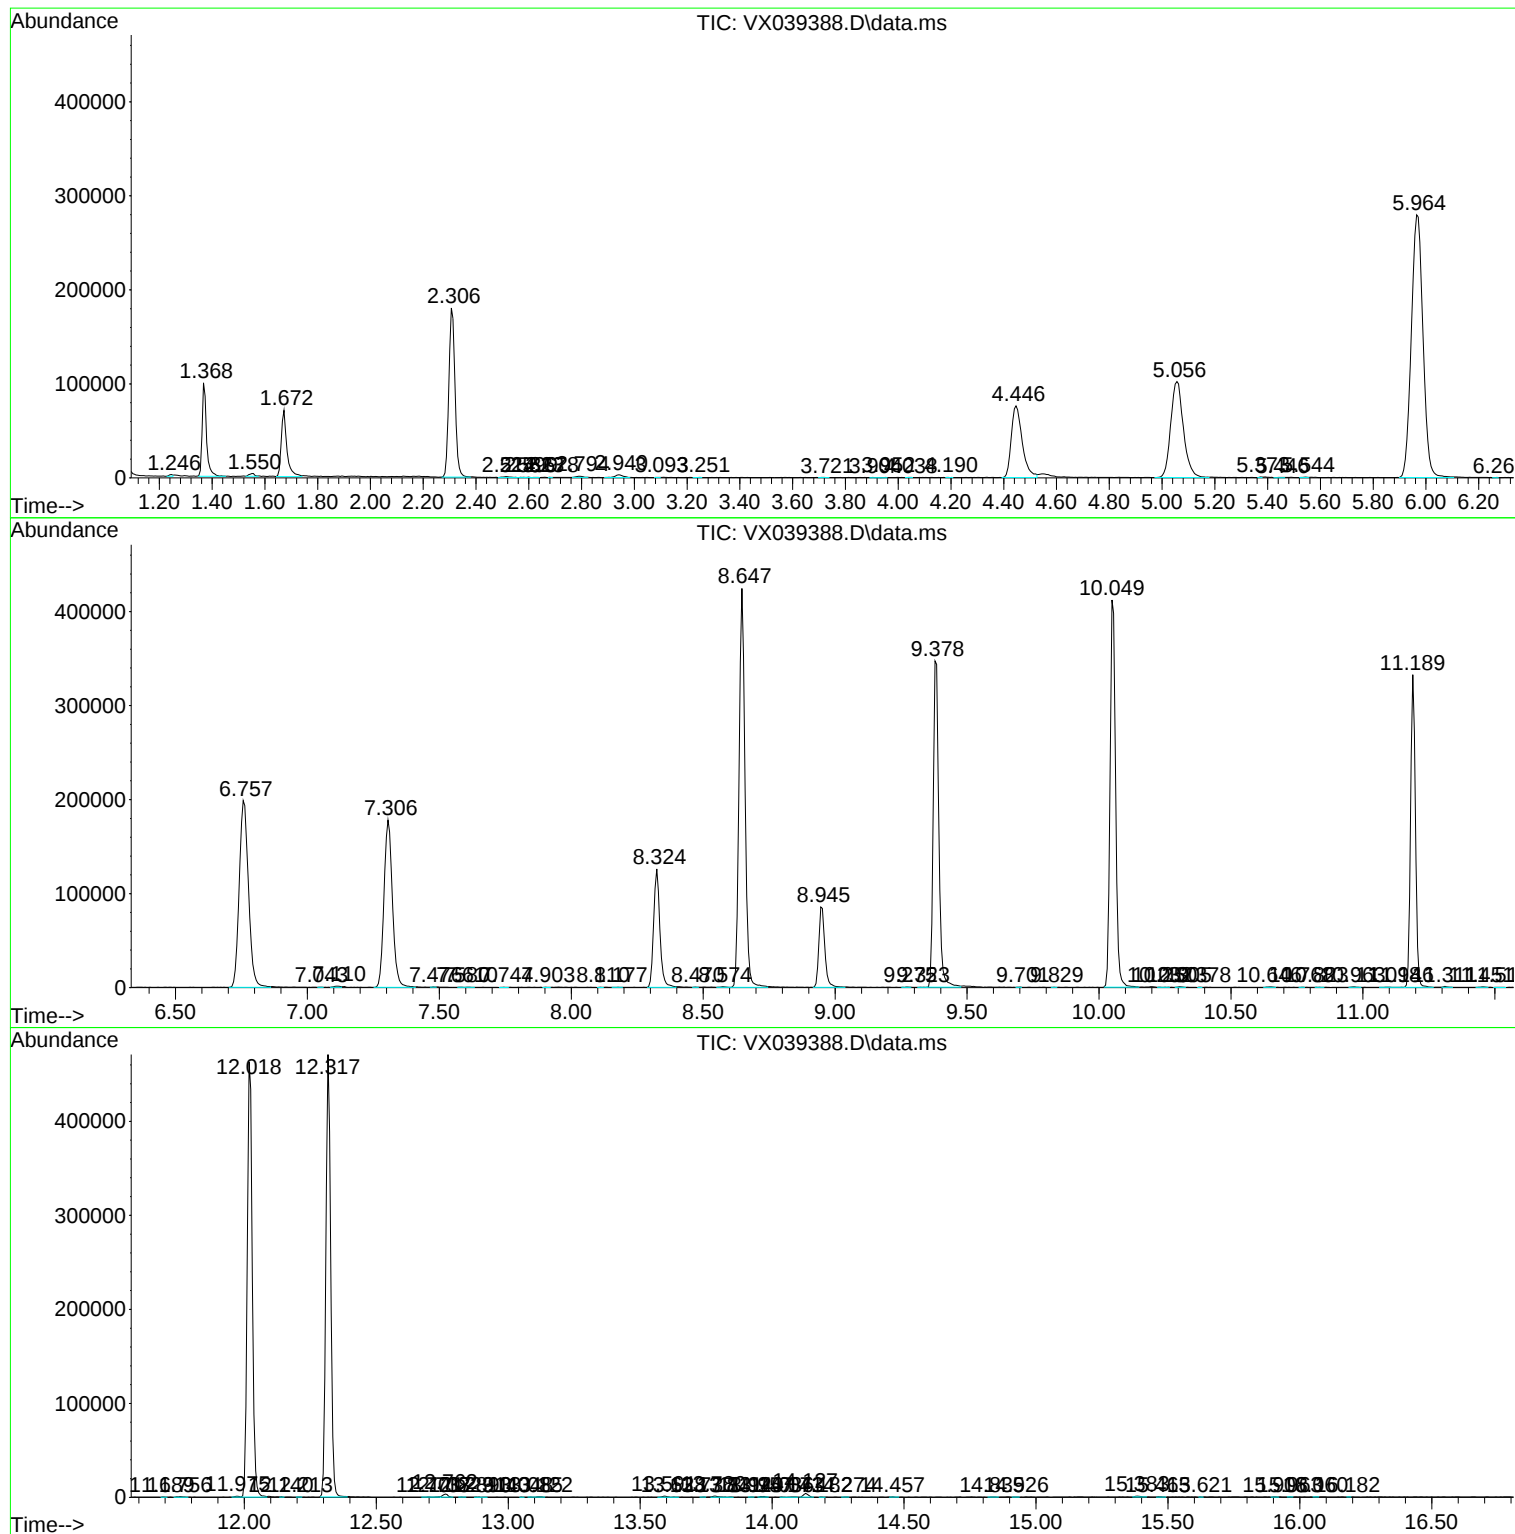

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039388.D
Acq On : 20 Dec 2023 09:46
Operator : JC/MD
Sample : VX1220WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK655

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039388.D
Acq On : 20 Dec 2023 09:46
Operator : JC/MD
Sample : VX1220WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK655

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc