

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039392.D
 Acq On : 20 Dec 2023 11:17
 Operator : JC/MD
 Sample : 05807-04 5X
 Misc : 2.46g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039392.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	23	25	27	rBV	2272	2586	0.41%	0.054%
2	1.367	43	46	57	rVB	51514	60475	9.70%	1.262%
3	1.648	89	92	102	rVB	43624	66184	10.62%	1.381%
4	2.300	192	199	209	rBV	90186	145217	23.30%	3.029%
5	2.702	261	265	271	rBV2	2839	5182	0.83%	0.108%
6	2.788	274	279	287	rVV2	3684	6674	1.07%	0.139%
7	2.940	297	304	317	rVB2	12497	30150	4.84%	0.629%
8	3.056	321	323	326	rVV	337	280	0.04%	0.006%
9	3.086	326	328	329	rVV	205	162	0.03%	0.003%
10	3.105	329	331	337	rVB3	330	540	0.09%	0.011%
11	3.355	369	372	374	rVB2	212	273	0.04%	0.006%
12	3.440	385	386	390	rBV2	113	193	0.03%	0.004%
13	3.586	407	410	414	rVV2	171	236	0.04%	0.005%
14	3.635	416	418	423	rVB2	188	188	0.03%	0.004%
15	3.720	429	432	436	rVB2	144	208	0.03%	0.004%
16	4.159	502	504	507	rBV	207	210	0.03%	0.004%
17	4.452	543	552	570	rBV	63649	187671	30.11%	3.915%
18	4.720	594	596	599	rBV2	298	270	0.04%	0.006%
19	5.056	638	651	669	rBV	77169	247786	39.75%	5.169%
20	5.263	683	685	688	rVB	210	180	0.03%	0.004%
21	5.324	692	695	699	rBV2	258	439	0.07%	0.009%
22	5.391	704	706	711	rVB4	413	583	0.09%	0.012%
23	5.495	720	723	725	rBV2	161	200	0.03%	0.004%
24	5.549	727	732	733	rBV	388	457	0.07%	0.010%
25	5.598	738	740	741	rVB2	246	164	0.03%	0.003%
26	5.793	769	772	775	rVV2	194	289	0.05%	0.006%
27	5.964	789	800	822	rBV2	204370	623296	100.00%	13.003%
28	6.177	833	835	838	rVB3	279	268	0.04%	0.006%
29	6.220	838	842	845	rBV2	169	245	0.04%	0.005%
30	6.305	852	856	857	rBV2	159	226	0.04%	0.005%
31	6.379	866	868	871	rVV2	208	175	0.03%	0.004%
32	6.586	901	902	908	rVB	217	291	0.05%	0.006%
33	6.756	921	930	946	rBV	165480	401431	64.40%	8.375%
34	7.116	984	989	995	rVB4	1294	2421	0.39%	0.051%
35	7.305	1011	1020	1035	rBV	129968	291367	46.75%	6.078%
36	7.470	1045	1047	1050	rBV3	274	438	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039392.D
 Acq On : 20 Dec 2023 11:17
 Operator : JC/MD
 Sample : 05807-04 5X
 Misc : 2.46g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.695	1082	1084	1088	rBV2	184	212	0.03%	0.004%
38	7.957	1125	1127	1129	rBV2	311	297	0.05%	0.006%
39	8.037	1136	1140	1141	rBV	190	221	0.04%	0.005%
40	8.323	1181	1187	1201	rBV	79423	134244	21.54%	2.801%
41	8.457	1208	1209	1210	rBV	461	208	0.03%	0.004%
42	8.518	1218	1219	1224	rVB2	291	266	0.04%	0.006%
43	8.573	1226	1228	1229	rVV2	237	231	0.04%	0.005%
44	8.646	1233	1240	1261	rVV	231066	371094	59.54%	7.742%
45	8.951	1284	1290	1302	rBV	59430	91850	14.74%	1.916%
46	9.158	1321	1324	1327	rBV2	196	246	0.04%	0.005%
47	9.280	1339	1344	1347	rBV	625	847	0.14%	0.018%
48	9.329	1349	1352	1354	rBV2	188	259	0.04%	0.005%
49	9.384	1356	1361	1383	rBV	299778	446042	71.56%	9.305%
50	9.707	1410	1414	1418	rVB2	1595	2210	0.35%	0.046%
51	10.055	1465	1471	1473	rBV	339700	515019	82.63%	10.744%
52	10.225	1498	1499	1503	rBV2	254	327	0.05%	0.007%
53	10.292	1509	1510	1513	rBV3	403	490	0.08%	0.010%
54	10.646	1566	1568	1574	rBV3	291	595	0.10%	0.012%
55	10.768	1586	1588	1590	rBV	208	195	0.03%	0.004%
56	10.798	1590	1593	1594	rVB	183	163	0.03%	0.003%
57	10.902	1606	1610	1612	rVB2	232	329	0.05%	0.007%
58	10.926	1612	1614	1616	rBV2	180	193	0.03%	0.004%
59	10.969	1619	1621	1625	rVB3	223	222	0.04%	0.005%
60	11.091	1636	1641	1643	rBV2	206	249	0.04%	0.005%
61	11.189	1652	1657	1670	rBV	261122	344713	55.30%	7.191%
62	11.365	1685	1686	1688	rVV	296	197	0.03%	0.004%
63	11.457	1697	1701	1704	rVV3	422	534	0.09%	0.011%
64	11.652	1732	1733	1737	rVB2	257	207	0.03%	0.004%
65	11.756	1747	1750	1754	rVB2	417	406	0.07%	0.008%
66	11.798	1754	1757	1760	rBV	158	173	0.03%	0.004%
67	11.938	1776	1780	1782	rBV2	190	224	0.04%	0.005%
68	11.975	1782	1786	1789	rBV2	2376	3005	0.48%	0.063%
69	12.024	1789	1794	1809	rVB	329055	461283	74.01%	9.623%
70	12.316	1837	1842	1851	rBV	250680	325643	52.25%	6.793%
71	12.499	1869	1872	1875	rVB2	234	225	0.04%	0.005%
72	12.755	1909	1914	1920	rBV2	1729	2493	0.40%	0.052%
73	13.200	1986	1987	1991	rBV	144	169	0.03%	0.004%
74	13.322	2005	2007	2010	rBV	202	190	0.03%	0.004%
75	13.444	2023	2027	2030	rBV2	161	320	0.05%	0.007%
76	13.511	2036	2038	2041	rVB2	274	227	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039392.D
 Acq On : 20 Dec 2023 11:17
 Operator : JC/MD
 Sample : 05807-04 5X
 Misc : 2.46g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.591	2049	2051	2053	rBV2	373	404	0.06%	0.008%
78	13.780	2079	2082	2088	rVV2	424	758	0.12%	0.016%
79	13.877	2096	2098	2100	rBV	201	232	0.04%	0.005%
80	13.956	2109	2111	2116	rBV3	340	583	0.09%	0.012%
81	14.048	2122	2126	2128	rVB	170	194	0.03%	0.004%
82	14.127	2135	2139	2143	rBV2	2654	3519	0.56%	0.073%
83	14.334	2170	2173	2177	rVB2	261	364	0.06%	0.008%
84	14.377	2179	2180	2187	rBV2	198	351	0.06%	0.007%
85	14.511	2200	2202	2204	rBV2	147	179	0.03%	0.004%
86	14.584	2212	2214	2215	rBV	182	168	0.03%	0.004%
87	14.658	2224	2226	2229	rVB	215	189	0.03%	0.004%
88	14.682	2229	2230	2234	rVV2	359	340	0.05%	0.007%
89	14.725	2234	2237	2239	rVB2	262	293	0.05%	0.006%
90	14.786	2244	2247	2249	rBV2	202	281	0.05%	0.006%
91	14.871	2260	2261	2263	rVB2	334	199	0.03%	0.004%
92	14.914	2263	2268	2270	rVB3	230	342	0.05%	0.007%
93	15.029	2284	2287	2290	rBV3	237	350	0.06%	0.007%
94	15.310	2331	2333	2334	rBV2	305	191	0.03%	0.004%
95	15.346	2337	2339	2340	rBV	240	230	0.04%	0.005%
96	15.493	2361	2363	2364	rBV2	315	201	0.03%	0.004%
97	15.670	2390	2392	2394	rBV	274	262	0.04%	0.005%
98	15.865	2422	2424	2429	rVB3	282	357	0.06%	0.007%
99	15.907	2429	2431	2433	rBV2	253	249	0.04%	0.005%
100	16.017	2448	2449	2453	rVB3	277	262	0.04%	0.005%




Sum of corrected areas: 4793471

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039392.D
Acq On : 20 Dec 2023 11:17
Operator : JC/MD
Sample : 05807-04 5X
Misc : 2.46g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

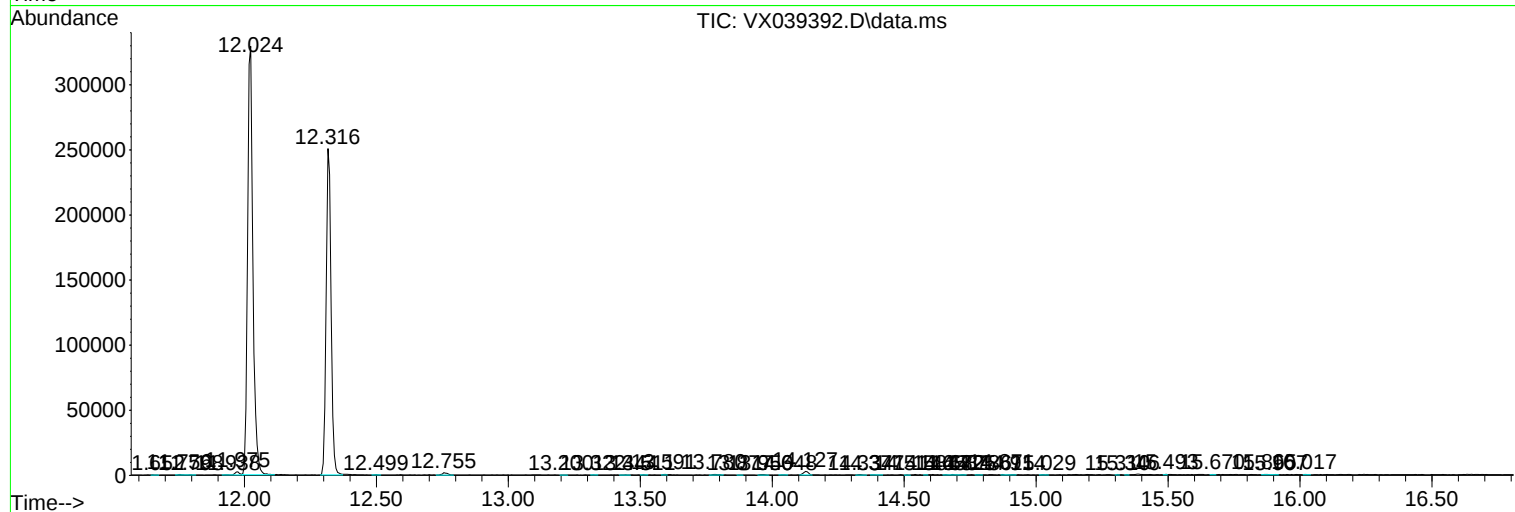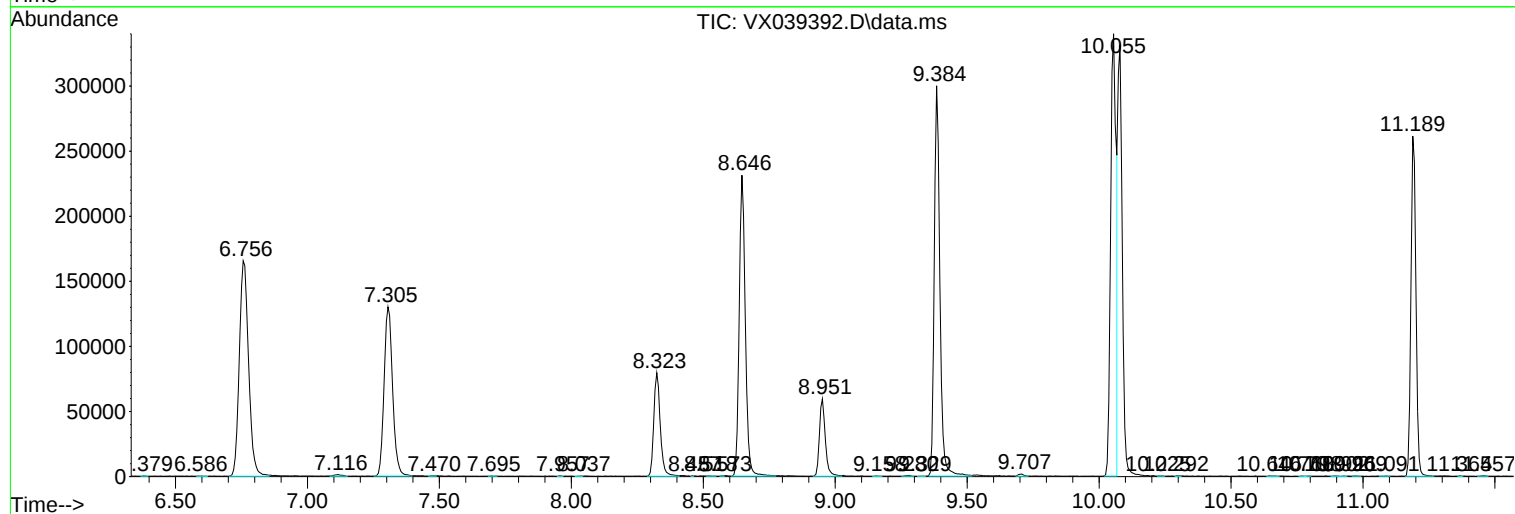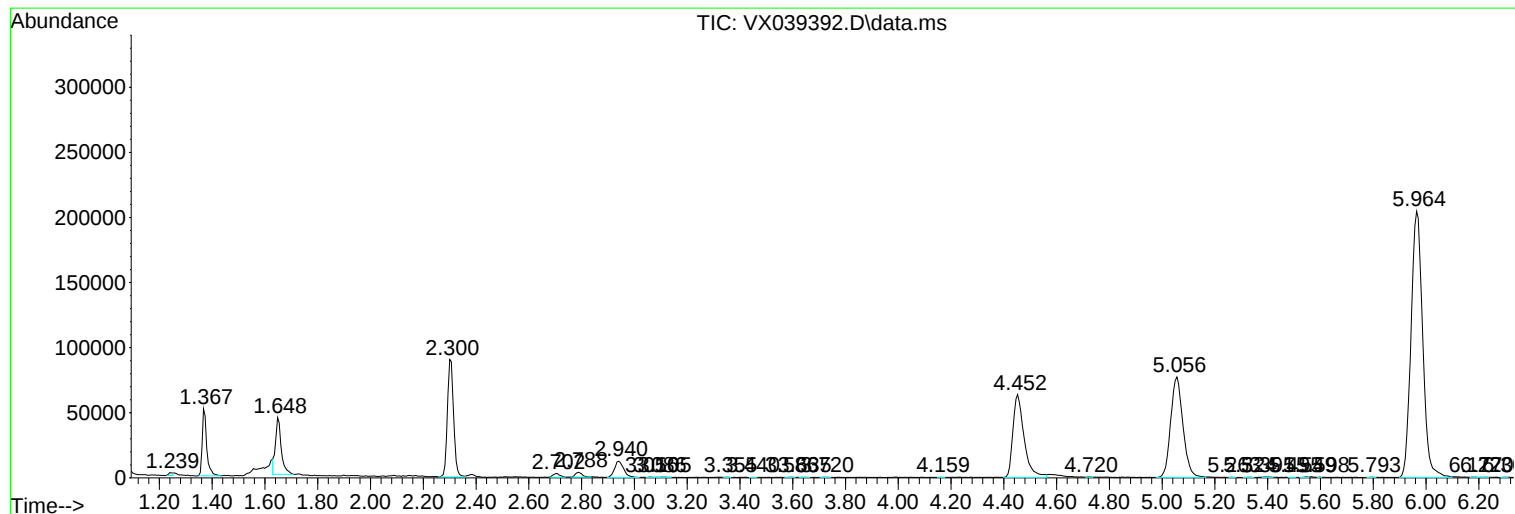

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039392.D
Acq On : 20 Dec 2023 11:17
Operator : JC/MD
Sample : 05807-04 5X
Misc : 2.46g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039392.D
Acq On : 20 Dec 2023 11:17
Operator : JC/MD
Sample : 05807-04 5X
Misc : 2.46g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc