

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039394.D
 Acq On : 20 Dec 2023 12:25
 Operator : JC/MD
 Sample : 05869-08 100X
 Misc : 3.72g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AT4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	54	rVB	56496	63431	9.79%	1.252%
2	1.672	91	96	111	rVB	45552	72140	11.14%	1.424%
3	2.306	194	200	209	rBV	102901	164065	25.33%	3.238%
4	2.520	232	235	239	rVB3	417	656	0.10%	0.013%
5	2.709	262	266	272	rVB2	247	400	0.06%	0.008%
6	2.794	275	280	287	rBV4	2098	4104	0.63%	0.081%
7	2.891	294	296	297	rBV	327	242	0.04%	0.005%
8	2.940	298	304	314	rVB2	6521	15365	2.37%	0.303%
9	3.013	314	316	318	rVB2	227	204	0.03%	0.004%
10	3.087	326	328	330	rBV2	267	275	0.04%	0.005%
11	3.349	369	371	375	rVB2	177	262	0.04%	0.005%
12	3.410	379	381	385	rVB2	192	197	0.03%	0.004%
13	3.452	385	388	389	rBV2	224	181	0.03%	0.004%
14	3.568	406	407	411	rBV	177	223	0.03%	0.004%
15	3.721	430	432	436	rVB2	217	238	0.04%	0.005%
16	3.812	445	447	450	rVB2	196	216	0.03%	0.004%
17	3.836	450	451	455	rBV2	142	178	0.03%	0.004%
18	3.879	455	458	459	rBV	187	205	0.03%	0.004%
19	3.989	474	476	480	rBV2	231	249	0.04%	0.005%
20	4.257	517	520	521	rBV2	215	253	0.04%	0.005%
21	4.446	543	551	563	rBV	65783	187141	28.90%	3.694%
22	4.861	618	619	623	rBV3	339	491	0.08%	0.010%
23	5.056	639	651	667	rBV2	80635	258890	39.98%	5.110%
24	5.470	715	719	722	rVV2	169	248	0.04%	0.005%
25	5.684	752	754	756	rBV2	201	180	0.03%	0.004%
26	5.775	767	769	773	rBV	193	235	0.04%	0.005%
27	5.964	788	800	822	rBV2	209733	647587	100.00%	12.783%
28	6.220	841	842	846	rBV2	193	201	0.03%	0.004%
29	6.757	921	930	949	rBV	174187	424032	65.48%	8.370%
30	7.037	975	976	979	rVB2	287	197	0.03%	0.004%
31	7.116	983	989	995	rVB4	1338	2986	0.46%	0.059%
32	7.214	1002	1005	1008	rBV2	134	209	0.03%	0.004%
33	7.305	1011	1020	1040	rVV	140517	309576	47.80%	6.111%
34	7.439	1040	1042	1046	rVB2	532	419	0.06%	0.008%
35	7.488	1046	1050	1052	rBV2	478	599	0.09%	0.012%
36	7.683	1081	1082	1085	rBV	325	237	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039394.D
 Acq On : 20 Dec 2023 12:25
 Operator : JC/MD
 Sample : 05869-08 100X
 Misc : 3.72g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COAT4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.744	1089	1092	1095	rVB2	185	267	0.04%	0.005%
38	8.025	1136	1138	1141	rBV	254	221	0.03%	0.004%
39	8.208	1163	1168	1170	rBV2	181	215	0.03%	0.004%
40	8.323	1181	1187	1197	rBV	88727	144838	22.37%	2.859%
41	8.506	1215	1217	1221	rVB	249	289	0.04%	0.006%
42	8.646	1234	1240	1258	rBV	274489	436047	67.33%	8.607%
43	8.890	1278	1280	1284	rVB	182	255	0.04%	0.005%
44	8.951	1284	1290	1304	rBV	61860	98736	15.25%	1.949%
45	9.116	1313	1317	1319	rVB3	424	448	0.07%	0.009%
46	9.140	1319	1321	1322	rBV	261	183	0.03%	0.004%
47	9.183	1326	1328	1333	rVB2	163	199	0.03%	0.004%
48	9.268	1340	1342	1346	rVB3	311	362	0.06%	0.007%
49	9.384	1355	1361	1377	rBV	300310	442949	68.40%	8.743%
50	9.695	1409	1412	1418	rVB2	1335	1815	0.28%	0.036%
51	9.933	1449	1451	1454	rVB2	204	179	0.03%	0.004%
52	10.000	1461	1462	1465	rBV	184	229	0.04%	0.005%
53	10.055	1465	1471	1486	rBV	359841	526818	81.35%	10.399%
54	10.201	1492	1495	1498	rBV3	330	398	0.06%	0.008%
55	10.305	1509	1512	1517	rVB3	399	443	0.07%	0.009%
56	10.353	1519	1520	1524	rBV2	208	216	0.03%	0.004%
57	10.646	1564	1568	1570	rBV2	563	495	0.08%	0.010%
58	10.731	1580	1582	1583	rBV	319	182	0.03%	0.004%
59	10.963	1617	1620	1624	rBV3	292	341	0.05%	0.007%
60	11.085	1638	1640	1642	rBV2	201	178	0.03%	0.004%
61	11.189	1652	1657	1666	rBV	269153	344318	53.17%	6.796%
62	11.311	1675	1677	1681	rBV3	454	424	0.07%	0.008%
63	11.366	1681	1686	1690	rBV2	1956	2460	0.38%	0.049%
64	11.451	1696	1700	1703	rBV4	455	641	0.10%	0.013%
65	11.628	1726	1729	1731	rBV	311	229	0.04%	0.005%
66	11.762	1747	1751	1755	rBV2	472	643	0.10%	0.013%
67	11.975	1781	1786	1788	rBV2	470	632	0.10%	0.012%
68	12.018	1788	1793	1805	rBV	372973	500857	77.34%	9.886%
69	12.280	1834	1836	1837	rBV	282	222	0.03%	0.004%
70	12.317	1837	1842	1853	rVV	304792	388884	60.05%	7.676%
71	12.390	1853	1854	1855	rBV	560	250	0.04%	0.005%
72	12.615	1890	1891	1894	rVB2	242	210	0.03%	0.004%
73	12.713	1905	1907	1911	rBV2	153	195	0.03%	0.004%
74	12.762	1911	1915	1919	rVB3	1401	2098	0.32%	0.041%
75	12.823	1924	1925	1927	rBV	263	239	0.04%	0.005%
76	12.926	1941	1942	1947	rBV2	277	223	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039394.D
 Acq On : 20 Dec 2023 12:25
 Operator : JC/MD
 Sample : 05869-08 100X
 Misc : 3.72g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AT4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.493	2032	2035	2038	rVB	257	294	0.05%	0.006%
78	13.676	2064	2065	2068	rBV2	224	227	0.04%	0.004%
79	13.761	2075	2079	2080	rBV	176	230	0.04%	0.005%
80	13.963	2110	2112	2116	rVB	371	343	0.05%	0.007%
81	14.127	2134	2139	2143	rVB	3041	3731	0.58%	0.074%
82	14.298	2162	2167	2170	rVB2	166	232	0.04%	0.005%
83	14.328	2170	2172	2176	rVB2	244	248	0.04%	0.005%
84	14.377	2176	2180	2186	rBV	276	592	0.09%	0.012%
85	14.469	2192	2195	2196	rBV	282	300	0.05%	0.006%
86	14.688	2229	2231	2234	rVB3	218	196	0.03%	0.004%
87	14.749	2238	2241	2243	rVV2	302	279	0.04%	0.006%
88	14.834	2253	2255	2256	rBV	336	272	0.04%	0.005%
89	14.938	2267	2272	2273	rBV2	206	285	0.04%	0.006%
90	15.029	2285	2287	2288	rBV2	242	184	0.03%	0.004%
91	15.048	2288	2290	2293	rVV3	213	247	0.04%	0.005%
92	15.383	2343	2345	2350	rVB4	717	1109	0.17%	0.022%
93	15.846	2420	2421	2424	rBV2	422	370	0.06%	0.007%
94	16.279	2490	2492	2493	rVB2	415	270	0.04%	0.005%
95	16.304	2493	2496	2497	rBV3	277	301	0.05%	0.006%
96	16.340	2499	2502	2503	rVV2	243	189	0.03%	0.004%
97	16.383	2507	2509	2513	rVV3	277	316	0.05%	0.006%
98	16.578	2538	2541	2542	rBV2	294	277	0.04%	0.005%
99	16.688	2558	2559	2561	rBV	403	247	0.04%	0.005%
100	16.736	2566	2567	2569	rBV2	344	258	0.04%	0.005%




Sum of corrected areas: 5066137

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039394.D
Acq On : 20 Dec 2023 12:25
Operator : JC/MD
Sample : 05869-08 100X
Misc : 3.72g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AT4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

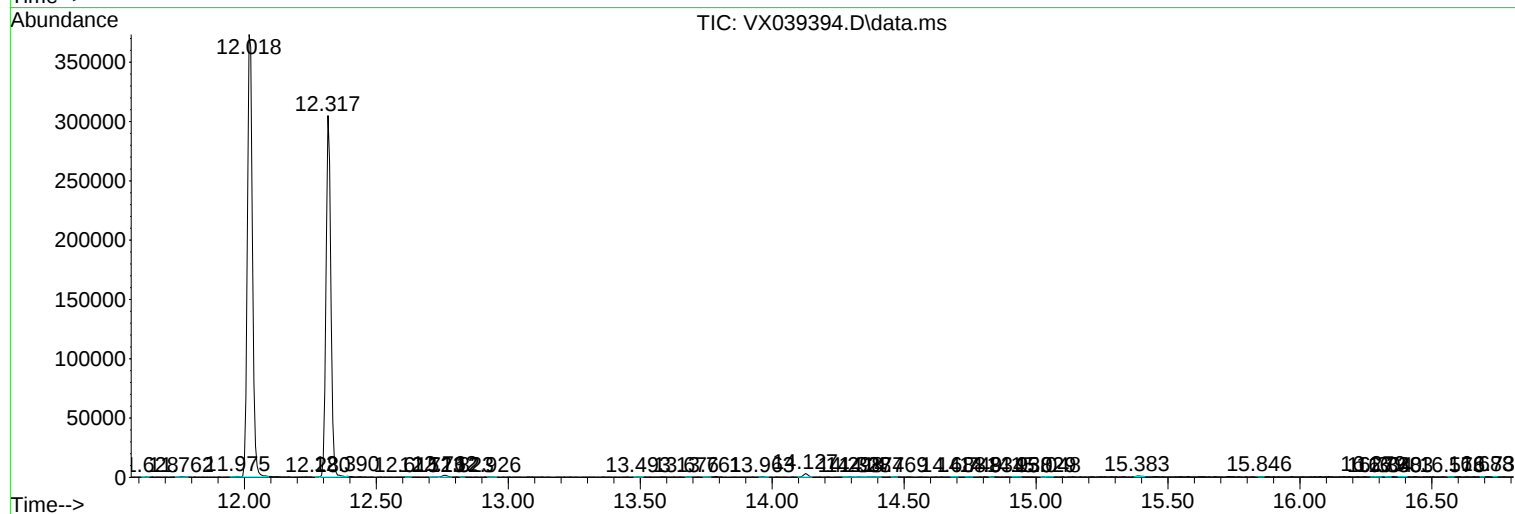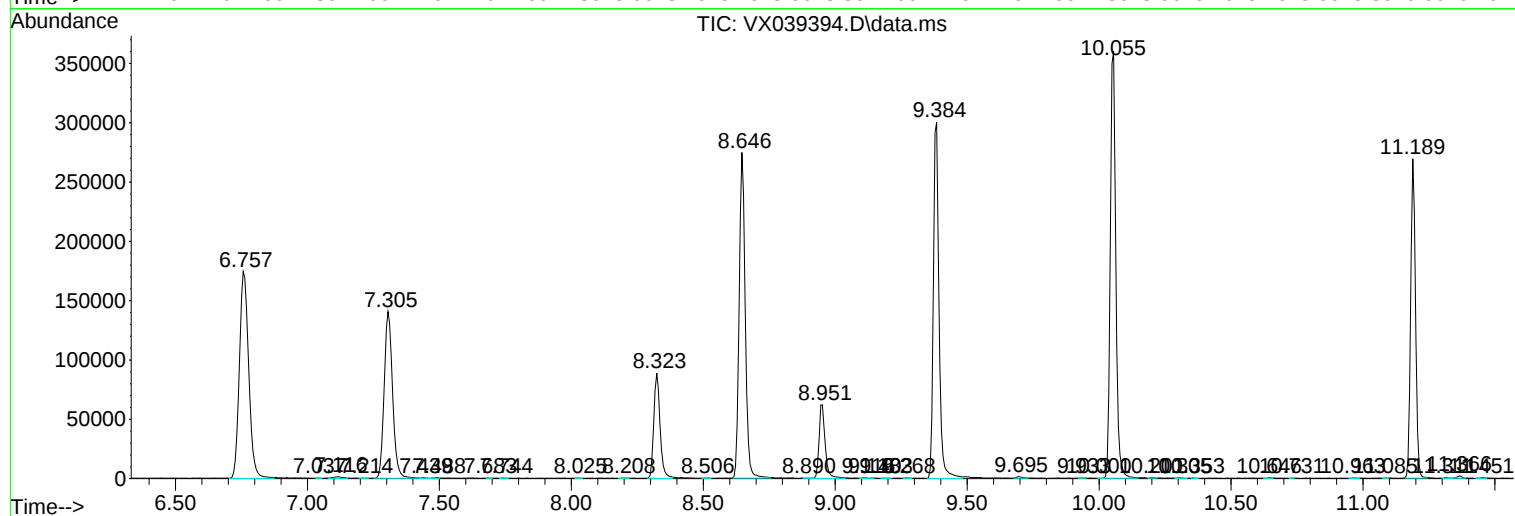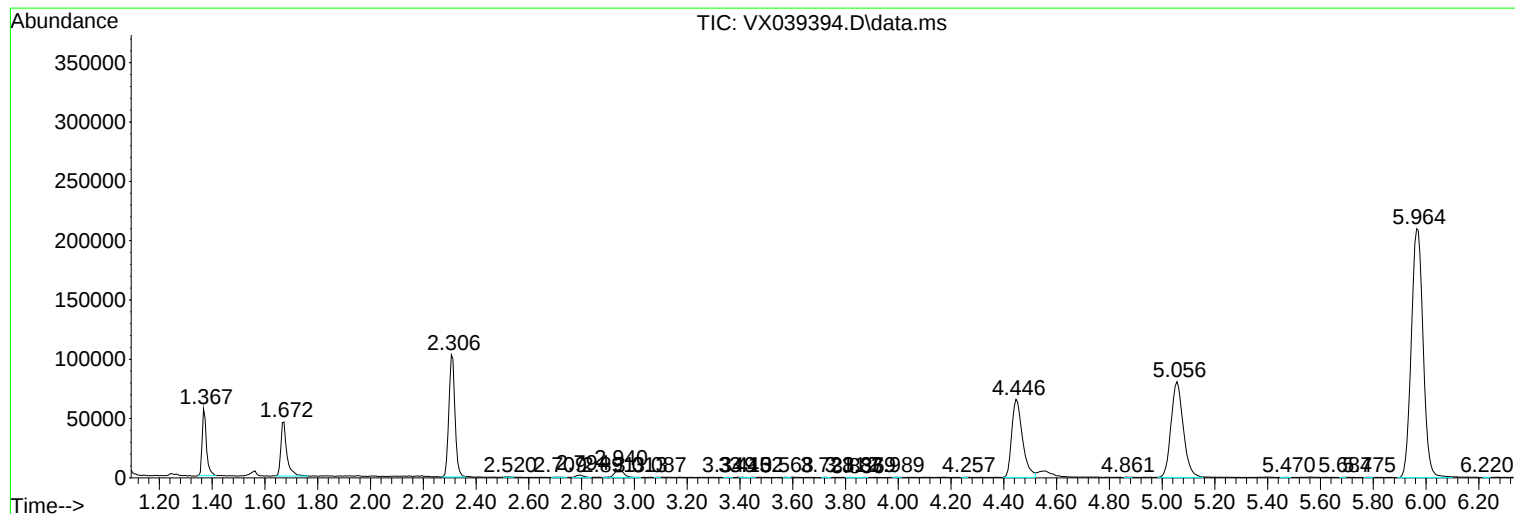

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039394.D
Acq On : 20 Dec 2023 12:25
Operator : JC/MD
Sample : 05869-08 100X
Misc : 3.72g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AT4










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.323	17.08 ug/L	144838	1,4-Difluorobenzene	6.757

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	25
2			.alpha.,.alpha.-Dichloromethyl m...	114	C2H4Cl2O	004885-02-3	25
3			1,3-Cyclohexadiene	80	C6H8	000592-57-4	25
4			1,3,5-Hexatriene	80	C6H8	002235-12-3	25
5			Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	23

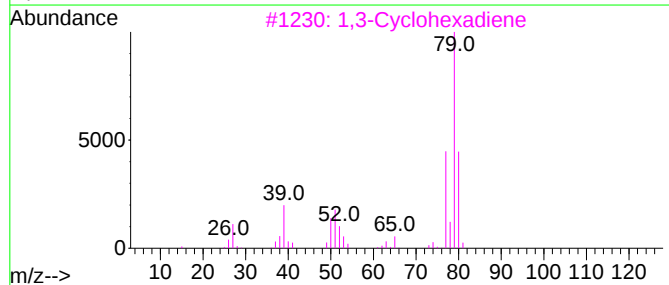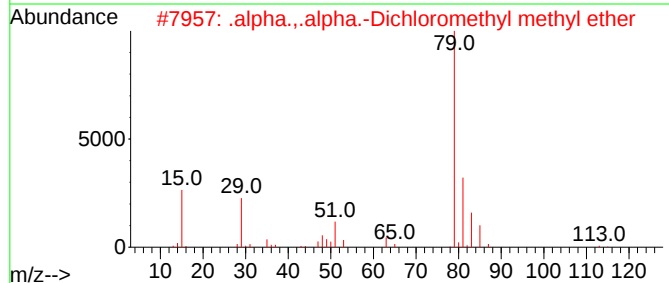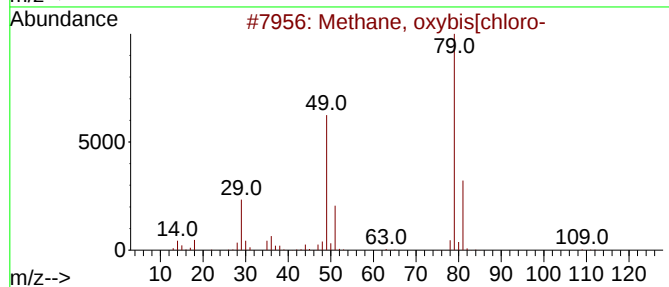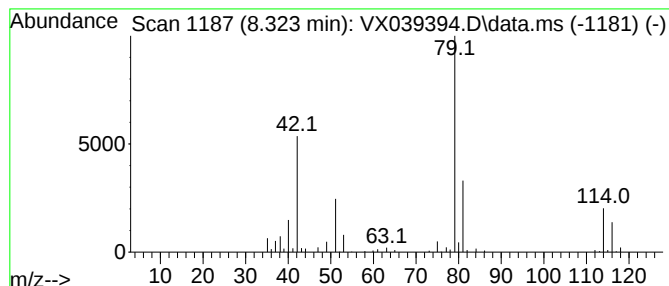

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039394.D
Acq On : 20 Dec 2023 12:25
Operator : JC/MD
Sample : 05869-08 100X
Misc : 3.72g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AT4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	8.323	17.1	ug/L	144838	1	6.757	424032	50.0