

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039405.D
 Acq On : 20 Dec 2023 16:36
 Operator : JC/MD
 Sample : 05835-18DL 500X
 Misc : 3.34g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039405.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	54	rVB	58986	60533	5.32%	1.041%
2	1.672	91	96	108	rVB	46162	67277	5.91%	1.157%
3	2.306	194	200	210	rBV	96403	151342	13.29%	2.604%
4	2.465	224	226	227	rBV	291	138	0.01%	0.002%
5	2.666	254	259	268	rVB	2973	5476	0.48%	0.094%
6	2.788	273	279	288	rBV	6971	13535	1.19%	0.233%
7	2.892	293	296	297	rBV2	141	133	0.01%	0.002%
8	2.940	297	304	314	rVB	7041	16019	1.41%	0.276%
9	3.014	314	316	319	rBV	227	317	0.03%	0.005%
10	3.087	322	328	331	rBV2	292	605	0.05%	0.010%
11	3.282	358	360	363	rBV	164	139	0.01%	0.002%
12	3.361	371	373	375	rBV	218	152	0.01%	0.003%
13	3.672	422	424	427	rBV2	195	191	0.02%	0.003%
14	3.904	460	462	463	rBV	269	163	0.01%	0.003%
15	4.062	486	488	489	rBV	184	142	0.01%	0.002%
16	4.172	504	506	507	rBV	239	142	0.01%	0.002%
17	4.446	543	551	562	rBV	64888	182589	16.04%	3.141%
18	4.897	622	625	628	rBV2	222	369	0.03%	0.006%
19	4.958	633	635	636	rBV	164	134	0.01%	0.002%
20	4.977	636	638	639	rBV	214	139	0.01%	0.002%
21	5.056	640	651	671	rVB2	77046	248989	21.87%	4.284%
22	5.385	703	705	707	rBV2	289	248	0.02%	0.004%
23	5.477	718	720	721	rBV	229	151	0.01%	0.003%
24	5.544	729	731	732	rBV2	318	312	0.03%	0.005%
25	5.659	748	750	752	rBV2	166	135	0.01%	0.002%
26	5.739	761	763	765	rBV2	199	215	0.02%	0.004%
27	5.806	773	774	776	rBV	231	162	0.01%	0.003%
28	5.964	788	800	821	rBV2	203540	627115	55.09%	10.789%
29	6.476	881	884	886	rBV2	184	279	0.02%	0.005%
30	6.757	922	930	945	rBV	168902	406072	35.67%	6.986%
31	7.019	971	973	975	rBV2	300	351	0.03%	0.006%
32	7.117	983	989	996	rVB3	1600	3341	0.29%	0.057%
33	7.245	1006	1010	1011	rBV2	165	202	0.02%	0.003%
34	7.306	1011	1020	1034	rBV	137370	298193	26.19%	5.130%
35	7.513	1052	1054	1056	rBV2	258	170	0.01%	0.003%
36	7.738	1088	1091	1092	rVB	258	188	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039405.D
 Acq On : 20 Dec 2023 16:36
 Operator : JC/MD
 Sample : 05835-18DL 500X
 Misc : 3.34g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.885	1113	1115	1117	rVV	308	196	0.02%	0.003%
38	7.933	1121	1123	1124	rBV2	235	216	0.02%	0.004%
39	8.019	1136	1137	1142	rVB2	210	271	0.02%	0.005%
40	8.092	1145	1149	1150	rBV2	136	154	0.01%	0.003%
41	8.183	1162	1164	1165	rBV	242	173	0.02%	0.003%
42	8.324	1181	1187	1199	rBV	79243	135187	11.87%	2.326%
43	8.561	1224	1226	1227	rBV	263	235	0.02%	0.004%
44	8.647	1234	1240	1260	rBV	251541	395946	34.78%	6.812%
45	8.952	1284	1290	1307	rBV	61795	92648	8.14%	1.594%
46	9.116	1314	1317	1320	rVB	182	231	0.02%	0.004%
47	9.275	1340	1343	1344	rBV2	326	283	0.02%	0.005%
48	9.384	1355	1361	1378	rBV	295441	433700	38.10%	7.462%
49	9.653	1403	1405	1406	rVB2	263	142	0.01%	0.002%
50	9.701	1408	1413	1416	rVV2	1074	1706	0.15%	0.029%
51	9.866	1438	1440	1441	rVB2	233	138	0.01%	0.002%
52	10.055	1465	1471	1486	rBV2	347983	638095	56.05%	10.978%
53	10.177	1489	1491	1492	rBV2	200	132	0.01%	0.002%
54	10.232	1498	1500	1502	rVB	318	193	0.02%	0.003%
55	10.354	1518	1520	1522	rBV	167	179	0.02%	0.003%
56	10.482	1539	1541	1544	rVB	216	181	0.02%	0.003%
57	10.531	1548	1549	1551	rBV	254	190	0.02%	0.003%
58	10.640	1565	1567	1571	rVB	331	340	0.03%	0.006%
59	10.945	1615	1617	1619	rBV2	143	148	0.01%	0.003%
60	10.969	1619	1621	1624	rVB2	393	297	0.03%	0.005%
61	11.189	1652	1657	1666	rVV	259942	342700	30.10%	5.896%
62	11.274	1669	1671	1674	rVV2	361	360	0.03%	0.006%
63	11.317	1677	1678	1682	rVB	619	426	0.04%	0.007%
64	11.366	1684	1686	1687	rBV	213	162	0.01%	0.003%
65	11.421	1693	1695	1698	rBV2	150	156	0.01%	0.003%
66	11.451	1698	1700	1703	rBV	230	276	0.02%	0.005%
67	11.549	1713	1716	1717	rBV2	208	237	0.02%	0.004%
68	11.762	1748	1751	1754	rVB2	259	262	0.02%	0.005%
69	11.799	1754	1757	1759	rBV2	113	155	0.01%	0.003%
70	11.969	1781	1785	1788	rVV3	8510	10877	0.96%	0.187%
71	12.036	1788	1796	1815	rVB2	567857	1138420	100.00%	19.586%
72	12.177	1815	1819	1822	rBV3	312	532	0.05%	0.009%
73	12.317	1837	1842	1856	rBV	282784	398393	35.00%	6.854%
74	12.585	1884	1886	1888	rBV2	165	196	0.02%	0.003%
75	12.652	1895	1897	1900	rBV2	146	152	0.01%	0.003%
76	12.762	1911	1915	1922	rVV2	2237	3211	0.28%	0.055%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039405.D
 Acq On : 20 Dec 2023 16:36
 Operator : JC/MD
 Sample : 05835-18DL 500X
 Misc : 3.34g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.847	1926	1929	1932	rBV	150	211	0.02%	0.004%
78	12.878	1932	1934	1935	rVB	237	144	0.01%	0.002%
79	12.939	1941	1944	1945	rBV	189	181	0.02%	0.003%
80	12.981	1950	1951	1955	rBV2	211	234	0.02%	0.004%
81	13.067	1960	1965	1970	rVB3	1427	2335	0.21%	0.040%
82	13.115	1970	1973	1976	rBV	392	426	0.04%	0.007%
83	13.341	2008	2010	2012	rBV	138	135	0.01%	0.002%
84	13.384	2016	2017	2020	rBV	206	196	0.02%	0.003%
85	13.585	2046	2050	2058	rBV	46622	57780	5.08%	0.994%
86	13.786	2079	2083	2086	rVB2	514	786	0.07%	0.014%
87	13.878	2097	2098	2101	rBV2	216	209	0.02%	0.004%
88	13.957	2106	2111	2117	rBV	38209	50305	4.42%	0.865%
89	14.127	2133	2139	2146	rBV2	3559	4913	0.43%	0.085%
90	14.408	2182	2185	2186	rBV2	133	135	0.01%	0.002%
91	14.591	2214	2215	2217	rBV	317	219	0.02%	0.004%
92	14.774	2241	2245	2249	rVB4	771	1334	0.12%	0.023%
93	15.036	2285	2288	2289	rBV2	398	333	0.03%	0.006%
94	15.188	2311	2313	2315	rBV2	296	243	0.02%	0.004%
95	15.249	2318	2323	2328	rBV4	5358	7746	0.68%	0.133%
96	15.517	2366	2367	2369	rBV2	268	197	0.02%	0.003%
97	16.097	2459	2462	2464	rBV2	349	349	0.03%	0.006%
98	16.164	2471	2473	2476	rBV2	352	323	0.03%	0.006%
99	16.444	2518	2519	2521	rVB2	321	180	0.02%	0.003%
100	16.761	2569	2571	2572	rBV2	473	368	0.03%	0.006%

Sum of corrected areas: 5812436




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039405.D
Acq On : 20 Dec 2023 16:36
Operator : JC/MD
Sample : 05835-18DL 500X
Misc : 3.34g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

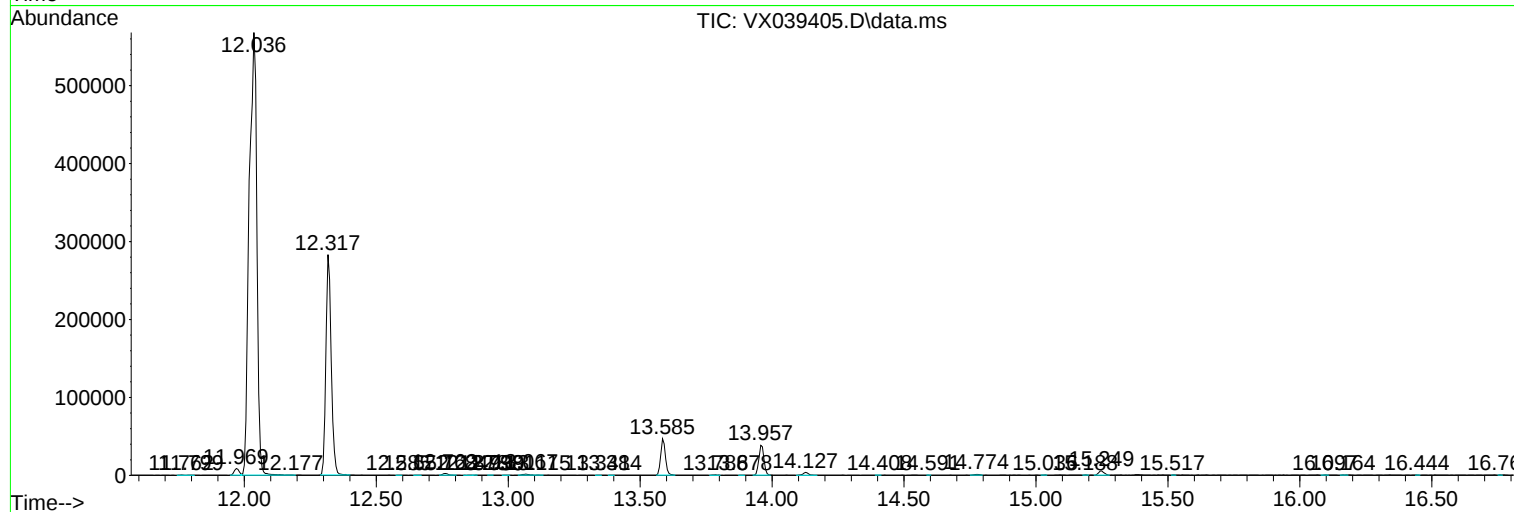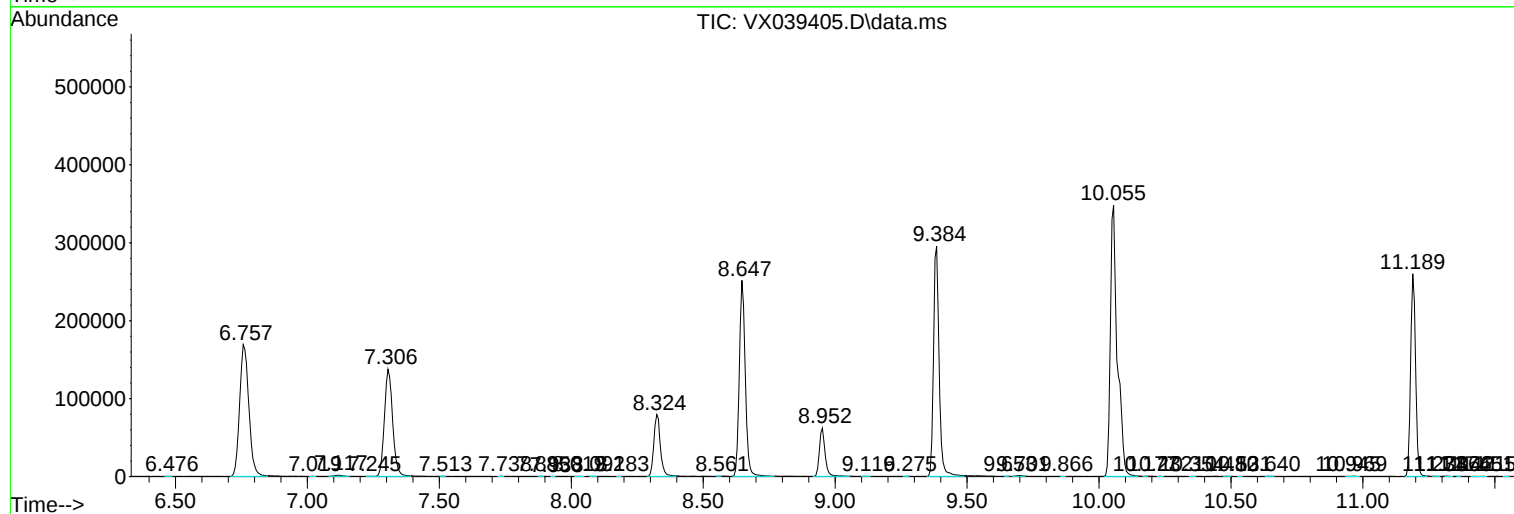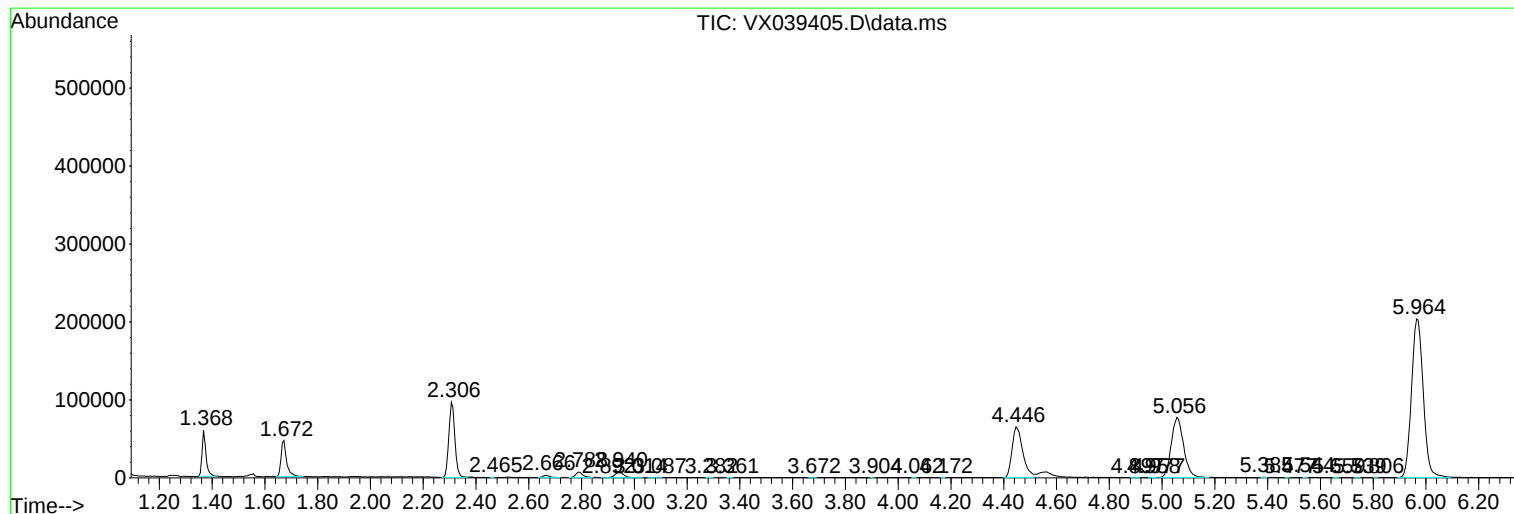

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039405.D
Acq On : 20 Dec 2023 16:36
Operator : JC/MD
Sample : 05835-18DL 500X
Misc : 3.34g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039405.D
Acq On : 20 Dec 2023 16:36
Operator : JC/MD
Sample : 05835-18DL 500X
Misc : 3.34g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc