

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039407.D
 Acq On : 20 Dec 2023 17:22
 Operator : JC/MD
 Sample : 05794-23ME
 Misc : 4.25g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGRG4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039407.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	63	rVB	51435	92713	12.71%	1.681%
2	1.648	89	92	101	rBV	17132	35940	4.93%	0.652%
3	2.282	190	196	205	rBV	132409	228608	31.35%	4.146%
4	2.788	273	279	283	rBV4	2335	4518	0.62%	0.082%
5	2.941	298	304	314	rBV	7157	17611	2.41%	0.319%
6	3.270	356	358	361	rVB2	199	207	0.03%	0.004%
7	3.325	365	367	371	rBV2	360	331	0.05%	0.006%
8	3.428	382	384	388	rVB2	941	961	0.13%	0.017%
9	4.489	548	558	581	rBV2	35335	174794	23.97%	3.170%
10	5.056	639	651	670	rBV	88431	284782	39.05%	5.165%
11	5.343	697	698	701	rBV	214	235	0.03%	0.004%
12	5.397	703	707	711	rVB	474	651	0.09%	0.012%
13	5.434	711	713	715	rBV2	265	210	0.03%	0.004%
14	5.519	725	727	728	rBV	318	216	0.03%	0.004%
15	5.623	742	744	747	rBV2	208	286	0.04%	0.005%
16	5.800	770	773	776	rBV	265	235	0.03%	0.004%
17	5.964	789	800	820	rBV2	251190	729282	100.00%	13.226%
18	6.190	836	837	841	rVB	417	333	0.05%	0.006%
19	6.245	841	846	848	rBV2	230	313	0.04%	0.006%
20	6.263	848	849	854	rVV2	167	196	0.03%	0.004%
21	6.373	860	867	876	rVV4	1323	3962	0.54%	0.072%
22	6.525	890	892	894	rVB2	243	203	0.03%	0.004%
23	6.757	920	930	946	rBV	177758	447747	61.40%	8.120%
24	7.123	983	990	999	rBV7	1369	4599	0.63%	0.083%
25	7.214	999	1005	1006	rBV2	2342	3685	0.51%	0.067%
26	7.306	1012	1020	1032	rBV2	145338	328207	45.00%	5.952%
27	7.446	1041	1043	1045	rBV	278	254	0.03%	0.005%
28	7.495	1048	1051	1056	rVB4	502	746	0.10%	0.014%
29	7.641	1072	1075	1079	rBV	251	404	0.06%	0.007%
30	7.964	1124	1128	1130	rBV4	635	854	0.12%	0.015%
31	8.086	1146	1148	1155	rVB3	497	808	0.11%	0.015%
32	8.135	1155	1156	1161	rBV2	204	249	0.03%	0.005%
33	8.220	1167	1170	1174	rBB2	187	264	0.04%	0.005%
34	8.263	1174	1177	1179	rBV2	266	234	0.03%	0.004%
35	8.324	1181	1187	1198	rBV	82119	152906	20.97%	2.773%
36	8.592	1227	1231	1233	rBV	285	335	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039407.D
 Acq On : 20 Dec 2023 17:22
 Operator : JC/MD
 Sample : 05794-23ME
 Misc : 4.25g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGRG4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	8.647	1234	1240	1251	rBV	336502	554882	76.09%	10.063%
38	8.848	1271	1273	1274	rBV2	404	300	0.04%	0.005%
39	8.952	1285	1290	1301	rBV	59098	100018	13.71%	1.814%
40	9.110	1314	1316	1319	rBV3	423	477	0.07%	0.009%
41	9.397	1357	1363	1380	rVV	209789	408001	55.95%	7.399%
42	9.695	1410	1412	1413	rBV2	363	353	0.05%	0.006%
43	9.708	1413	1414	1422	rVB4	1069	1595	0.22%	0.029%
44	10.055	1465	1471	1488	rBV	360694	526001	72.13%	9.539%
45	10.195	1492	1494	1496	rBV3	430	343	0.05%	0.006%
46	10.244	1499	1502	1505	rVB2	253	382	0.05%	0.007%
47	10.305	1508	1512	1513	rBV3	451	435	0.06%	0.008%
48	10.512	1542	1546	1547	rVB2	281	287	0.04%	0.005%
49	10.537	1547	1550	1552	rBV2	182	220	0.03%	0.004%
50	10.628	1561	1565	1566	rBV2	183	205	0.03%	0.004%
51	10.646	1566	1568	1571	rVV2	426	415	0.06%	0.008%
52	10.842	1596	1600	1602	rBV	266	289	0.04%	0.005%
53	10.890	1605	1608	1611	rVB2	222	285	0.04%	0.005%
54	10.963	1618	1620	1624	rVB2	305	415	0.06%	0.008%
55	11.037	1628	1632	1633	rBV2	150	219	0.03%	0.004%
56	11.098	1639	1642	1643	rBV2	204	204	0.03%	0.004%
57	11.122	1643	1646	1652	rVB2	510	561	0.08%	0.010%
58	11.195	1652	1658	1664	rBV	253750	332139	45.54%	6.024%
59	11.311	1673	1677	1681	rVB4	1420	1955	0.27%	0.035%
60	11.421	1694	1695	1699	rBV2	220	242	0.03%	0.004%
61	11.591	1721	1723	1725	rVB2	435	337	0.05%	0.006%
62	11.634	1725	1730	1735	rBV4	661	854	0.12%	0.015%
63	11.683	1735	1738	1741	rBV2	769	740	0.10%	0.013%
64	11.756	1747	1750	1754	rVV3	397	607	0.08%	0.011%
65	11.872	1768	1769	1772	rVB2	289	254	0.03%	0.005%
66	11.969	1784	1785	1788	rVB2	629	524	0.07%	0.010%
67	12.024	1789	1794	1804	rVV	433085	543963	74.59%	9.865%
68	12.116	1807	1809	1810	rBV2	359	231	0.03%	0.004%
69	12.219	1823	1826	1828	rBV2	267	317	0.04%	0.006%
70	12.256	1831	1832	1837	rBV	217	215	0.03%	0.004%
71	12.323	1837	1843	1853	rBV	366929	489836	67.17%	8.883%
72	12.664	1898	1899	1902	rBV	238	206	0.03%	0.004%
73	12.762	1910	1915	1920	rBV2	4767	6320	0.87%	0.115%
74	13.030	1956	1959	1962	rBV2	435	547	0.08%	0.010%
75	13.073	1964	1966	1970	rVB2	260	286	0.04%	0.005%
76	13.122	1970	1974	1978	rBV2	389	479	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039407.D
 Acq On : 20 Dec 2023 17:22
 Operator : JC/MD
 Sample : 05794-23ME
 Misc : 4.25g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGRG4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.170	1980	1982	1985	rBV	216	252	0.03%	0.005%
78	13.213	1985	1989	1991	rVV	195	253	0.03%	0.005%
79	13.237	1991	1993	1995	rVV2	179	201	0.03%	0.004%
80	13.445	2022	2027	2028	rBV2	265	288	0.04%	0.005%
81	13.518	2033	2039	2042	rVB2	262	410	0.06%	0.007%
82	13.597	2047	2052	2056	rVB3	538	877	0.12%	0.016%
83	13.786	2079	2083	2089	rBV2	464	759	0.10%	0.014%
84	13.835	2089	2091	2093	rVB	264	238	0.03%	0.004%
85	13.969	2108	2113	2117	rBV4	434	721	0.10%	0.013%
86	14.128	2135	2139	2143	rBV2	7191	9555	1.31%	0.173%
87	14.390	2181	2182	2186	rVV	294	224	0.03%	0.004%
88	14.432	2186	2189	2191	rVV2	212	269	0.04%	0.005%
89	14.603	2214	2217	2219	rVB2	263	203	0.03%	0.004%
90	15.146	2304	2306	2308	rBV3	363	290	0.04%	0.005%
91	15.390	2340	2346	2352	rVB4	1575	2704	0.37%	0.049%
92	15.487	2358	2362	2364	rBV3	424	521	0.07%	0.009%
93	15.572	2374	2376	2377	rBV	343	214	0.03%	0.004%
94	15.621	2382	2384	2386	rVB2	465	342	0.05%	0.006%
95	15.652	2387	2389	2392	rBV2	247	215	0.03%	0.004%
96	16.097	2459	2462	2465	rBV	228	263	0.04%	0.005%
97	16.371	2504	2507	2508	rBV2	208	221	0.03%	0.004%
98	16.621	2546	2548	2553	rVB3	370	599	0.08%	0.011%
99	16.664	2553	2555	2559	rVB3	277	329	0.05%	0.006%
100	16.700	2559	2561	2562	rBV2	316	285	0.04%	0.005%




Sum of corrected areas: 5514051

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039407.D
Acq On : 20 Dec 2023 17:22
Operator : JC/MD
Sample : 05794-23ME
Misc : 4.25g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGRG4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

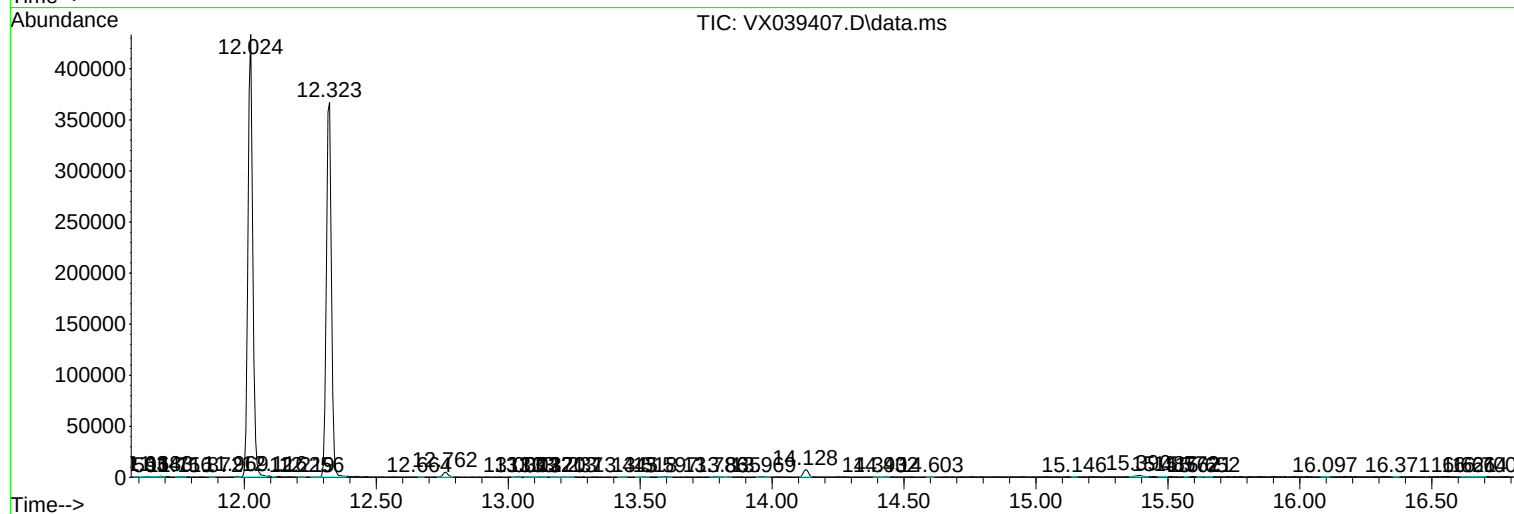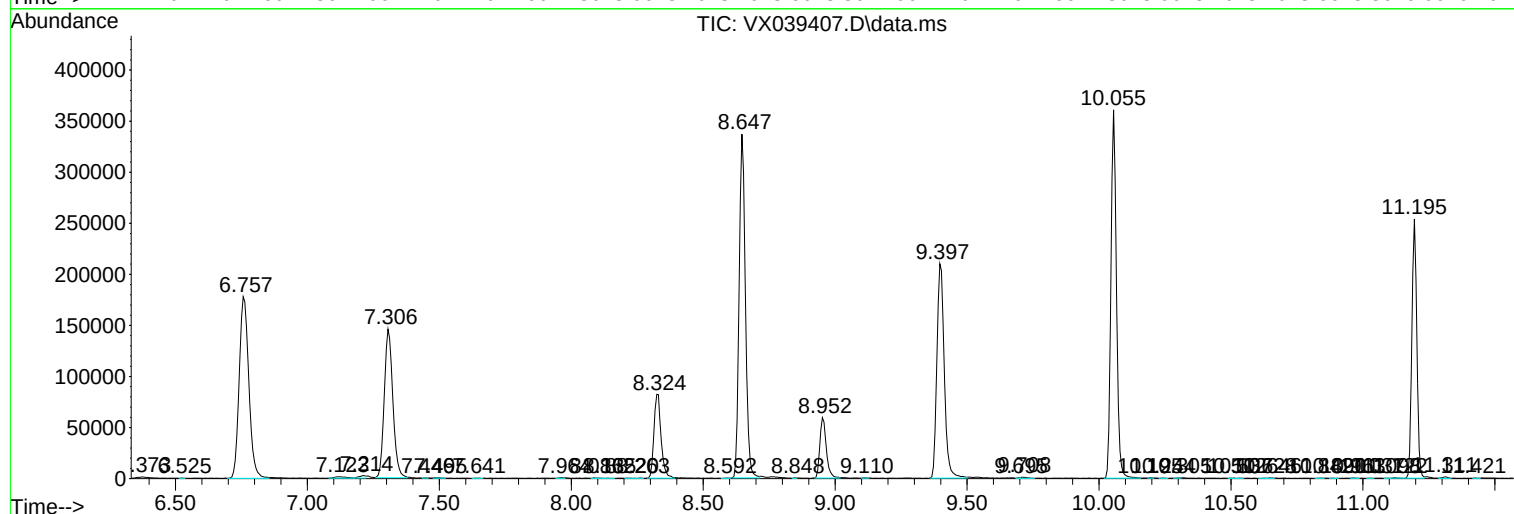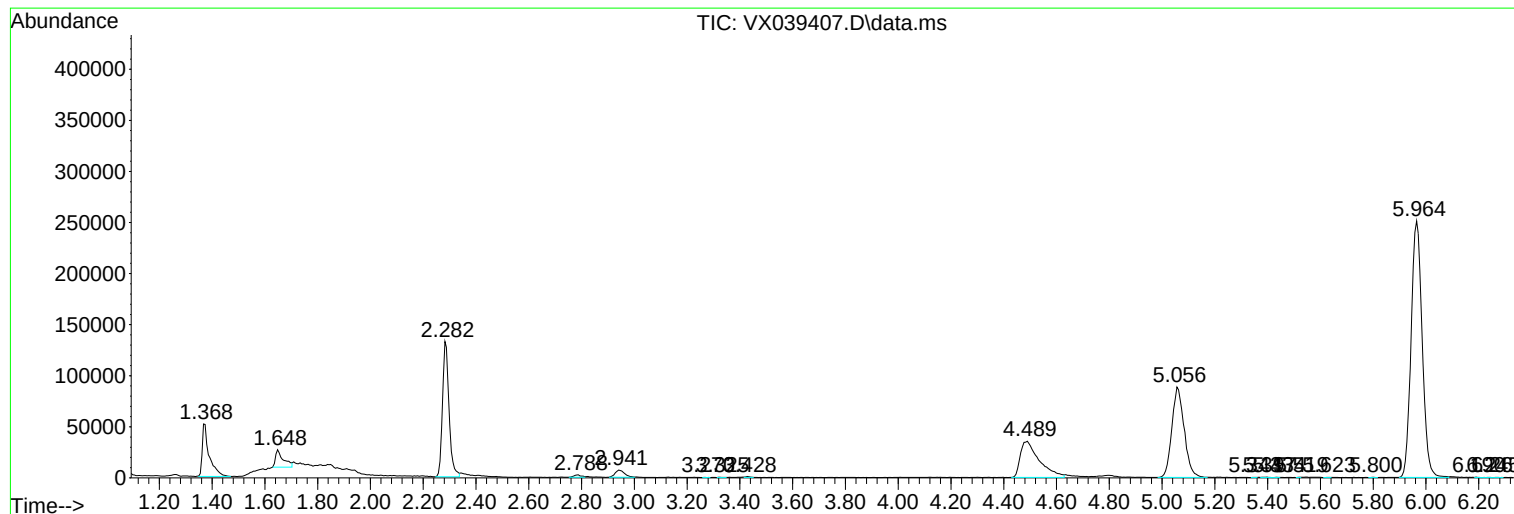

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039407.D
Acq On : 20 Dec 2023 17:22
Operator : JC/MD
Sample : 05794-23ME
Misc : 4.25g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGRG4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039407.D
Acq On : 20 Dec 2023 17:22
Operator : JC/MD
Sample : 05794-23ME
Misc : 4.25g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGRG4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc