

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039410.D
 Acq On : 20 Dec 2023 18:30
 Operator : JC/MD
 Sample : VIBLK628
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK628

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039410.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	23	25	27	rBV2	1470	1647	0.19%	0.025%
2	1.368	42	46	58	rVB	105131	109098	12.36%	1.625%
3	1.672	91	96	109	rVB	67438	100474	11.38%	1.497%
4	2.306	194	200	213	rVB	181685	284871	32.26%	4.244%
5	2.520	233	235	236	rVB	358	253	0.03%	0.004%
6	2.703	263	265	269	rVB	215	183	0.02%	0.003%
7	2.794	275	280	286	rVB3	1708	3238	0.37%	0.048%
8	2.947	300	305	306	rBV3	983	1445	0.16%	0.022%
9	3.075	325	326	328	rBV2	185	162	0.02%	0.002%
10	3.136	334	336	339	rVB	264	258	0.03%	0.004%
11	3.312	362	365	368	rBV2	207	313	0.04%	0.005%
12	3.367	373	374	377	rVB2	177	178	0.02%	0.003%
13	3.709	426	430	433	rVB2	322	442	0.05%	0.007%
14	3.745	433	436	437	rBV	332	299	0.03%	0.004%
15	3.812	442	447	450	rBV2	222	421	0.05%	0.006%
16	4.196	508	510	513	rBV2	176	175	0.02%	0.003%
17	4.276	521	523	524	rBV	204	181	0.02%	0.003%
18	4.294	524	526	527	rVV2	187	161	0.02%	0.002%
19	4.446	543	551	568	rBV	83278	242211	27.43%	3.609%
20	4.855	614	618	619	rBV2	153	179	0.02%	0.003%
21	5.056	639	651	669	rBV	110035	346479	39.24%	5.162%
22	5.257	682	684	687	rVB2	282	249	0.03%	0.004%
23	5.403	702	708	714	rVB2	446	1135	0.13%	0.017%
24	5.464	714	718	719	rBV2	214	196	0.02%	0.003%
25	5.538	729	730	731	rBV	339	208	0.02%	0.003%
26	5.629	743	745	748	rVB	236	243	0.03%	0.004%
27	5.666	748	751	752	rBV	257	311	0.04%	0.005%
28	5.751	764	765	770	rBV2	164	195	0.02%	0.003%
29	5.970	786	801	819	rBV2	293407	882937	100.00%	13.154%
30	6.537	891	894	897	rBV2	176	220	0.02%	0.003%
31	6.568	897	899	901	rVB	243	176	0.02%	0.003%
32	6.659	912	914	915	rVB	327	165	0.02%	0.002%
33	6.684	915	918	920	rBV2	182	195	0.02%	0.003%
34	6.763	922	931	950	rBV	194220	475201	53.82%	7.080%
35	7.031	973	975	979	rBV2	223	289	0.03%	0.004%
36	7.110	983	988	993	rBV4	1349	2835	0.32%	0.042%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039410.D
 Acq On : 20 Dec 2023 18:30
 Operator : JC/MD
 Sample : VIBLK628
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK628

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	7.220	1005	1006	1009	rVB2	263	208	0.02%	0.003%
38	7.251	1009	1011	1012	rBV	265	163	0.02%	0.002%
39	7.306	1012	1020	1038	rVV	180119	407491	46.15%	6.071%
40	7.488	1043	1050	1051	rBV4	509	797	0.09%	0.012%
41	7.836	1105	1107	1110	rVB2	244	191	0.02%	0.003%
42	7.958	1125	1127	1130	rVV2	266	341	0.04%	0.005%
43	7.982	1130	1131	1133	rVV	308	174	0.02%	0.003%
44	8.055	1140	1143	1144	rBV	202	186	0.02%	0.003%
45	8.324	1181	1187	1200	rBV	117264	197324	22.35%	2.940%
46	8.568	1225	1227	1230	rBV	385	392	0.04%	0.006%
47	8.647	1234	1240	1257	rBV	425864	685368	77.62%	10.211%
48	8.952	1284	1290	1303	rBV	86002	131446	14.89%	1.958%
49	9.269	1340	1342	1343	rBV	218	179	0.02%	0.003%
50	9.384	1355	1361	1384	rBV	383143	562178	63.67%	8.376%
51	9.628	1399	1401	1404	rBV2	350	397	0.04%	0.006%
52	9.701	1410	1413	1415	rVB3	644	794	0.09%	0.012%
53	9.958	1454	1455	1459	rBV	233	182	0.02%	0.003%
54	9.988	1459	1460	1465	rBV2	199	240	0.03%	0.004%
55	10.055	1465	1471	1485	rBV	410378	583807	66.12%	8.698%
56	10.207	1494	1496	1499	rVB3	432	281	0.03%	0.004%
57	10.293	1508	1510	1511	rBV	342	175	0.02%	0.003%
58	10.415	1527	1530	1534	rVV	146	170	0.02%	0.003%
59	10.482	1539	1541	1543	rBV	368	222	0.03%	0.003%
60	10.970	1617	1621	1624	rBV3	401	538	0.06%	0.008%
61	11.104	1640	1643	1645	rBV3	240	237	0.03%	0.004%
62	11.122	1645	1646	1649	rVB2	268	239	0.03%	0.004%
63	11.189	1652	1657	1671	rVB	349066	441193	49.97%	6.573%
64	11.293	1671	1674	1675	rBV3	202	258	0.03%	0.004%
65	11.311	1675	1677	1683	rVB2	933	1177	0.13%	0.018%
66	11.378	1683	1688	1689	rBV	225	248	0.03%	0.004%
67	11.457	1698	1701	1705	rBV3	320	548	0.06%	0.008%
68	11.524	1709	1712	1713	rBV2	192	185	0.02%	0.003%
69	11.604	1724	1725	1730	rBV2	190	327	0.04%	0.005%
70	11.975	1784	1786	1788	rBV	440	472	0.05%	0.007%
71	12.018	1788	1793	1807	rBV	452572	597007	67.62%	8.894%
72	12.317	1837	1842	1853	rBV	477125	622374	70.49%	9.272%
73	12.518	1874	1875	1879	rVB2	223	243	0.03%	0.004%
74	12.603	1888	1889	1893	rVB2	221	226	0.03%	0.003%
75	12.762	1909	1915	1919	rVB2	4028	5394	0.61%	0.080%
76	13.000	1951	1954	1955	rBV2	202	168	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
 Data File : VX039410.D
 Acq On : 20 Dec 2023 18:30
 Operator : JC/MD
 Sample : VIBLK628
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK628

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

77	13.067	1962	1965	1967	rBV2	190	237	0.03%	0.004%
78	13.152	1975	1979	1980	rBV2	151	178	0.02%	0.003%
79	13.317	2004	2006	2009	rBV	225	216	0.02%	0.003%
80	13.567	2044	2047	2048	rBV2	163	217	0.02%	0.003%
81	13.603	2050	2053	2057	rVV2	495	643	0.07%	0.010%
82	13.719	2068	2072	2073	rVV	178	250	0.03%	0.004%
83	13.731	2073	2074	2077	rVV	290	237	0.03%	0.004%
84	13.786	2081	2083	2088	rVB	473	580	0.07%	0.009%
85	13.829	2088	2090	2091	rBV2	250	177	0.02%	0.003%
86	13.865	2094	2096	2097	rVV2	235	170	0.02%	0.003%
87	13.884	2097	2099	2101	rVB	233	158	0.02%	0.002%
88	13.914	2101	2104	2105	rBV	244	184	0.02%	0.003%
89	14.128	2135	2139	2144	rVB	3974	5461	0.62%	0.081%
90	14.292	2163	2166	2169	rBV	233	233	0.03%	0.003%
91	14.323	2169	2171	2174	rBV2	189	194	0.02%	0.003%
92	14.420	2185	2187	2190	rVB2	220	219	0.02%	0.003%
93	14.457	2190	2193	2195	rBV2	159	176	0.02%	0.003%
94	14.591	2212	2215	2218	rBV2	281	363	0.04%	0.005%
95	14.975	2277	2278	2281	rVB2	300	235	0.03%	0.004%
96	14.999	2281	2282	2285	rBV	314	219	0.02%	0.003%
97	15.261	2324	2325	2328	rVB2	300	259	0.03%	0.004%
98	15.536	2368	2370	2372	rBV	367	317	0.04%	0.005%
99	15.585	2376	2378	2379	rBV2	269	220	0.02%	0.003%
100	15.731	2400	2402	2404	rBB3	332	250	0.03%	0.004%


Sum of corrected areas: 6712156

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039410.D
Acq On : 20 Dec 2023 18:30
Operator : JC/MD
Sample : VIBLK628
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK628

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

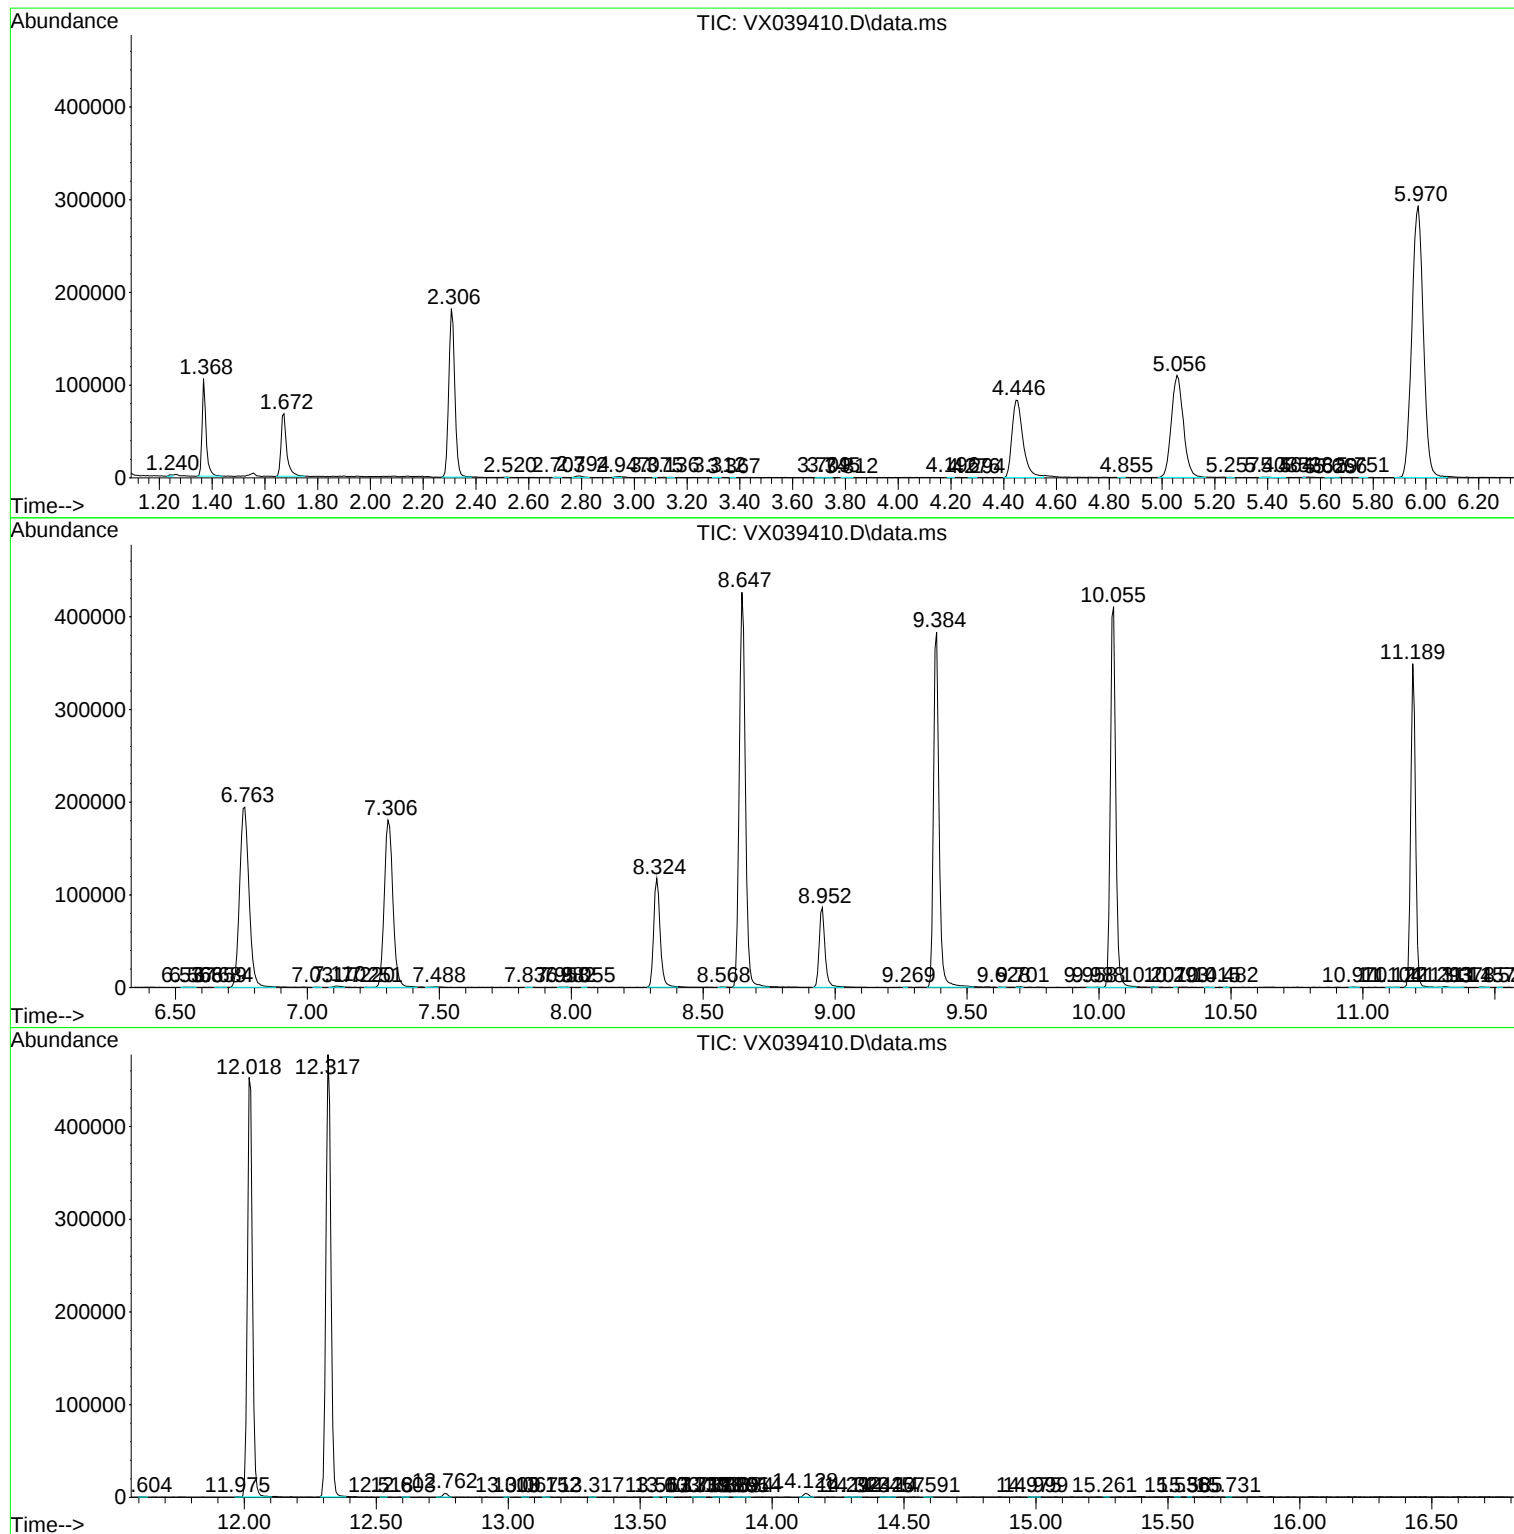

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039410.D
Acq On : 20 Dec 2023 18:30
Operator : JC/MD
Sample : VIBLK628
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK628

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039410.D
Acq On : 20 Dec 2023 18:30
Operator : JC/MD
Sample : VIBLK628
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK628

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------