
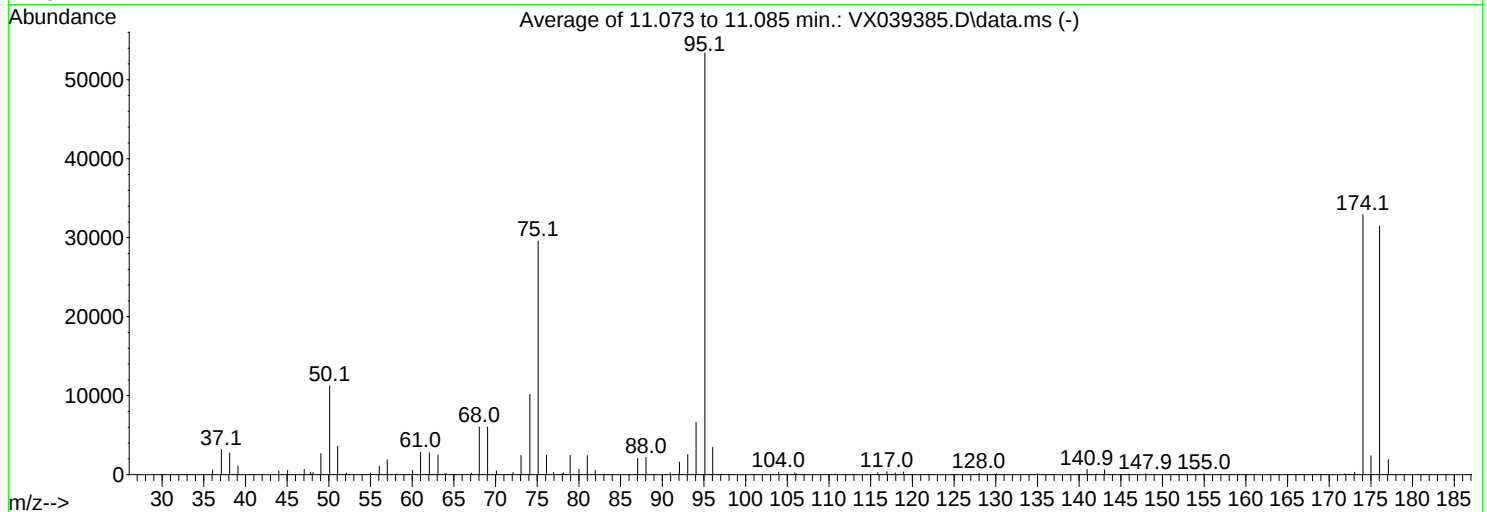


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122023\
Data File : VX039385.D
Acq On : 20 Dec 2023 08:18
Operator : JC/MD
Sample : BFB658
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB658

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Title : VOC Analysis
Last Update : Fri Dec 22 00:41:09 2023

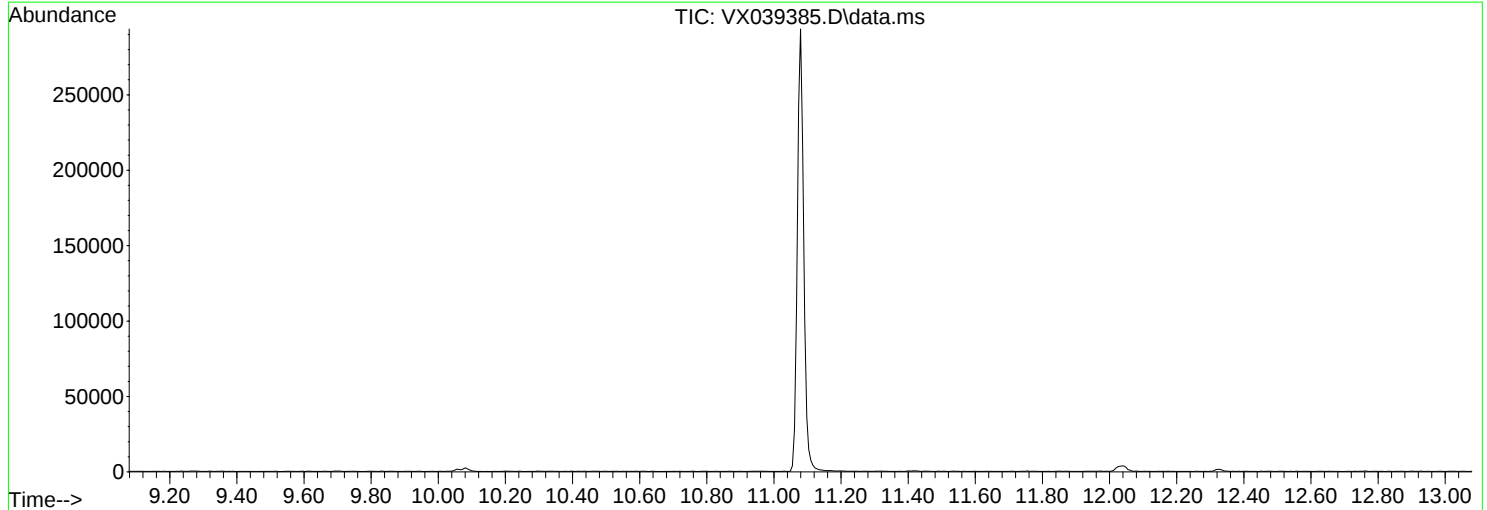

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	11216	PASS
75	95	30	80	55.4	29573	PASS
95	95	100	100	100.0	53408	PASS
96	95	5	9	6.5	3459	PASS
173	174	0.00	2	0.9	309	PASS
174	95	50	120	61.6	32896	PASS
175	174	5	9	7.2	2383	PASS
176	174	95	101	95.7	31488	PASS
177	176	5	9	6.0	1903	PASS

m/z	Abundance
40.00	247.0
44.00	126.0

Instrument :
MSVOA_X
ClientSampleId :
BFB658

m/z	Abundance
36.00	586.0
37.10	3636.0
38.10	3092.0
39.10	1098.0
40.00	186.0
44.10	545.0
45.10	633.0
47.10	889.0
47.90	460.0
49.00	2635.0
50.10	11606.0
51.00	3763.0
52.10	286.0
54.90	245.0
56.00	931.0
57.00	2058.0
58.10	140.0
59.10	59.0
60.00	478.0
61.00	3131.0
62.10	2811.0
63.10	2606.0
63.90	238.0
65.30	80.0
67.20	144.0
68.10	6056.0
69.00	6260.0
70.10	511.0
72.10	266.0
73.10	2597.0
74.10	10359.0
75.10	30080.0
76.10	2486.0
76.90	239.0
78.00	276.0
79.00	2533.0
80.00	851.0
81.00	2400.0
82.00	586.0
83.20	54.0
86.00	53.0
87.10	2043.0
88.10	1941.0
91.00	245.0
92.00	1556.0
93.10	2636.0
94.00	6637.0
95.10	53680.0
96.10	3458.0
97.10	126.0
103.90	284.0
105.00	92.0
105.90	267.0
106.90	84.0
110.70	102.0
112.90	62.0
115.80	287.0
117.00	429.0
117.90	230.0
119.00	300.0
128.00	122.0
129.00	73.0
129.80	179.0
131.10	67.0
134.70	78.0
135.00	94.0
136.90	54.0
141.00	565.0
142.00	107.0
143.10	449.0
145.90	105.0
148.00	102.0
149.10	51.0
155.00	118.0
156.90	107.0
159.00	87.0
161.10	56.0
171.90	105.0
173.10	300.0
174.10	27392.0
175.00	2019.0
176.00	26104.0
177.10	1783.0

Instrument :
MSVOA_X
ClientSampleId :
BFB658

m/z	Abundance
36.10	744.0
37.10	3590.0
38.10	3035.0
39.10	1304.0
40.00	253.0
44.00	710.0
45.10	519.0
47.10	746.0
47.70	405.0
48.10	462.0
49.10	3232.0
50.10	13137.0
51.00	4011.0
52.10	182.0
55.00	153.0
56.00	1300.0
57.00	2127.0
58.10	79.0
60.10	741.0
61.00	3255.0
62.00	3334.0
63.10	2994.0
64.10	315.0
65.20	64.0
67.00	212.0
68.00	7082.0
69.10	7189.0
70.10	628.0
72.10	308.0
73.00	2896.0
74.10	11778.0
75.10	34744.0
76.10	2929.0
77.00	413.0
78.20	481.0
78.90	2660.0
80.00	737.0
81.00	3065.0
81.90	576.0
83.10	79.0
86.00	65.0
87.00	2279.0
88.00	2660.0
90.90	317.0
92.10	1874.0
93.00	2918.0
94.10	7674.0
95.10	62664.0
96.10	4132.0
97.10	118.0
104.00	345.0
104.90	63.0
105.90	402.0
106.80	75.0
109.90	54.0
110.80	85.0
112.10	56.0
112.80	86.0
115.10	52.0
115.90	366.0
117.00	397.0
117.90	198.0
118.90	451.0
127.90	213.0
129.00	56.0
130.10	220.0
131.00	73.0
135.10	153.0
136.80	73.0
140.90	744.0
142.10	88.0
143.00	758.0
145.90	78.0
148.00	99.0
149.00	52.0
152.90	65.0
155.00	182.0
156.90	75.0
159.20	92.0
171.80	114.0
172.30	173.0
173.10	336.0
174.00	38344.0
175.00	2703.0
176.00	36880.0
177.10	2308.0

Instrument :
MSVOA_X
ClientSampleId :
BFB658

m/z	Abundance
36.00	372.0
37.10	2313.0
38.10	2132.0
39.10	886.0
40.00	226.0
44.00	502.0
45.00	458.0
45.90	76.0
46.90	364.0
48.10	320.0
49.10	2150.0
50.10	8905.0
51.10	3077.0
52.10	171.0
55.10	214.0
56.10	949.0
57.00	1480.0
60.00	433.0
61.00	2138.0
62.10	2199.0
63.00	1811.0
64.00	244.0
65.00	52.0
67.10	114.0
68.10	4952.0
69.00	4741.0
70.10	345.0
72.10	236.0
73.00	1876.0
74.10	8405.0
75.10	23896.0
76.10	1886.0
76.90	193.0
78.10	186.0
78.90	2183.0
79.90	399.0
81.00	1787.0
81.90	422.0
83.00	80.0
87.00	1902.0
88.00	1947.0
90.90	191.0
92.00	1390.0
93.00	2064.0
94.10	5631.0
95.10	43880.0
96.00	2787.0
104.00	360.0
104.90	70.0
106.10	275.0
109.80	55.0
110.80	53.0
115.00	64.0
115.90	160.0
116.90	320.0
118.00	257.0
118.90	264.0
128.10	216.0
128.90	74.0
130.10	157.0
131.00	57.0
134.90	104.0
136.80	81.0
140.90	617.0
142.00	125.0
143.10	596.0
146.00	82.0
147.90	110.0
155.00	59.0
159.20	50.0
172.00	165.0
172.90	291.0
174.00	32952.0
175.00	2428.0
176.10	31480.0
177.10	1617.0

Instrument :
MSVOA_X
ClientSampleId :
BFB658