

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122024\
 Data File : VX044453.D
 Acq On : 20 Dec 2024 15:33
 Operator : JC/MD
 Sample : P5356-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STAND-PIPE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
 Title : SW846 8260

Signal : TIC: VX044453.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	19	rVB	27839	30872	4.63%	0.869%
2	1.264	27	29	33	rVB	7332	7243	1.09%	0.204%
3	1.368	43	46	54	rVB	6113	7533	1.13%	0.212%
4	1.593	66	83	86	rBV3	18440	67938	10.19%	1.913%
5	1.618	86	87	91	rVB	16835	11510	1.73%	0.324%
6	2.386	207	213	219	rBV2	4173	7767	1.16%	0.219%
7	5.385	692	705	721	rBV2	78011	237559	35.63%	6.689%
8	5.544	721	731	747	rVV2	125250	360708	54.10%	10.157%
9	5.952	786	798	811	rBV	93909	246386	36.95%	6.938%
10	6.757	922	930	943	rBV	199605	487464	73.11%	13.726%
11	8.647	1233	1240	1250	rBV	419069	666732	100.00%	18.773%
12	8.720	1250	1252	1257	rVB3	4898	6927	1.04%	0.195%
13	10.055	1465	1471	1485	rBV	394248	573689	86.04%	16.154%
14	11.079	1634	1639	1656	rBV	296893	392689	58.90%	11.057%
15	12.018	1788	1793	1802	rBV	341318	446446	66.96%	12.571%




Sum of corrected areas: 3551463

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122024\
Data File : VX044453.D
Acq On : 20 Dec 2024 15:33
Operator : JC/MD
Sample : P5356-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STAND-PIPE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

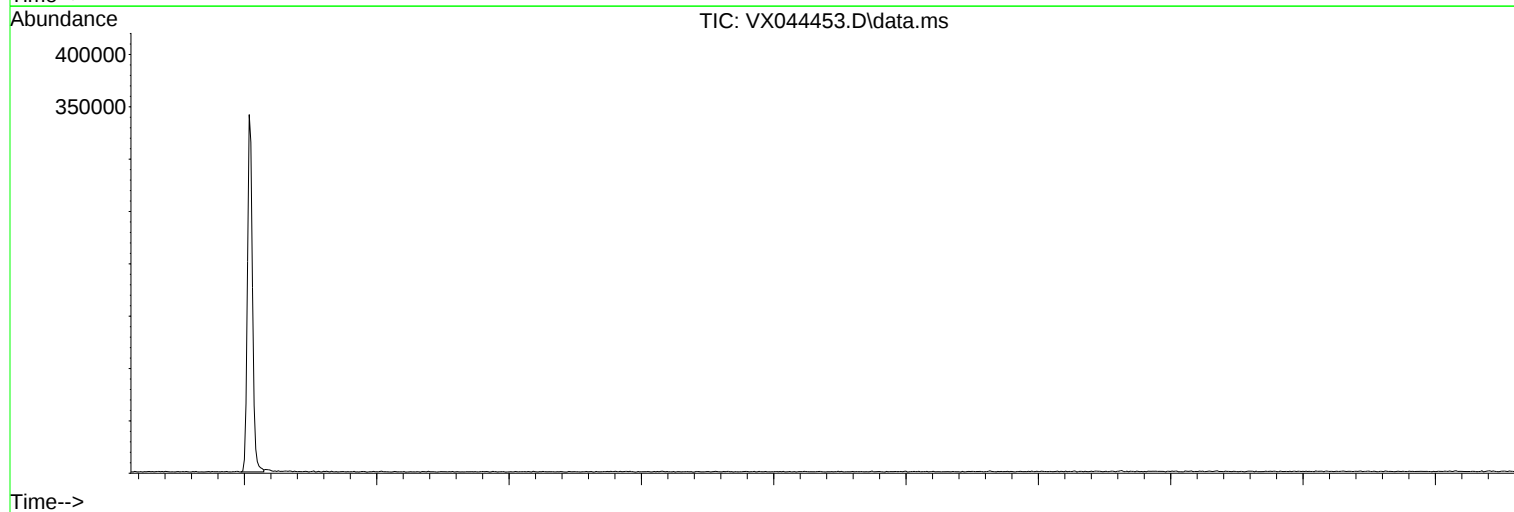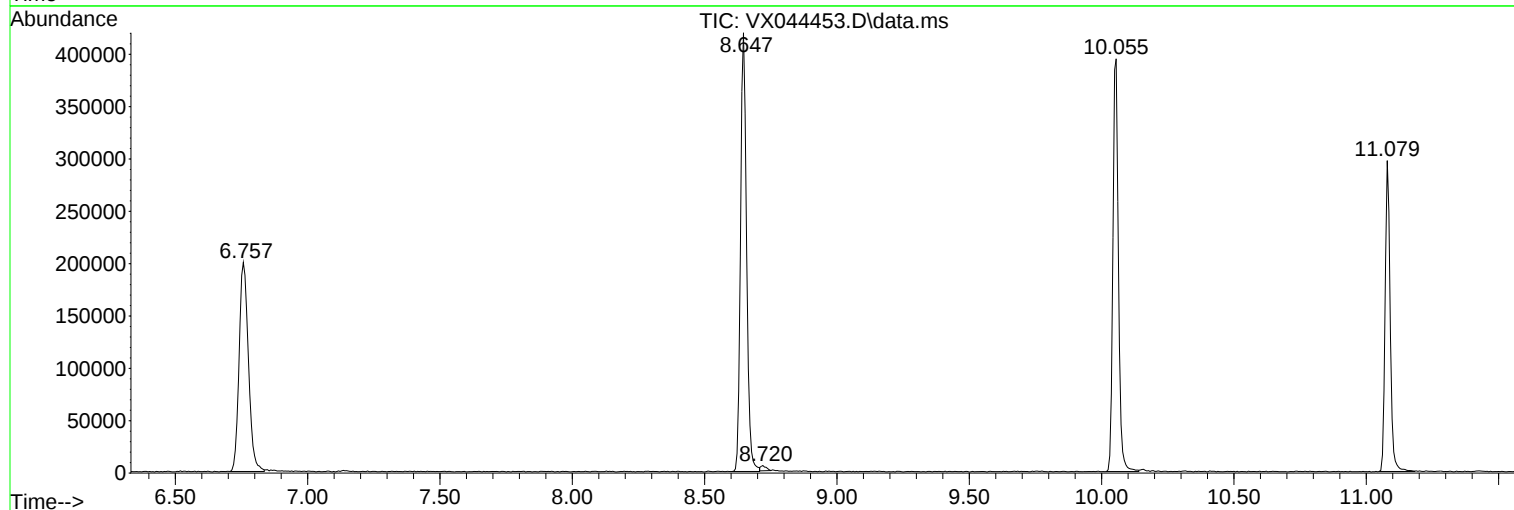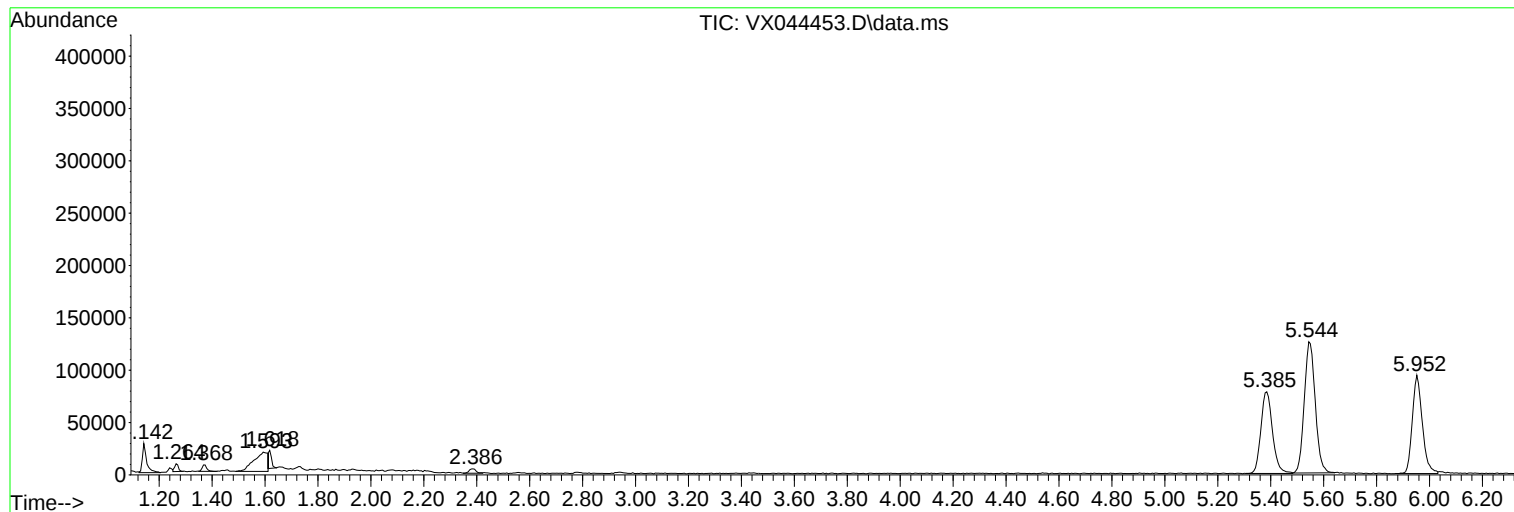

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122024\
Data File : VX044453.D
Acq On : 20 Dec 2024 15:33
Operator : JC/MD
Sample : P5356-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STAND-PIPE










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.593 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
1.593	9.42 ug/l	67938	Pentafluorobenzene	5.544	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1 (-)	Norephedrine	151	C9H13NO	000492-41-1	10
2	Cathine	151	C9H13NO	000492-39-7	10
3	N-Methyl-2-phenyl-1-propylamine	149	C10H15N	000093-88-9	9
4	1-(5-Bicyclo[2.2.1]heptyl)ethyla...	139	C9H17N	1000222-20-9	9
5	N-(3,5-Dinitropyridin-2-yl)-L-as...	300	C9H8N4O8	035899-60-6	9

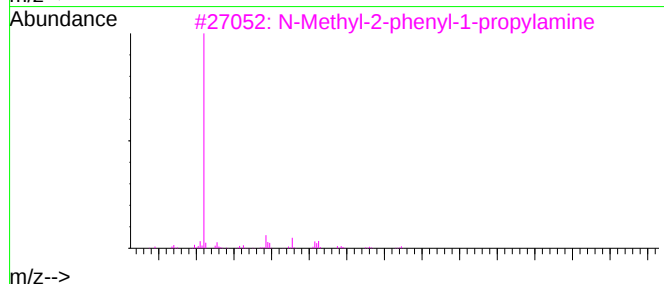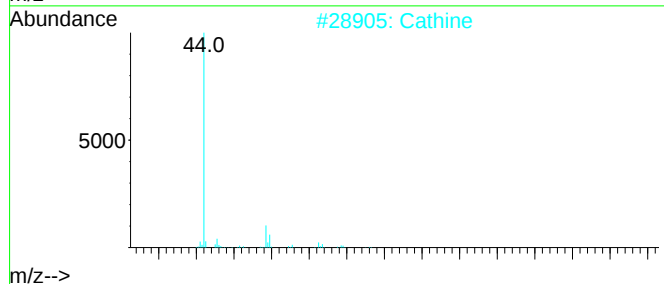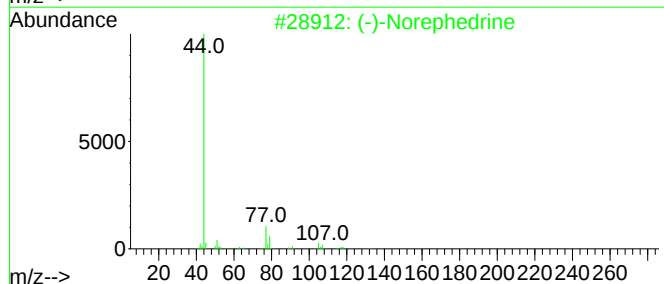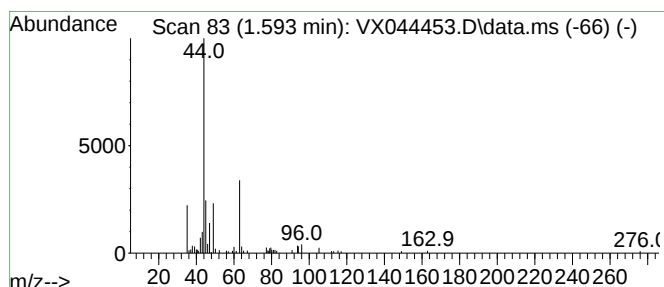

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122024\
Data File : VX044453.D
Acq On : 20 Dec 2024 15:33
Operator : JC/MD
Sample : P5356-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STAND-PIPE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.593	1.593	9.4	ug/l	67938	1	5.544	360708	50.0