

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122024\
 Data File : VX044458.D
 Acq On : 20 Dec 2024 17:30
 Operator : JC/MD
 Sample : P5280-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BPOW6-11-20241212

Integration Parameters: RTEINT.P
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
 Title : SW846 8260

Signal : TIC: VX044458.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	21	25	27	rBV	5318	7467	1.18%	0.227%
2	1.593	67	83	84	rBV7	17695	57421	9.05%	1.749%
3	2.709	262	266	272	rVB4	3724	6444	1.02%	0.196%
4	5.379	694	704	719	rBV	73927	225518	35.56%	6.868%
5	5.550	719	732	745	rVV	120279	346695	54.66%	10.558%
6	5.952	789	798	813	rBV2	87229	235301	37.10%	7.166%
7	6.757	920	930	944	rBV	191218	466726	73.59%	14.214%
8	8.647	1233	1240	1255	rBV	400781	634252	100.00%	19.315%
9	10.055	1464	1471	1487	rBV	365053	534627	84.29%	16.281%
10	11.079	1634	1639	1653	rBV	277179	363037	57.24%	11.056%
11	12.018	1788	1793	1806	rBV	308397	406164	64.04%	12.369%




Sum of corrected areas: 3283652

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122024\
Data File : VX044458.D
Acq On : 20 Dec 2024 17:30
Operator : JC/MD
Sample : P5280-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPOW6-11-20241212

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

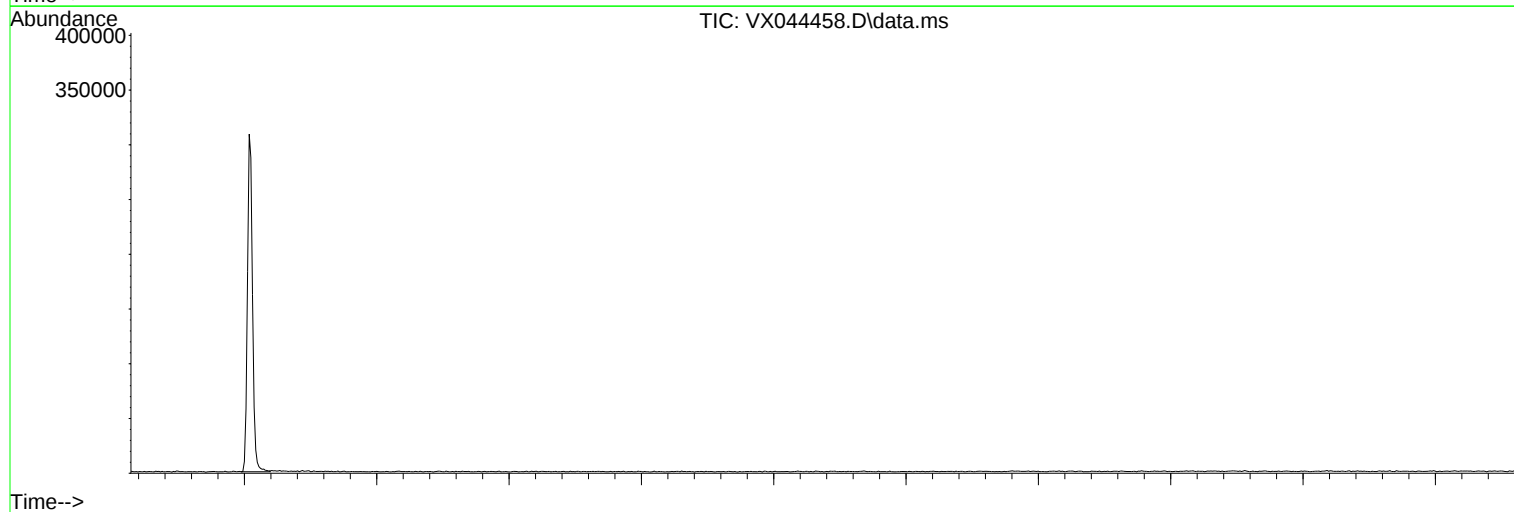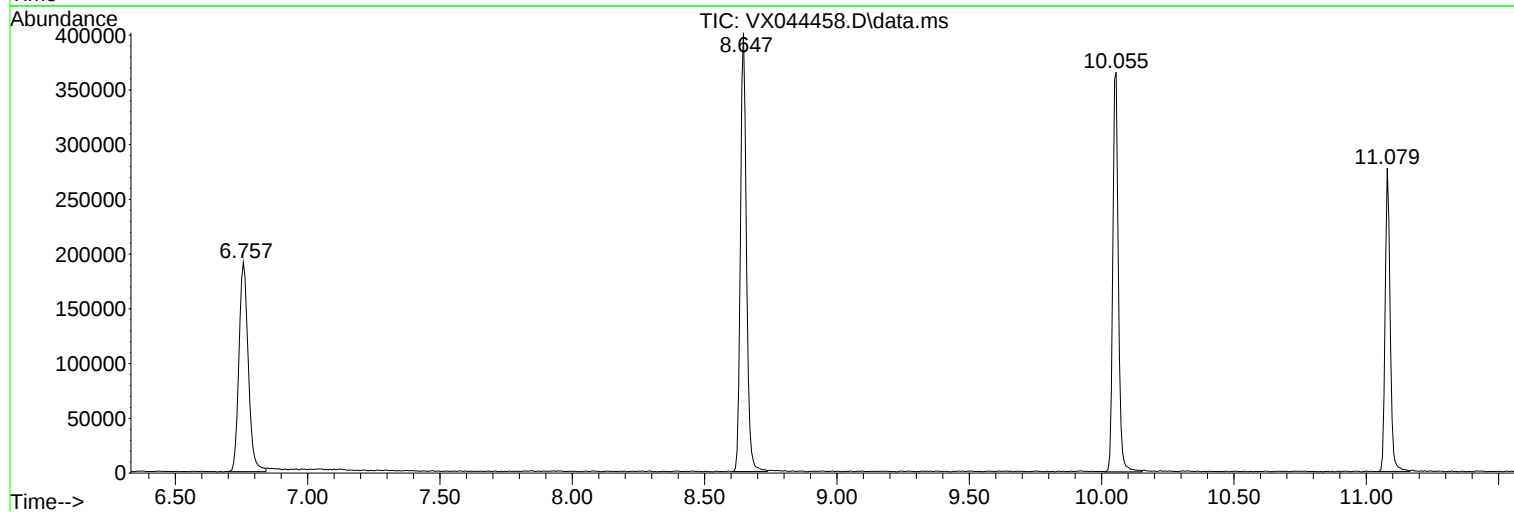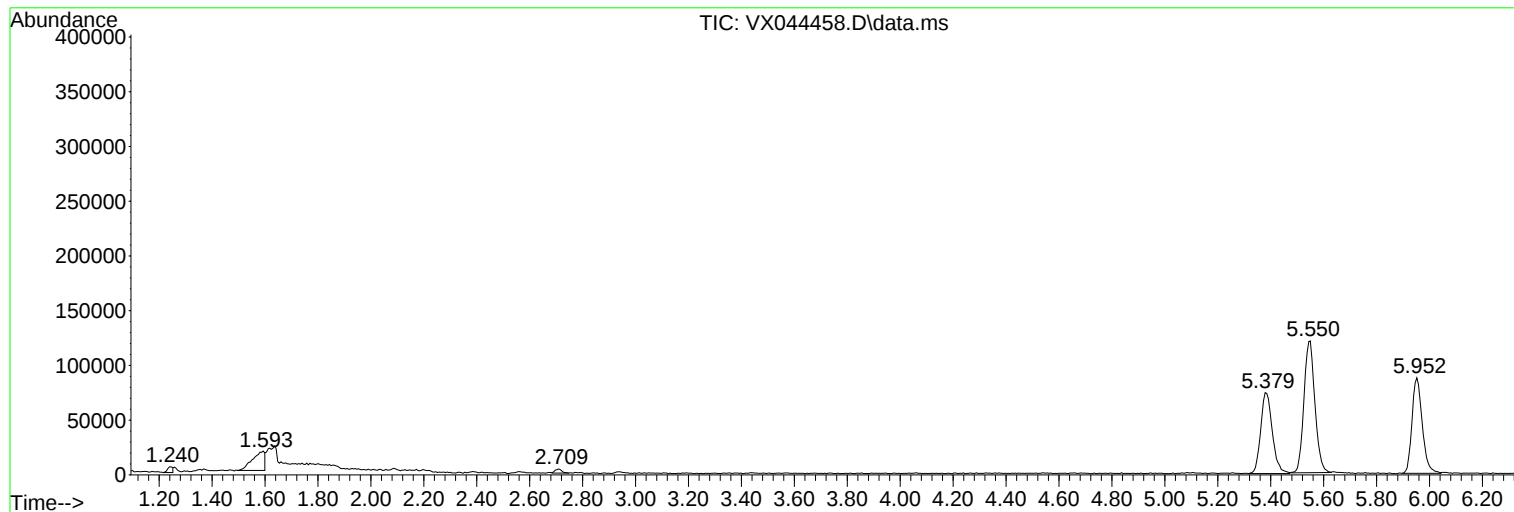

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122024\
Data File : VX044458.D
Acq On : 20 Dec 2024 17:30
Operator : JC/MD
Sample : P5280-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPOW6-11-20241212










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.593 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.593	8.28 ug/l	57421	Pentafluorobenzene	5.544

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Acetamide, 2-fluoro-	77	C2H4FNO	000640-19-7	14
2			2-Methylaminomethyl-1,3-dioxolane	117	C5H11NO2	057366-77-5	9
3			Paradrine	151	C9H13NO	000103-86-6	9
4			Acetamide, 2,2,2-trifluoro-	113	C2H2F3NO	000354-38-1	9
5			DL-Cystine	240	C6H12N2O4S2	000923-32-0	9

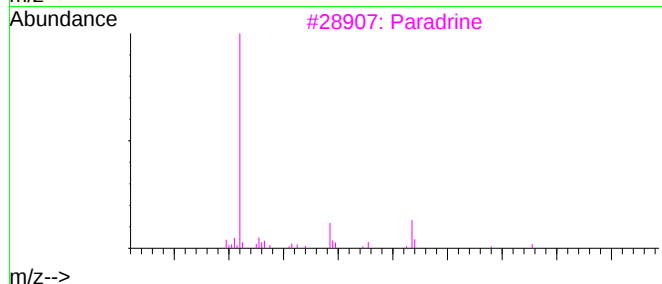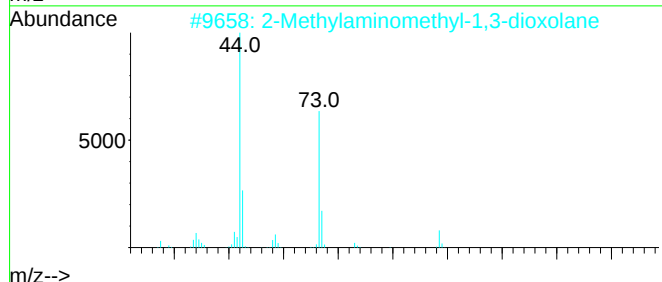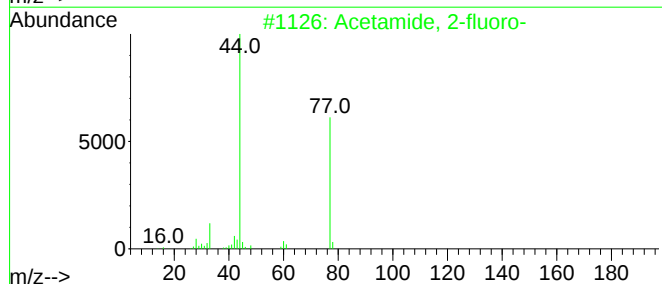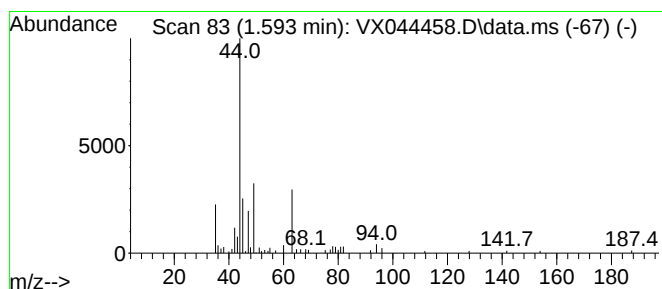

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122024\
Data File : VX044458.D
Acq On : 20 Dec 2024 17:30
Operator : JC/MD
Sample : P5280-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPOW6-11-20241212

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.593	1.593	8.3	ug/l	57421	1	5.544	346695	50.0