

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122120\
 Data File : VX020269.D
 Acq On : 21 Dec 2020 23:26
 Operator : JC/MD
 Sample : PB133709TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB133709TB

Quant Time: Dec 22 05:14:38 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 18 13:09:49 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.629	168	269425	50.00	ug/l	0.01
34) 1,4-Difluorobenzene	6.830	114	455764	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.098	117	439877	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.061	152	181873	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.031	65	179790	49.78	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	99.56%		
35) Dibromofluoromethane	5.464	113	143805	49.32	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	98.64%		
50) Toluene-d8	8.696	98	576159	51.34	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	102.68%		
62) 4-Bromofluorobenzene	11.122	95	200658	46.72	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	93.44%		
Target Compounds						Qvalue
5) Bromomethane	1.636	94	1114	0.94	ug/l	82
10) Methyl Iodide	2.495	142	1555	3.69	ug/l #	96
11) Tert butyl alcohol	2.989	59	6956	8.60	ug/l #	75
13) Acrolein	2.276	56	276	0.55	ug/l #	43
15) Acrylonitrile	3.117	53	529	0.28	ug/l	91
16) Acetone	2.416	43	18027	10.95	ug/l	98
17) Carbon Disulfide	2.550	76	2103	0.26	ug/l #	94
18) Methyl Acetate	2.745	43	1872	0.51	ug/l #	86
20) Methylene Chloride	2.831	84	9748	2.63	ug/l	97
25) 2-Butanone	4.641	43	7175	2.99	ug/l	92
29) Tetrahydrofuran	5.099	42	531	0.35	ug/l #	74
31) Cyclohexane	5.629	56	5497	1.10	ug/l #	1
36) 1,1-Dichloropropene	5.629	75	21764	4.83	ug/l #	48
37) Ethyl Acetate	4.641	43	7175	1.53	ug/l #	67
38) Carbon Tetrachloride	5.623	117	26900	6.28	ug/l #	17
41) Methacrylonitrile	5.105	41	721	0.29	ug/l #	30
43) Isopropyl Acetate	6.409	43	25129	3.40	ug/l	97
48) Methyl methacrylate	7.647	41	7525	2.08	ug/l #	10
49) 1,4-Dioxane	7.848	88	304	3.59	ug/l #	1
51) 4-Methyl-2-Pentanone	8.592	43	88006	19.24	ug/l #	47
52) Toluene	8.763	92	1727	0.20	ug/l	99
54) cis-1,3-Dichloropropene	8.592	75	45470	8.15	ug/l #	61
57) 1,3-Dichloropropane	9.525	76	29305	4.88	ug/l #	43
59) 2-Hexanone	9.525	43	360382	103.37	ug/l #	46
76) 1,2,3-Trichloropropane	11.122	75	95752	21.37	ug/l #	39
80) 1,3,5-Trimethylbenzene	11.488	105	2812	0.25	ug/l	92
81) trans-1,4-Dichloro-2-b...	11.122	75	95752	63.41	ug/l #	12
93) 1,2,4-Trichlorobenzene	13.628	180	948	0.24	ug/l	96
94) Hexachlorobutadiene	13.762	225	464	2.91	ug/l	89
96) 1,2,3-Trichlorobenzene	13.999	180	792	0.20	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122120\
Data File : VX020269.D
Acq On : 21 Dec 2020 23:26
Operator : JC/MD
Sample : PB133709TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB133709TB


Quant Time: Dec 22 05:14:38 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 18 13:09:49 2020
Response via : Initial Calibration

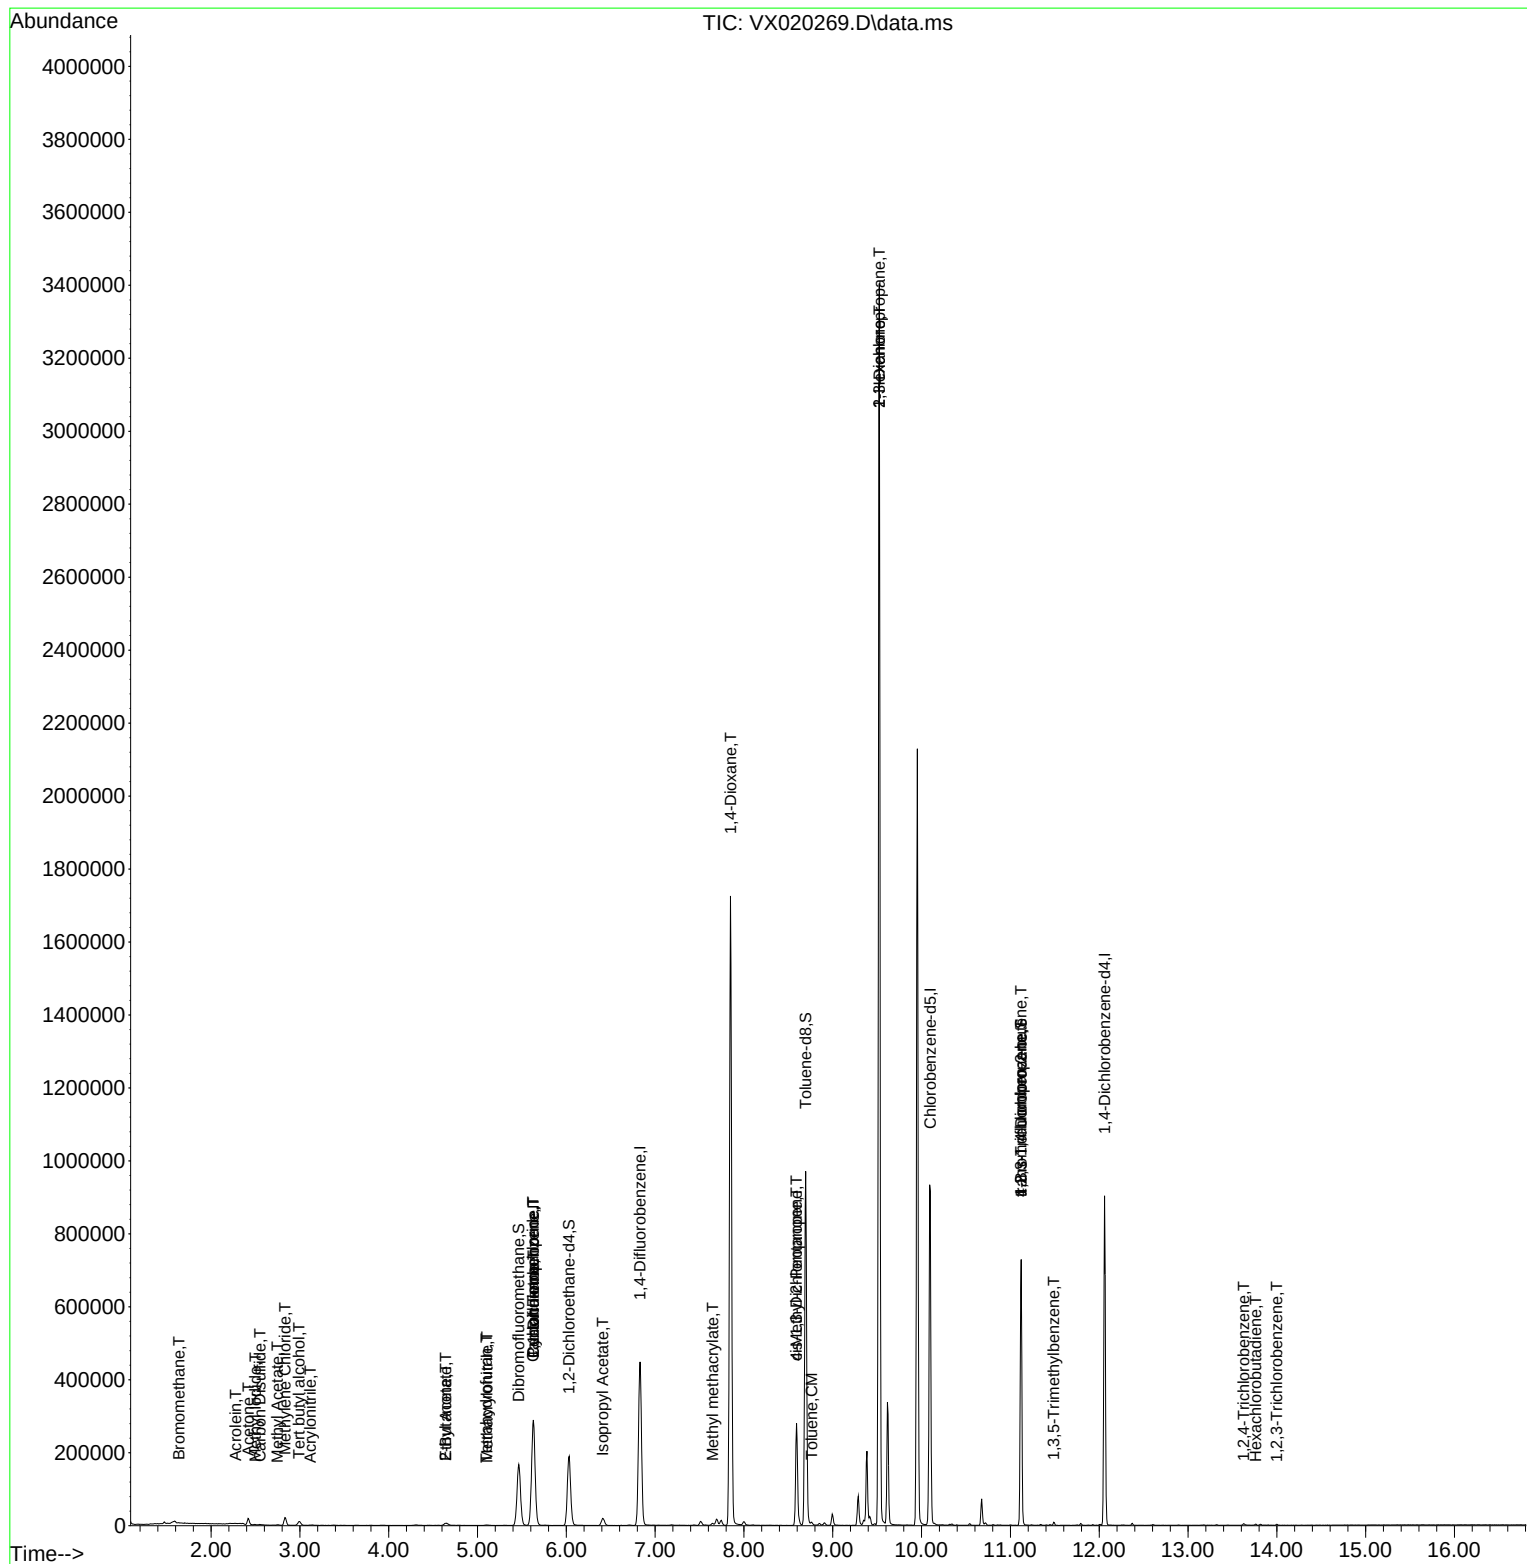






#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 745
Delta R.T. 0.012 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26

Instrument :
MSVOA_X
ClientSampleId :
PB133709TB







Tgt Ion:168 Resp: 269425
Ion Ratio Lower Upper
168 100
99 58.2 45.8 68.6

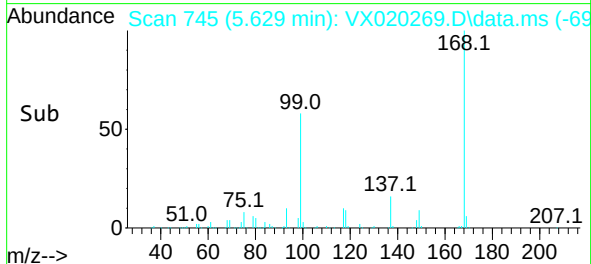

#5
Bromomethane
Concen: 0.94 ug/l
RT: 1.636 min Scan# 90
Delta R.T. 0.012 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26


Tgt Ion: 94 Resp: 1114
Ion Ratio Lower Upper
94 100
96 78.3 76.4 114.6








#10
Methyl Iodide
Concen: 3.69 ug/l
RT: 2.495 min Scan# 231
Delta R.T. 0.006 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26


Instrument :
MSVOA_X
ClientSampleId :
PB133709TB





Tgt Ion:142 Resp: 1555
Ion Ratio Lower Upper
142 100
127 43.0 33.3 49.9
141 11.1 11.4 17.0#

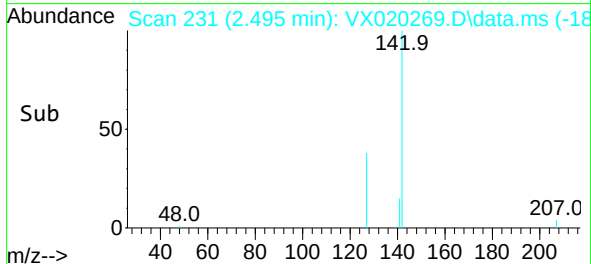


#11
Tert butyl alcohol
Concen: 8.60 ug/l
RT: 2.989 min Scan# 312
Delta R.T. -0.025 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26



Tgt Ion: 59 Resp: 6956
Ion Ratio Lower Upper
59 100
57 0.6 7.8 11.8#




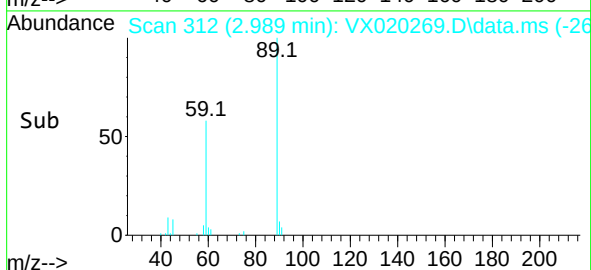


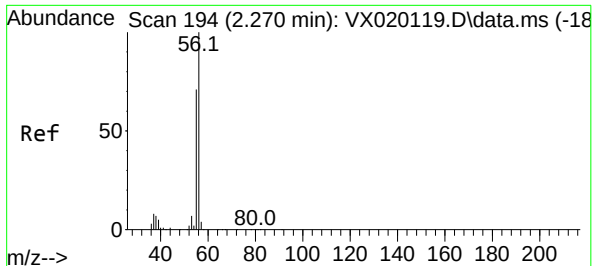

#13
Acrolein
Concen: 0.55 ug/l
RT: 2.276 min Scan# 195
Delta R.T. 0.006 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26




Instrument :
MSVOA_X
ClientSampleId :
PB133709TB


Tgt Ion: 56 Resp: 276
Ion Ratio Lower Upper
56 100
55 117.8 56.4 84.6#

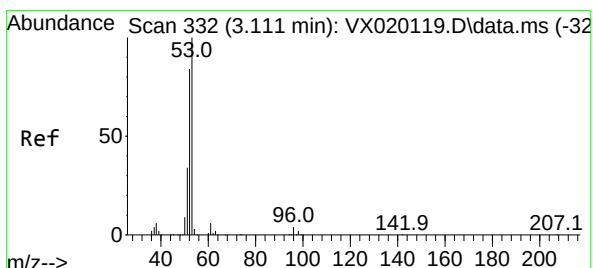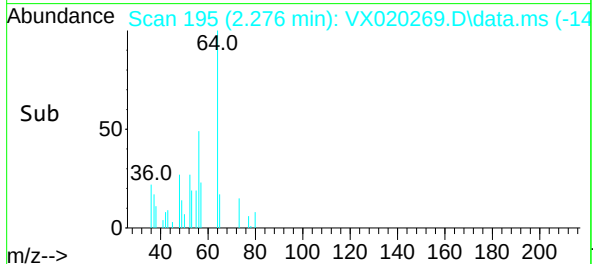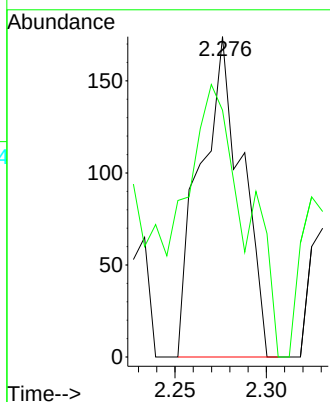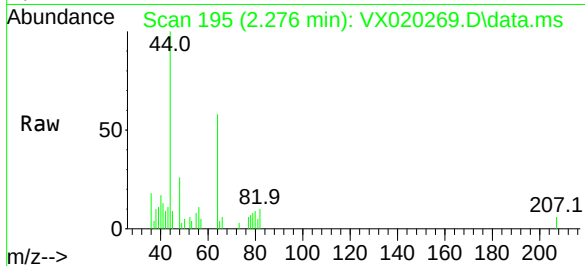

#15
Acrylonitrile
Concen: 0.28 ug/l
RT: 3.117 min Scan# 333
Delta R.T. 0.006 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26

Tgt Ion: 53 Resp: 529
Ion Ratio Lower Upper
53 100
52 74.7 65.3 97.9
51 28.4 28.2 42.2


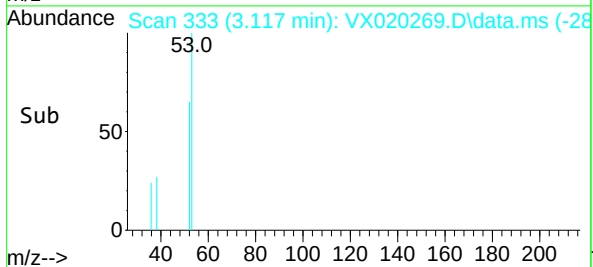
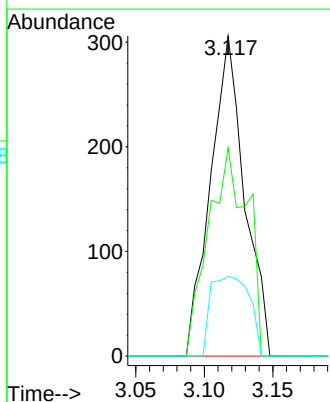
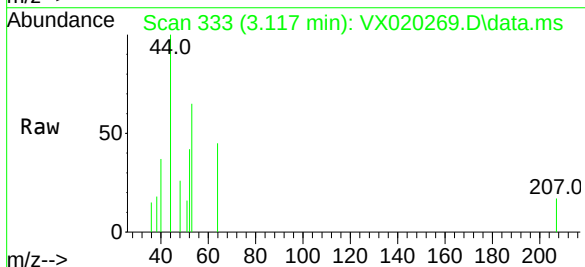




#16
Acetone
Concen: 10.95 ug/l
RT: 2.416 min Scan# 218
Delta R.T. 0.000 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26




Instrument :
MSVOA_X
ClientSampleId :
PB133709TB


Tgt Ion: 43 Resp: 18027
Ion Ratio Lower Upper
43 100
58 33.7 27.8 41.8

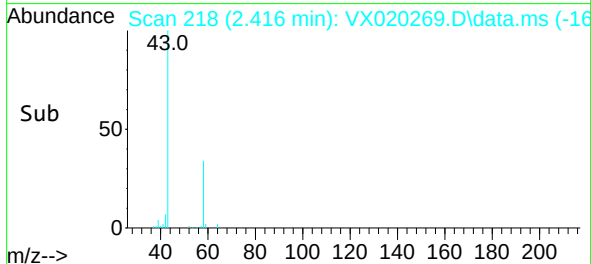

#17
Carbon Disulfide
Concen: 0.26 ug/l
RT: 2.550 min Scan# 240
Delta R.T. 0.006 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26

Tgt Ion: 76 Resp: 2103
Ion Ratio Lower Upper
76 100
78 11.1 7.2 10.8#


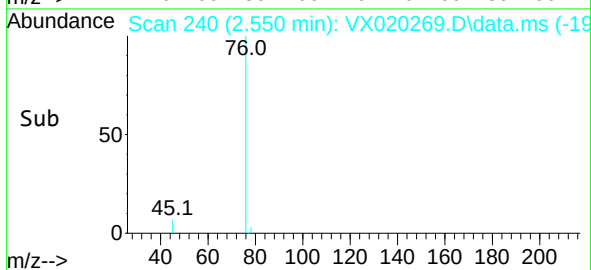






#18
Methyl Acetate
Concen: 0.51 ug/l
RT: 2.745 min Scan# 272
Delta R.T. 0.000 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26




Instrument :
MSVOA_X
ClientSampleId :
PB133709TB


Tgt Ion: 43 Resp: 1872
Ion Ratio Lower Upper
43 100
74 20.0 21.9 32.9#

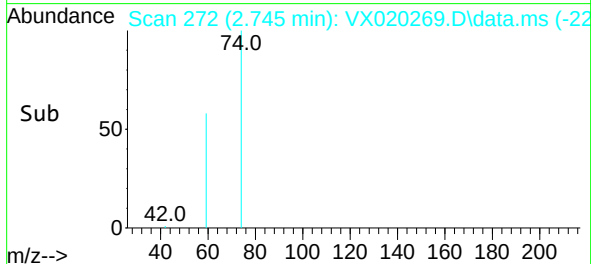

#20
Methylene Chloride
Concen: 2.63 ug/l
RT: 2.831 min Scan# 286
Delta R.T. -0.000 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26

Tgt Ion: 84 Resp: 9748
Ion Ratio Lower Upper
84 100
49 107.9 88.6 132.8
51 35.2 27.0 40.6
86 65.8 50.3 75.5


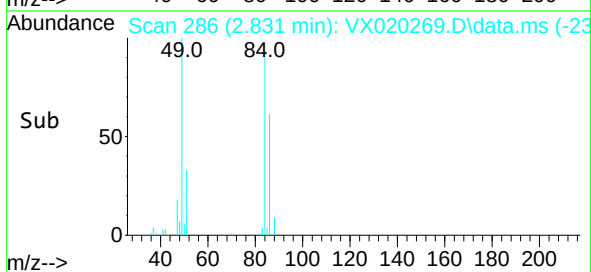






#25
2-Butanone
Concen: 2.99 ug/l
RT: 4.641 min Scan# 583
Delta R.T. 0.018 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26




Instrument :
MSVOA_X
ClientSampleId :
PB133709TB


Tgt Ion: 43 Resp: 7175
Ion Ratio Lower Upper
43 100
72 25.5 23.7 35.5

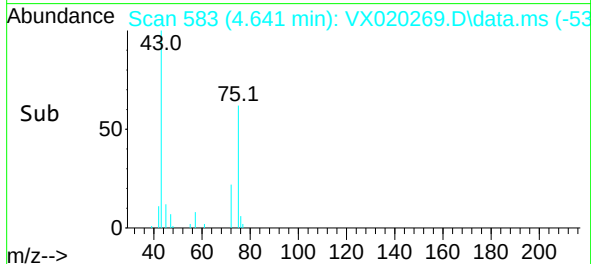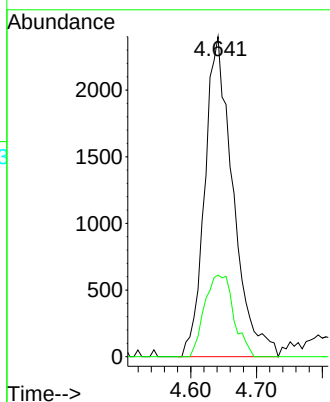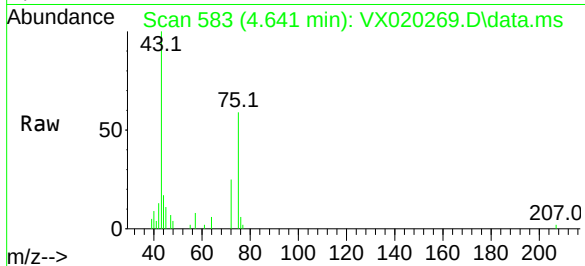

#29
Tetrahydrofuran
Concen: 0.35 ug/l
RT: 5.099 min Scan# 658
Delta R.T. 0.019 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26


Tgt Ion: 42 Resp: 531
Ion Ratio Lower Upper
42 100
72 71.9 41.7 62.5#
71 31.8 38.4 57.6#

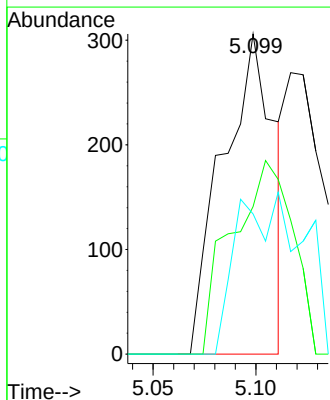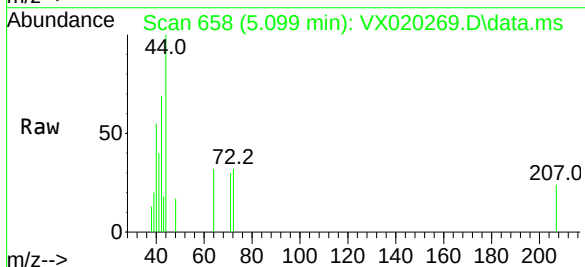






#31
Cyclohexane
Concen: 1.10 ug/l
RT: 5.629 min Scan# 745
Delta R.T. 0.092 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26


Instrument :
MSVOA_X
ClientSampleId :
PB133709TB

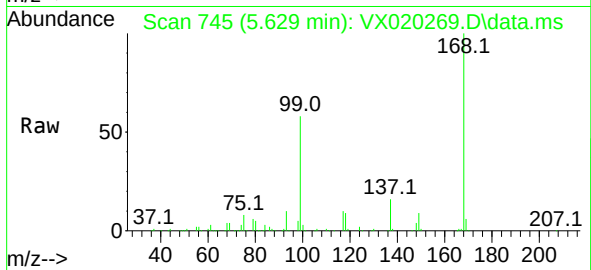



Tgt Ion: 56 Resp: 5497
Ion Ratio Lower Upper
56 100
69 205.3 25.3 37.9#
84 151.8 71.4 107.0#

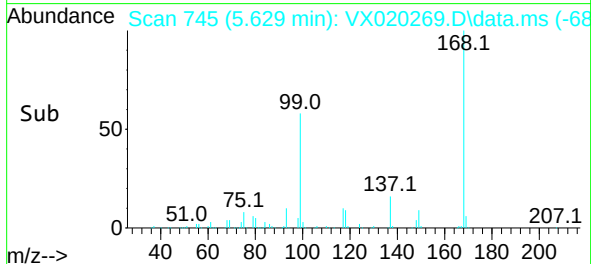


#33
1,2-Dichloroethane-d4
Concen: 49.78 ug/l
RT: 6.031 min Scan# 811
Delta R.T. 0.006 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26



Tgt Ion: 65 Resp: 179790
Ion Ratio Lower Upper
65 100
67 53.2 0.0 105.4









#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.830 min Scan# 942
Delta R.T. 0.006 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26




Instrument :
MSVOA_X
ClientSampleId :
PB133709TB


Tgt Ion:114 Resp: 455764
Ion Ratio Lower Upper
114 100
63 21.7 0.0 40.8
88 16.7 0.0 32.8

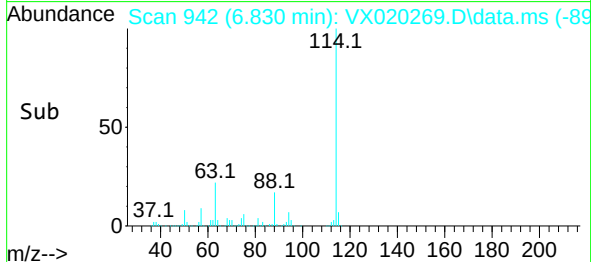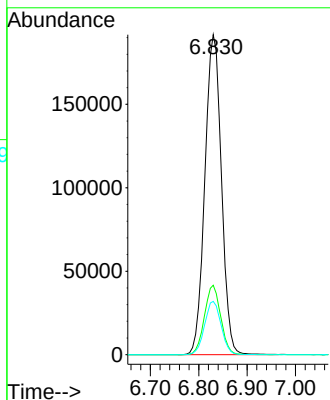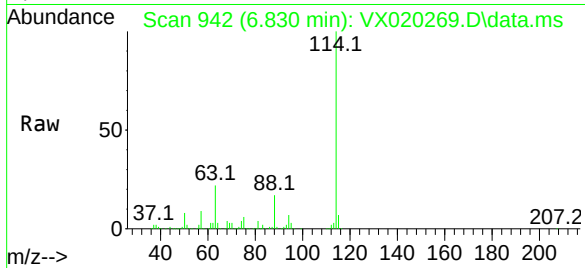

#35
Dibromofluoromethane
Concen: 49.32 ug/l
RT: 5.464 min Scan# 718
Delta R.T. 0.006 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26


Tgt Ion:113 Resp: 143805
Ion Ratio Lower Upper
113 100
111 104.5 81.9 122.9
192 20.3 16.7 25.1

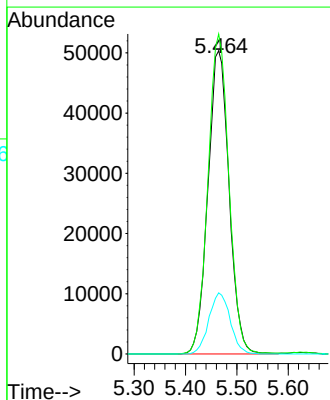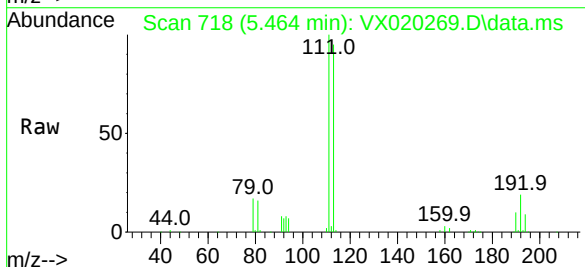






#36
1,1-Dichloropropene
Concen: 4.83 ug/l
RT: 5.629 min Scan# 745
Delta R.T. -0.134 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26


Instrument :
MSVOA_X
ClientSampleId :
PB133709TB





Tgt Ion: 75 Resp: 21764
Ion Ratio Lower Upper
75 100
110 8.4 18.1 54.4#
77 0.0 25.3 37.9#




#37
Ethyl Acetate
Concen: 1.53 ug/l
RT: 4.641 min Scan# 583
Delta R.T. -0.147 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26




Tgt Ion: 43 Resp: 7175
Ion Ratio Lower Upper
43 100
61 1.6 12.8 19.2#
70 0.0 10.5 15.7#

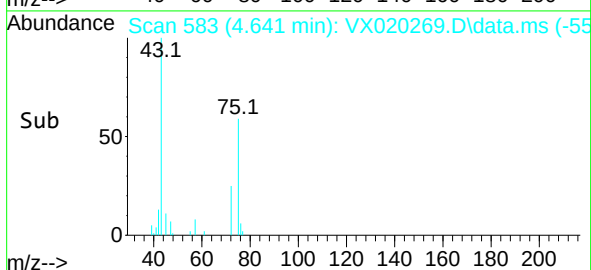






#38
Carbon Tetrachloride
Concen: 6.28 ug/l
RT: 5.623 min Scan# 744
Delta R.T. -0.122 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26

Instrument :
MSVOA_X
ClientSampleId :
PB133709TB







Tgt Ion: 117 Resp: 26900
Ion Ratio Lower Upper
117 100
119 6.1 76.2 114.2#
121 0.0 24.8 37.2#



#41
Methacrylonitrile
Concen: 0.29 ug/l
RT: 5.105 min Scan# 659
Delta R.T. 0.110 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26

Tgt Ion: 41 Resp: 721
Ion Ratio Lower Upper
41 100
39 20.0 42.5 63.7#
67 0.0 65.0 97.6#
52 0.0 25.3 37.9#


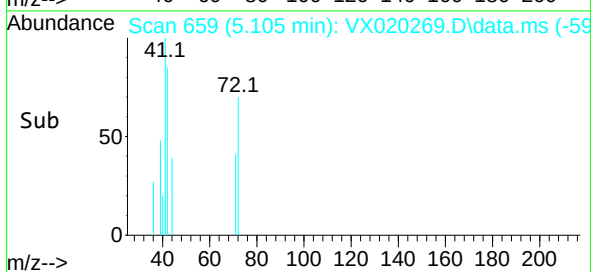




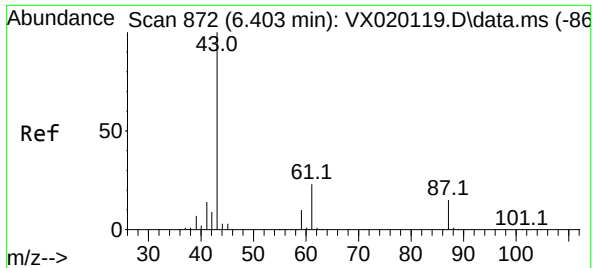

#43
Isopropyl Acetate
Concen: 3.40 ug/l
RT: 6.409 min Scan# 873
Delta R.T. 0.006 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26




Instrument :
MSVOA_X
ClientSampleId :
PB133709TB


Tgt Ion: 43	Resp: 25129
Ion Ratio	Lower Upper
43 100	
61 21.3	18.2 27.4
87 14.2	12.5 18.7

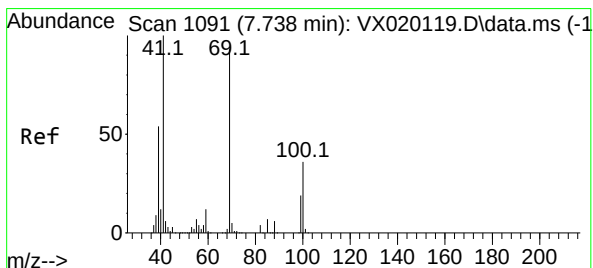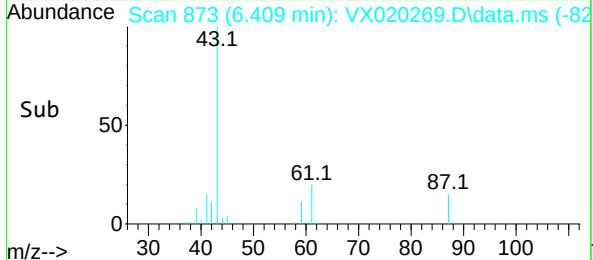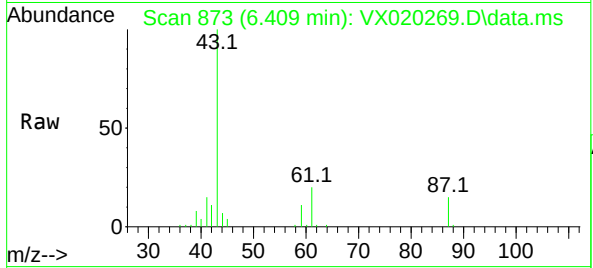

#48
Methyl methacrylate
Concen: 2.08 ug/l
RT: 7.647 min Scan# 1076
Delta R.T. -0.091 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26

Tgt Ion: 41	Resp: 7525
Ion Ratio	Lower Upper
41 100	
69 0.0	76.0 114.0#
39 0.0	44.6 67.0#


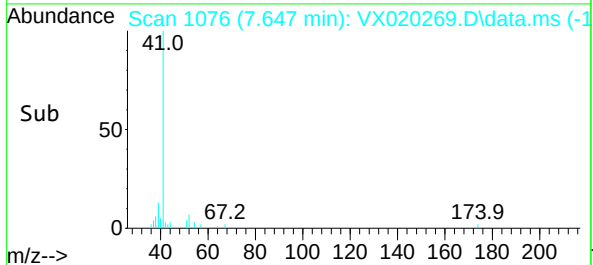

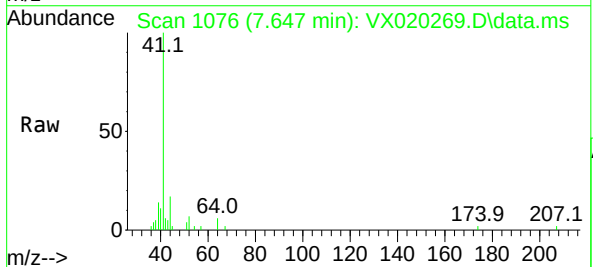




#49
1,4-Dioxane
Concen: 3.59 ug/l
RT: 7.848 min Scan# 1109
Delta R.T. 0.140 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26




Instrument :
MSVOA_X
ClientSampleId :
PB133709TB


Tgt Ion: 88 Resp: 304
Ion Ratio Lower Upper
88 100
43 486518.8 23.2 34.8#
58 2563.8 55.0 82.4#

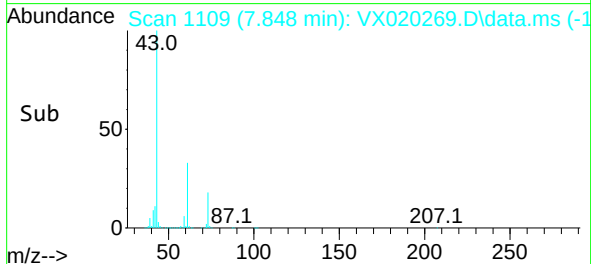

#50
Toluene-d8
Concen: 51.34 ug/l
RT: 8.696 min Scan# 1248
Delta R.T. 0.007 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26

Tgt Ion: 98 Resp: 576159
Ion Ratio Lower Upper
98 100
100 65.0 51.9 77.9









#51
4-Methyl-2-Pentanone
Concen: 19.24 ug/l
RT: 8.592 min Scan# 1231
Delta R.T. -0.024 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26




Instrument :
MSVOA_X
ClientSampleId :
PB133709TB


Tgt Ion: 43 Resp: 88006
Ion Ratio Lower Upper
43 100
58 9.9 35.4 53.0#

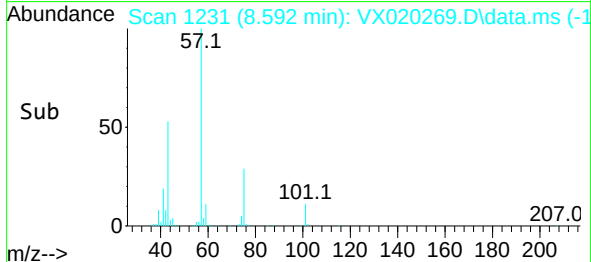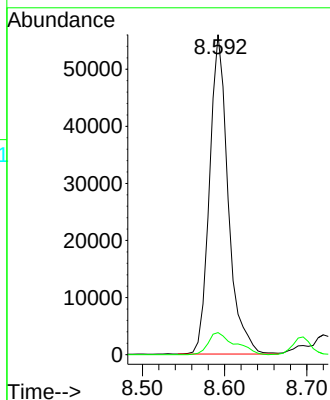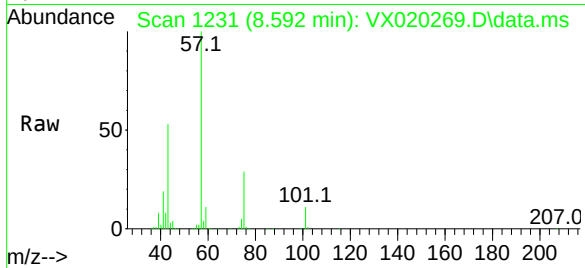

#52
Toluene
Concen: 0.20 ug/l
RT: 8.763 min Scan# 1259
Delta R.T. 0.001 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26

Tgt Ion: 92 Resp: 1727
Ion Ratio Lower Upper
92 100
91 170.7 137.1 205.7



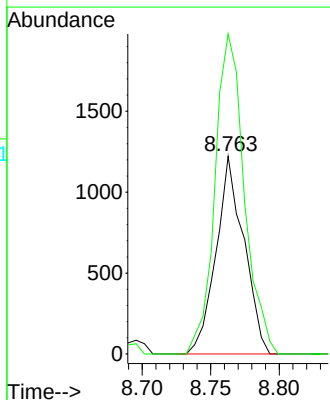
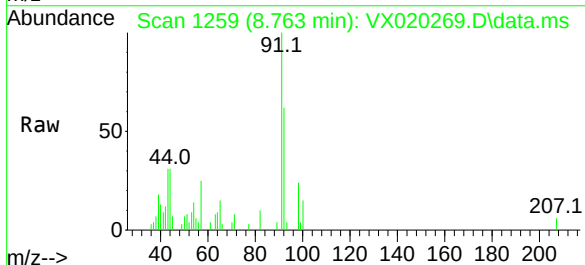




#54
cis-1,3-Dichloropropene
Concen: 8.15 ug/l
RT: 8.592 min Scan# 1231
Delta R.T. 0.183 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26




Instrument :
MSVOA_X
ClientSampleId :
PB133709TB


Tgt Ion: 75 Resp: 45470
Ion Ratio Lower Upper
75 100
77 0.9 25.7 38.5#
39 27.2 35.1 52.7#

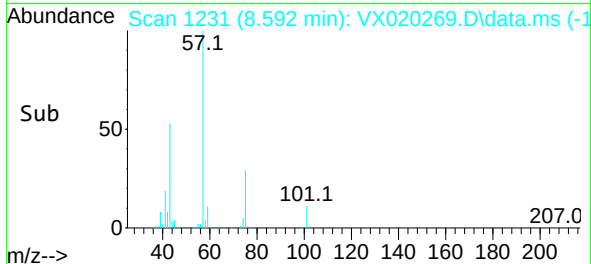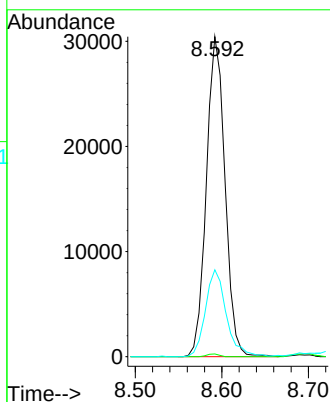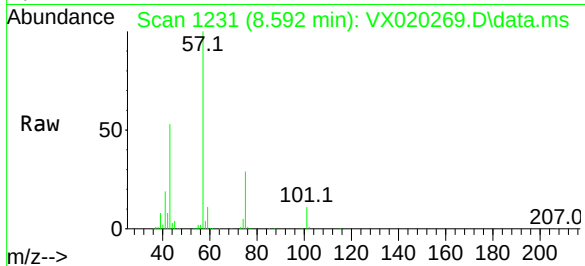

#57
1,3-Dichloropropane
Concen: 4.88 ug/l
RT: 9.525 min Scan# 1384
Delta R.T. 0.177 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26

Tgt Ion: 76 Resp: 29305
Ion Ratio Lower Upper
76 100
78 0.7 26.2 39.2#



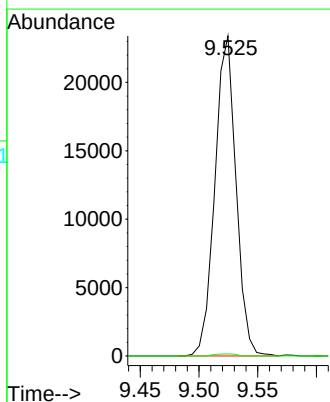
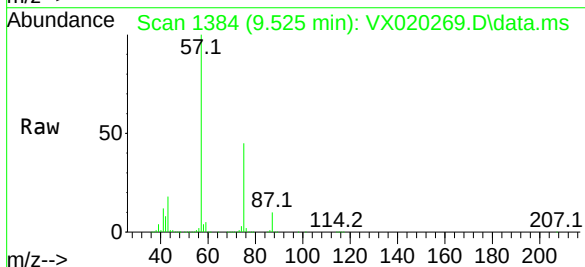




#59
2-Hexanone
Concen: 103.37 ug/l
RT: 9.525 min Scan# 1384
Delta R.T. 0.055 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26




Instrument :
MSVOA_X
ClientSampled :
PB133709TB


Tgt Ion: 43 Resp: 360382
Ion Ratio Lower Upper
43 100
58 20.5 30.9 92.8#

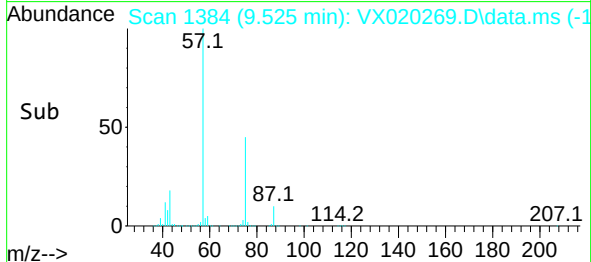

#62
4-Bromofluorobenzene
Concen: 46.72 ug/l
RT: 11.122 min Scan# 1646
Delta R.T. -0.000 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26

Tgt Ion: 95 Resp: 200658
Ion Ratio Lower Upper
95 100
174 74.2 0.0 154.6
176 73.0 0.0 155.8




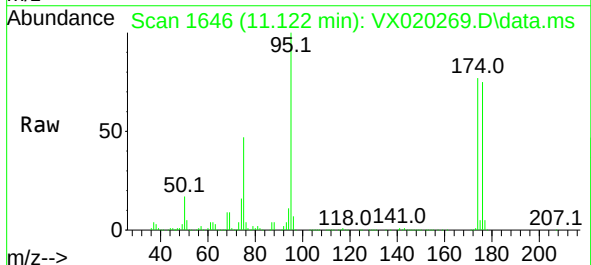




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.098 min Scan# 1478
Delta R.T. 0.006 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26




Instrument :
MSVOA_X
ClientSampleId :
PB133709TB


Tgt Ion:117 Resp: 439877
Ion Ratio Lower Upper
117 100
82 54.0 47.4 71.2
119 31.4 26.6 39.8

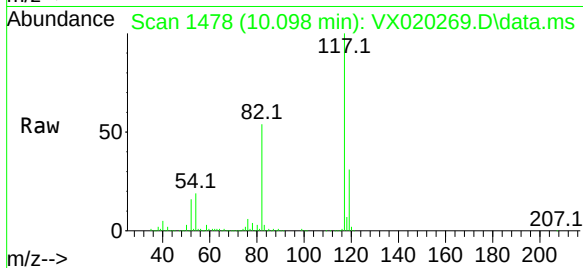

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.061 min Scan# 1800
Delta R.T. -0.000 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26

Tgt Ion:152 Resp: 181873
Ion Ratio Lower Upper
152 100
115 61.2 41.1 123.3
150 157.2 0.0 349.0


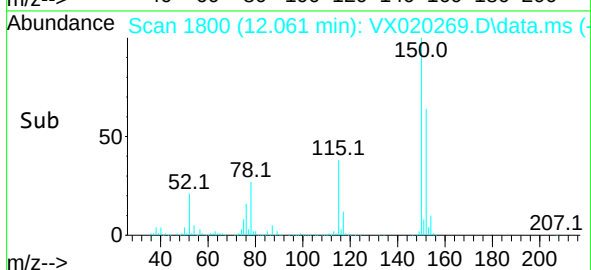

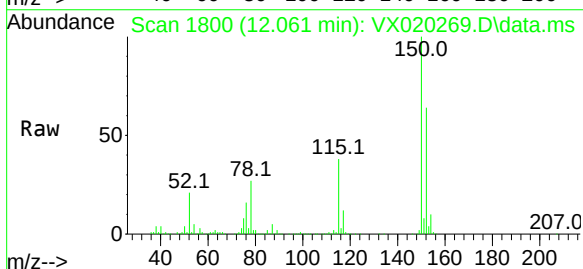




#76
1,2,3-Trichloropropane
Concen: 21.37 ug/l
RT: 11.122 min Scan# 1646
Delta R.T. -0.158 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26




Instrument :
MSVOA_X
ClientSampleId :
PB133709TB


Tgt Ion: 75 Resp: 95752
Ion Ratio Lower Upper
75 100
77 1.3 19.1 57.5#

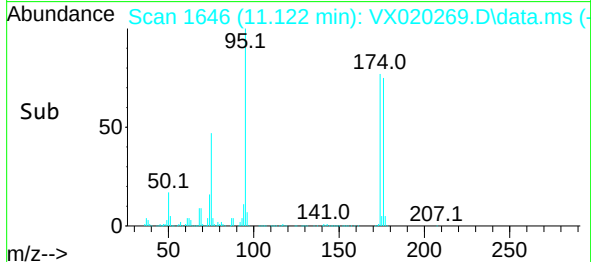

#80
1,3,5-Trimethylbenzene
Concen: 0.25 ug/l
RT: 11.488 min Scan# 1706
Delta R.T. -0.000 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26


Tgt Ion: 105 Resp: 2812
Ion Ratio Lower Upper
105 100
120 42.5 23.8 71.5

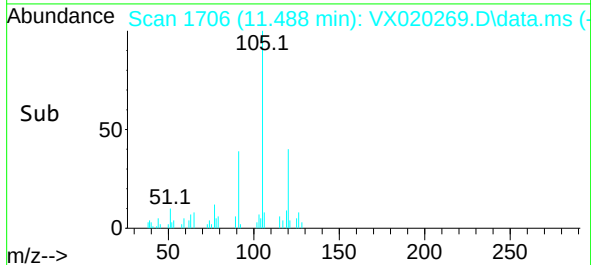






#81
trans-1,4-Dichloro-2-butene
Concen: 63.41 ug/l
RT: 11.122 min Scan# 1646
Delta R.T. 0.067 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26

Instrument :
MSVOA_X
ClientSampleId :
PB133709TB







Tgt Ion: 75 Resp: 95752
Ion Ratio Lower Upper
75 100
53 0.1 74.5 111.7#
89 0.0 37.9 56.9#



#93
1,2,4-Trichlorobenzene
Concen: 0.24 ug/l
RT: 13.628 min Scan# 2057
Delta R.T. 0.001 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26

Tgt Ion: 180 Resp: 948
Ion Ratio Lower Upper
180 100
182 99.3 47.7 143.1
145 27.1 15.0 45.0


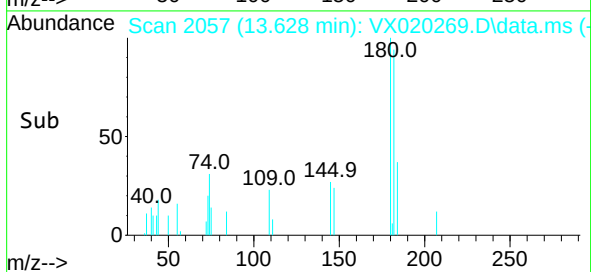






#94
Hexachlorobutadiene
Concen: 2.91 ug/l
RT: 13.762 min Scan# 2079
Delta R.T. -0.006 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26

Instrument :
MSVOA_X
ClientSampled :
PB133709TB

Tgt Ion:225 Resp: 464
Ion Ratio Lower Upper
225 100
223 59.5 31.1 93.2
227 78.2 31.6 95.0

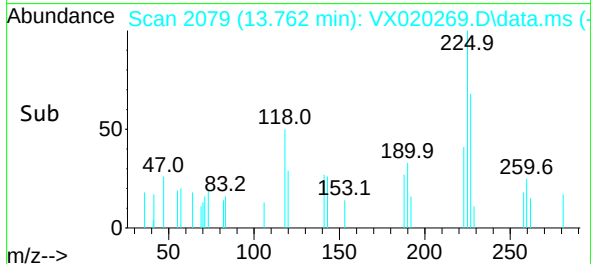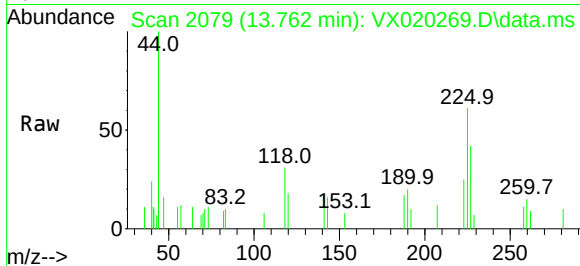

#96
1,2,3-Trichlorobenzene
Concen: 0.20 ug/l
RT: 13.999 min Scan# 2118
Delta R.T. 0.000 min
Lab File: VX020269.D
Acq: 21 Dec 2020 23:26

Tgt Ion:180 Resp: 792
Ion Ratio Lower Upper
180 100
182 97.5 47.6 142.9
145 28.3 16.1 48.3

