

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025965.D
 Acq On : 21 Dec 2021 18:29
 Operator : JC/MD
 Sample : M5126-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J25

Quant Time: Dec 22 05:40:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 22 05:35:20 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	126332	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	162811	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	50862	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	49247	48.352	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	96.700%	
7) Chloroethane-d5	1.666	69	47223	55.524	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	111.040%	
11) 1,1-Dichloroethene-d2	2.306	63	70414	39.804	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	79.600%	
21) 2-Butanone-d5	4.458	46	89041	121.185	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	121.190%	
24) Chloroform-d	5.062	84	104608	53.580	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	107.160%	
26) 1,2-Dichloroethane-d4	5.958	65	73121	57.424	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	114.840%	
32) Benzene-d6	5.976	84	207761	42.120	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	84.240%	
36) 1,2-Dichloropropane-d6	7.312	67	63246	42.098	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	84.200%	
41) Toluene-d8	8.653	98	246757	52.686	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	105.380%	
43) trans-1,3-Dichloroprop...	8.951	79	29595	44.615	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	89.240%	
47) 2-Hexanone-d5	9.384	63	93114	137.875	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	137.880%#	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	87657	41.186	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	82.380%	
66) 1,2-Dichlorobenzene-d4	12.323	152	59583	55.576	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	111.160%	
Target Compounds						
13) Acetone	2.380	43	2998	5.100	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025965.D
Acq On : 21 Dec 2021 18:29
Operator : JC/MD
Sample : M5126-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J25

Quant Time: Dec 22 05:40:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 22 05:35:20 2021
Response via : Initial Calibration

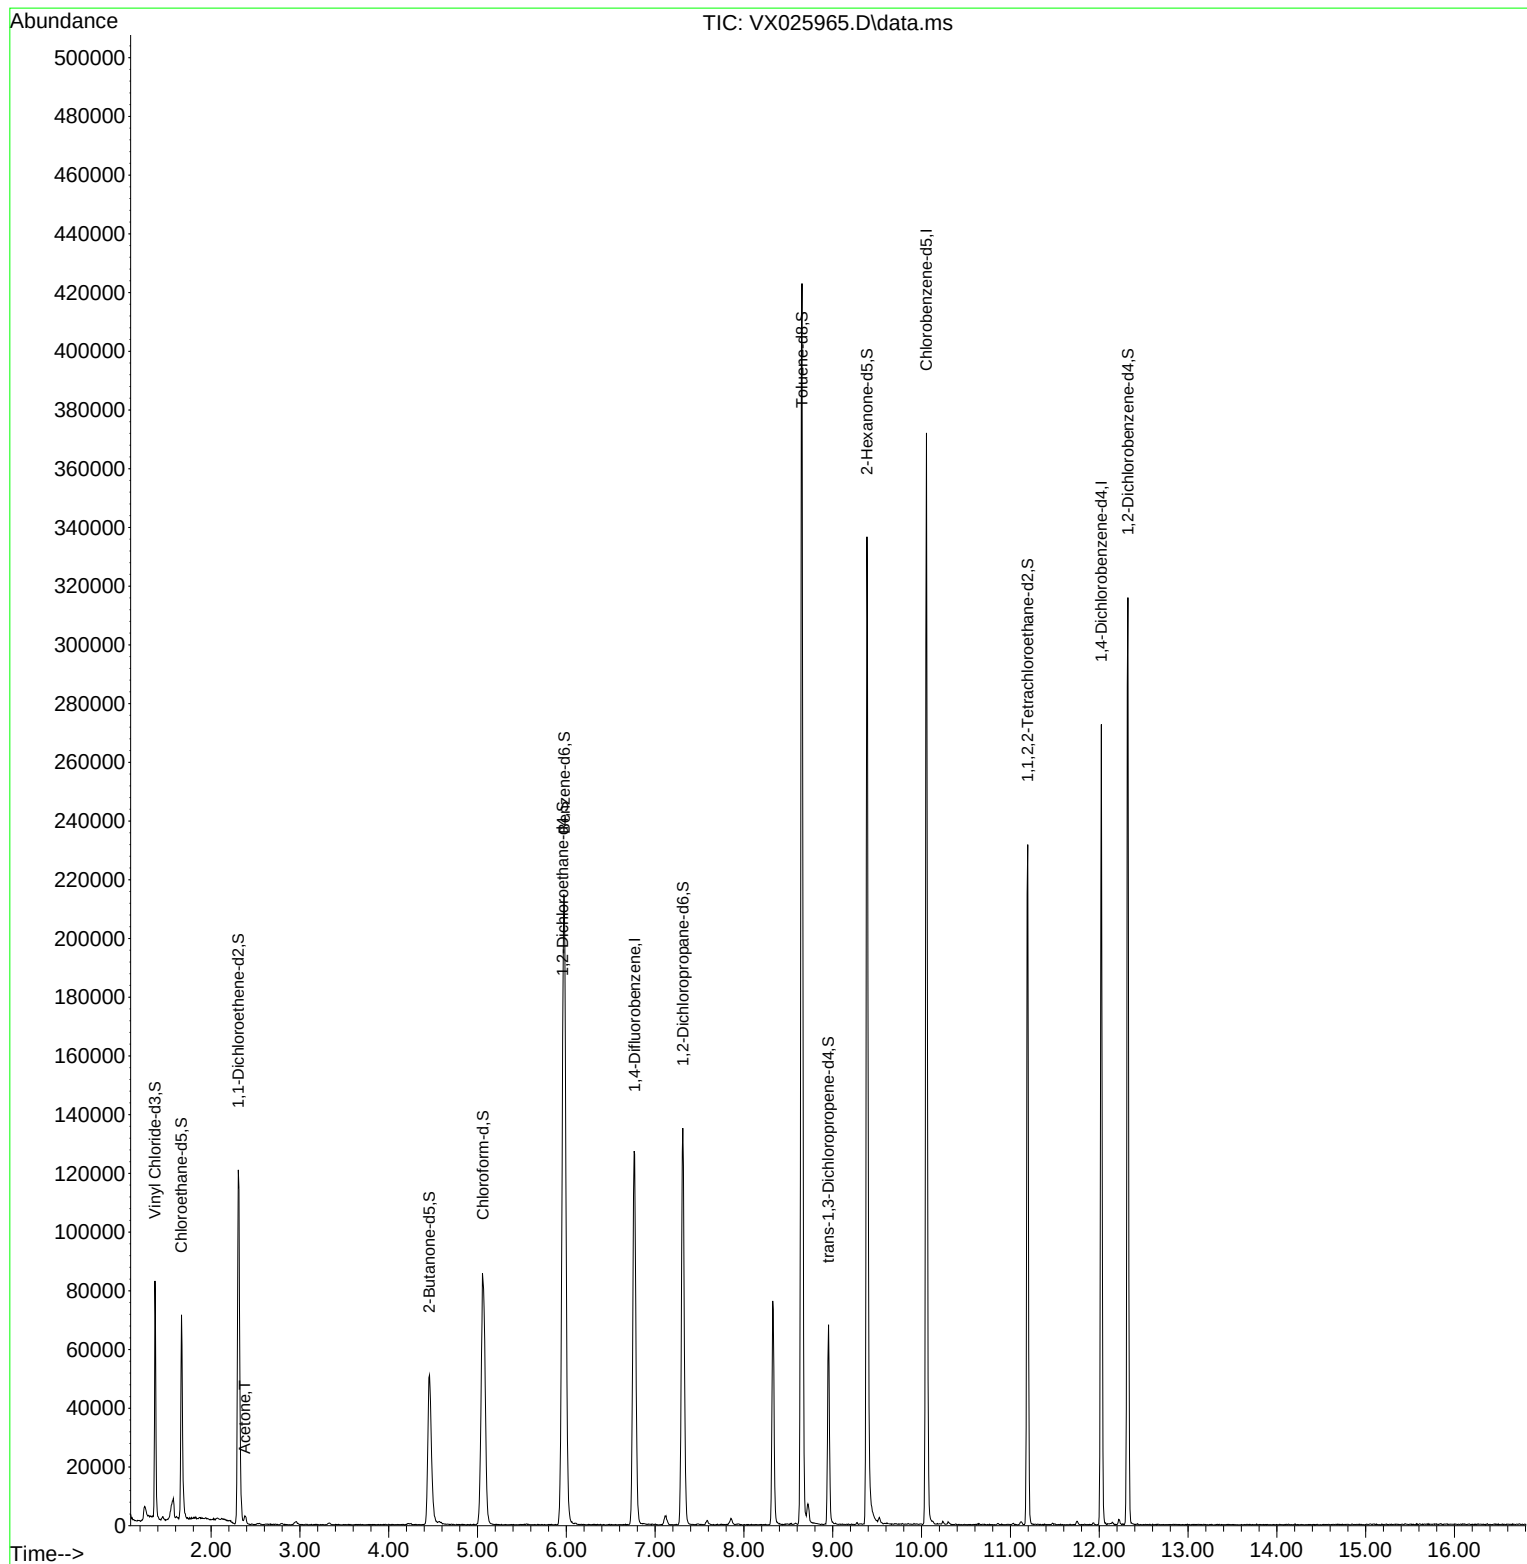

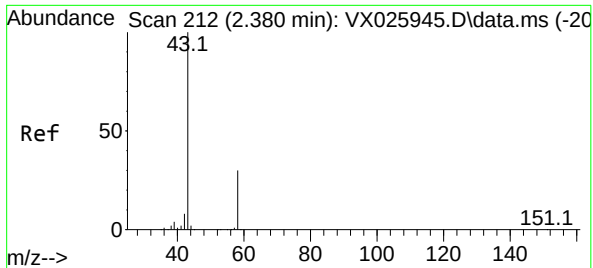

#13
 Acetone
 Concen: 5.100 ug/L
 RT: 2.380 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VX025965.D
 Acq: 21 Dec 2021 18:29

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J25

Tgt Ion: 43 Resp: 2998
 Ion Ratio Lower Upper
 43 100
 58 29.8 0.0 65.6

