

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025946.D
 Acq On : 21 Dec 2021 11:00
 Operator : JC/MD
 Sample : VX1221WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK655

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025946.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	55	rVB	92306	92271	12.93%	1.743%
2	1.666	91	95	106	rVB	74577	98087	13.74%	1.853%
3	2.306	193	200	213	rBV	140472	229277	32.12%	4.332%
4	2.514	229	234	240	rVV	2859	4968	0.70%	0.094%
5	2.581	243	245	248	rVB2	258	297	0.04%	0.006%
6	2.697	261	264	265	rBV2	283	301	0.04%	0.006%
7	2.715	265	267	269	rBV2	320	260	0.04%	0.005%
8	2.788	275	279	285	rBV3	1511	2655	0.37%	0.050%
9	3.032	317	319	323	rBV2	269	390	0.05%	0.007%
10	3.093	323	329	335	rVV4	1502	3494	0.49%	0.066%
11	3.160	338	340	341	rVB	351	192	0.03%	0.004%
12	3.404	377	380	383	rVB2	303	408	0.06%	0.008%
13	3.550	401	404	407	rBV	293	289	0.04%	0.005%
14	3.581	407	409	412	rBV	206	276	0.04%	0.005%
15	3.885	457	459	464	rVB2	214	262	0.04%	0.005%
16	4.294	524	526	528	rVB	279	249	0.03%	0.005%
17	4.452	541	552	572	rBV2	54718	161197	22.59%	3.045%
18	4.690	589	591	593	rVB2	281	218	0.03%	0.004%
19	4.714	593	595	597	rBV	187	204	0.03%	0.004%
20	4.733	597	598	601	rVB2	328	302	0.04%	0.006%
21	4.782	604	606	608	rVV2	330	280	0.04%	0.005%
22	4.873	619	621	622	rBV	227	200	0.03%	0.004%
23	4.897	622	625	626	rVV2	428	396	0.06%	0.007%
24	4.934	629	631	634	rBV	177	206	0.03%	0.004%
25	5.056	639	651	670	rBV	92552	291256	40.81%	5.502%
26	5.227	677	679	682	rBV	194	251	0.04%	0.005%
27	5.379	702	704	705	rBV	244	248	0.03%	0.005%
28	5.666	748	751	752	rBV	181	204	0.03%	0.004%
29	5.733	760	762	765	rVB	314	277	0.04%	0.005%
30	5.970	787	801	819	rBV2	237555	713715	100.00%	13.484%
31	6.184	835	836	837	rBV2	420	234	0.03%	0.004%
32	6.421	873	875	878	rVB2	200	234	0.03%	0.004%
33	6.476	882	884	888	rVV2	178	224	0.03%	0.004%
34	6.757	921	930	945	rBV	149431	357264	50.06%	6.749%
35	7.031	972	975	978	rVB2	203	236	0.03%	0.004%
36	7.110	981	988	998	rVB5	4823	12594	1.76%	0.238%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025946.D
 Acq On : 21 Dec 2021 11:00
 Operator : JC/MD
 Sample : VX1221WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK655

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

37	7.305	1012	1020	1039	rVV	143741	324575	45.48%	6.132%
38	7.434	1039	1041	1046	rVV2	420	660	0.09%	0.012%
39	7.476	1046	1048	1051	rVV2	644	683	0.10%	0.013%
40	7.507	1051	1053	1061	rVV2	279	487	0.07%	0.009%
41	7.921	1117	1121	1122	rBV	363	410	0.06%	0.008%
42	8.275	1177	1179	1181	rBV2	201	247	0.03%	0.005%
43	8.324	1181	1187	1201	rVV	94052	157860	22.12%	2.982%
44	8.476	1209	1212	1214	rBV3	420	479	0.07%	0.009%
45	8.647	1234	1240	1248	rBV	367850	570660	79.96%	10.781%
46	8.952	1284	1290	1299	rBV	64120	96773	13.56%	1.828%
47	9.086	1310	1312	1314	rVB2	209	190	0.03%	0.004%
48	9.159	1321	1324	1326	rBV2	602	518	0.07%	0.010%
49	9.275	1338	1343	1347	rBV3	2277	3079	0.43%	0.058%
50	9.384	1355	1361	1381	rBV	247511	355860	49.86%	6.723%
51	9.665	1405	1407	1410	rBV2	345	267	0.04%	0.005%
52	9.805	1426	1430	1431	rBV2	222	213	0.03%	0.004%
53	9.829	1431	1434	1437	rVB	328	348	0.05%	0.007%
54	9.860	1437	1439	1442	rBV	270	301	0.04%	0.006%
55	9.903	1444	1446	1448	rBV	174	187	0.03%	0.004%
56	10.055	1465	1471	1481	rBV	331655	457002	64.03%	8.634%
57	10.195	1490	1494	1498	rVB2	2868	3864	0.54%	0.073%
58	10.305	1507	1512	1519	rVB3	3033	4640	0.65%	0.088%
59	10.652	1563	1569	1575	rBV4	3729	6200	0.87%	0.117%
60	10.713	1577	1579	1582	rVB2	247	319	0.04%	0.006%
61	10.799	1591	1593	1596	rVV2	244	257	0.04%	0.005%
62	10.963	1616	1620	1624	rVV2	3057	3506	0.49%	0.066%
63	11.091	1639	1641	1643	rBV2	428	528	0.07%	0.010%
64	11.122	1643	1646	1652	rVB2	2244	2162	0.30%	0.041%
65	11.195	1652	1658	1664	rBV	255609	343001	48.06%	6.480%
66	11.274	1669	1671	1673	rBV2	304	347	0.05%	0.007%
67	11.451	1696	1700	1708	rBV2	3413	4400	0.62%	0.083%
68	11.549	1714	1716	1718	rVB	258	201	0.03%	0.004%
69	11.689	1737	1739	1742	rBV2	257	353	0.05%	0.007%
70	11.750	1745	1749	1756	rVB2	4899	6585	0.92%	0.124%
71	11.847	1761	1765	1767	rBV2	353	381	0.05%	0.007%
72	11.933	1776	1779	1782	rBV2	1041	1210	0.17%	0.023%
73	11.969	1782	1785	1789	rVV	5612	6699	0.94%	0.127%
74	12.024	1789	1794	1806	rVB	332230	433764	60.78%	8.195%
75	12.134	1806	1812	1813	rBV3	911	1346	0.19%	0.025%
76	12.152	1813	1815	1818	rVB3	1517	1371	0.19%	0.026%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025946.D
 Acq On : 21 Dec 2021 11:00
 Operator : JC/MD
 Sample : VX1221WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK655

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

77	12.213	1821	1825	1827	rVB2	233	266	0.04%	0.005%
78	12.238	1827	1829	1832	rVB2	185	190	0.03%	0.004%
79	12.323	1837	1843	1850	rVB	369546	483559	67.75%	9.135%
80	12.427	1858	1860	1863	rBV3	636	568	0.08%	0.011%
81	12.658	1896	1898	1901	rBV2	416	477	0.07%	0.009%
82	12.945	1941	1945	1951	rVB3	407	622	0.09%	0.012%
83	13.054	1961	1963	1968	rVB2	285	281	0.04%	0.005%
84	13.115	1968	1973	1979	rBV3	10304	12927	1.81%	0.244%
85	13.591	2047	2051	2056	rVB2	8629	10871	1.52%	0.205%
86	13.664	2060	2063	2065	rBV2	210	258	0.04%	0.005%
87	13.780	2078	2082	2087	rVB	3855	4580	0.64%	0.087%
88	13.920	2103	2105	2108	rBV	204	208	0.03%	0.004%
89	13.963	2108	2112	2118	rVB	8835	9935	1.39%	0.188%
90	14.292	2165	2166	2169	rBV	313	216	0.03%	0.004%
91	14.615	2218	2219	2225	rVB2	270	315	0.04%	0.006%
92	14.993	2280	2281	2286	rVB2	261	366	0.05%	0.007%
93	15.176	2310	2311	2314	rBV2	192	231	0.03%	0.004%
94	15.359	2338	2341	2344	rBV2	279	417	0.06%	0.008%
95	15.548	2369	2372	2374	rBV2	288	269	0.04%	0.005%
96	15.572	2374	2376	2378	rBV2	300	366	0.05%	0.007%
97	15.591	2378	2379	2381	rVB	456	196	0.03%	0.004%
98	15.975	2441	2442	2444	rBV	309	251	0.04%	0.005%
99	16.030	2449	2451	2453	rVV2	205	213	0.03%	0.004%
100	16.286	2491	2493	2496	rBV2	258	283	0.04%	0.005%




Sum of corrected areas: 5293214

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025946.D
Acq On : 21 Dec 2021 11:00
Operator : JC/MD
Sample : VX1221WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK655

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

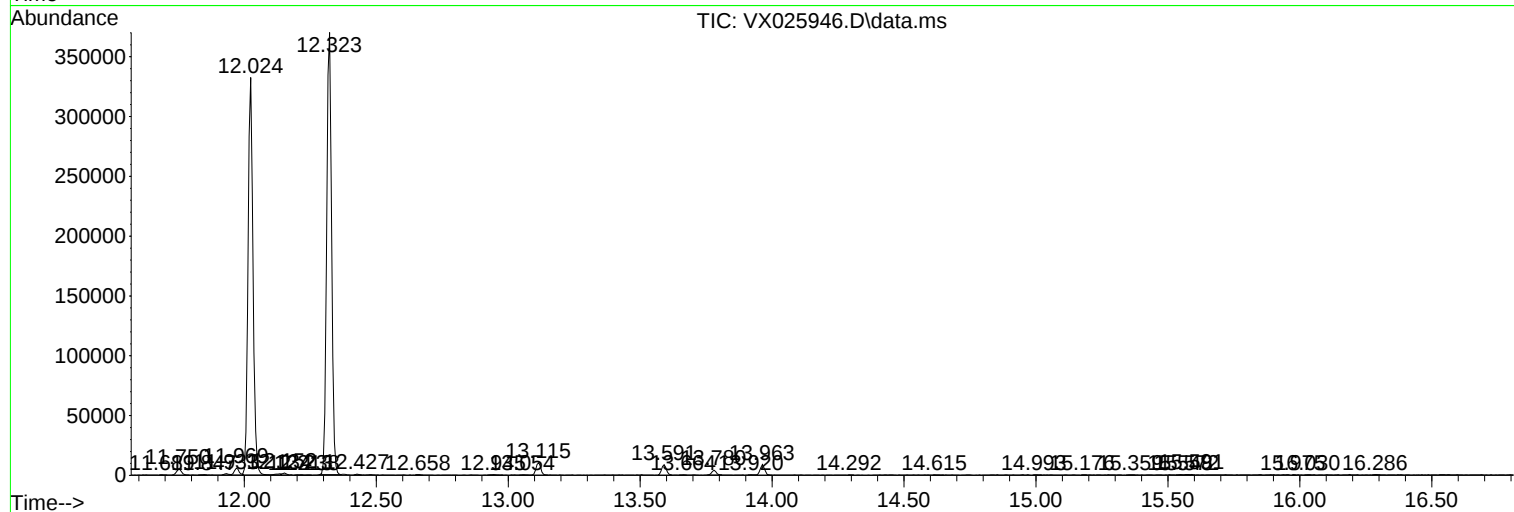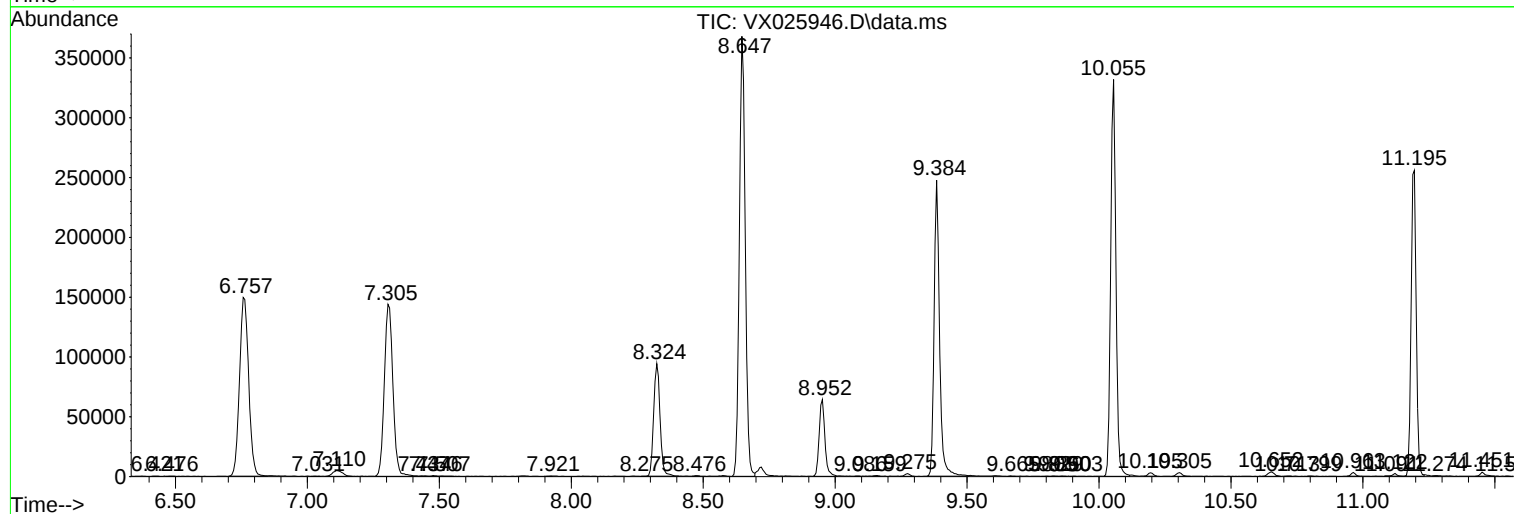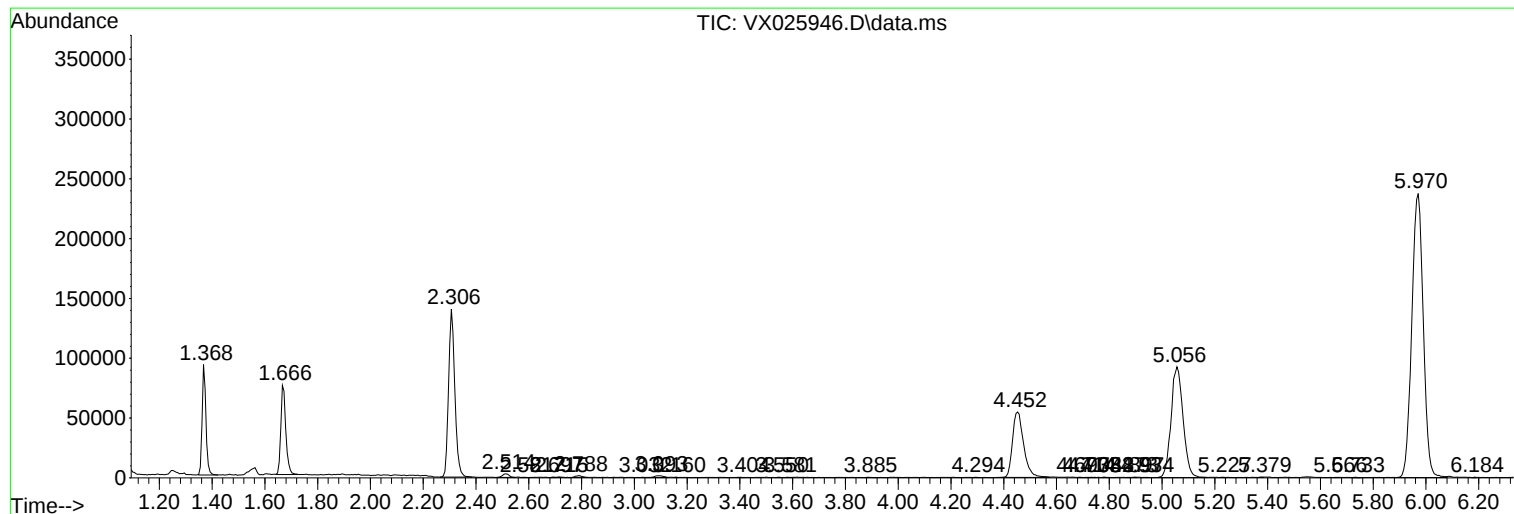

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025946.D
Acq On : 21 Dec 2021 11:00
Operator : JC/MD
Sample : VX1221WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK655

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025946.D
Acq On : 21 Dec 2021 11:00
Operator : JC/MD
Sample : VX1221WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK655

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc