

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025947.D
 Acq On : 21 Dec 2021 11:29
 Operator : JC/MD
 Sample : M5150-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025947.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	33	rBV2	3066	7103	0.34%	0.108%
2	1.368	43	46	53	rVB	77516	79912	3.80%	1.213%
3	1.666	91	95	103	rVB	65106	80475	3.83%	1.222%
4	2.307	194	200	208	rBV	115421	189956	9.04%	2.884%
5	2.380	208	212	221	rVB	13030	21254	1.01%	0.323%
6	2.514	231	234	237	rVB2	752	1029	0.05%	0.016%
7	2.703	262	265	266	rBV3	315	364	0.02%	0.006%
8	2.794	275	280	283	rVB4	474	897	0.04%	0.014%
9	2.880	293	294	297	rBV2	208	263	0.01%	0.004%
10	2.947	298	305	313	rVB2	2468	6109	0.29%	0.093%
11	3.087	326	328	332	rVV3	922	1055	0.05%	0.016%
12	3.337	367	369	372	rBV2	196	206	0.01%	0.003%
13	3.660	420	422	424	rBV2	186	185	0.01%	0.003%
14	4.056	485	487	489	rVV	219	189	0.01%	0.003%
15	4.166	504	505	508	rBV2	263	249	0.01%	0.004%
16	4.379	538	540	543	rBV2	226	236	0.01%	0.004%
17	4.465	543	554	555	rBV	51504	116085	5.52%	1.763%
18	4.806	608	610	612	rBV2	237	266	0.01%	0.004%
19	5.062	638	652	665	rBV	77749	243525	11.59%	3.697%
20	5.391	695	706	709	rBV3	834	1885	0.09%	0.029%
21	5.471	712	719	729	rVB3	4743	13562	0.65%	0.206%
22	5.623	740	744	745	rVB2	195	221	0.01%	0.003%
23	5.971	789	801	816	rBV2	199182	592896	28.21%	9.002%
24	6.214	839	841	844	rBV2	264	310	0.01%	0.005%
25	6.257	846	848	853	rVV2	281	382	0.02%	0.006%
26	6.342	860	862	867	rVV2	276	375	0.02%	0.006%
27	6.428	873	876	877	rBV	215	211	0.01%	0.003%
28	6.507	888	889	892	rBV2	240	202	0.01%	0.003%
29	6.544	892	895	897	rVB2	287	265	0.01%	0.004%
30	6.580	899	901	904	rVB	273	245	0.01%	0.004%
31	6.647	909	912	914	rBV2	257	255	0.01%	0.004%
32	6.763	921	931	943	rBV	144244	346044	16.47%	5.254%
33	7.123	981	990	1012	rVV	948054	2101687	100.00%	31.910%
34	7.306	1012	1020	1032	rVB	122717	266368	12.67%	4.044%
35	7.470	1044	1047	1048	rBV2	273	299	0.01%	0.005%
36	7.623	1069	1072	1075	rBV2	149	191	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025947.D
 Acq On : 21 Dec 2021 11:29
 Operator : JC/MD
 Sample : M5150-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

37	7.696	1083	1084	1088	rBV2	175	194	0.01%	0.003%
38	7.793	1096	1100	1101	rBV	233	259	0.01%	0.004%
39	7.836	1105	1107	1110	rVB2	253	279	0.01%	0.004%
40	7.891	1114	1116	1119	rBV2	270	268	0.01%	0.004%
41	8.244	1173	1174	1177	rVB	244	202	0.01%	0.003%
42	8.324	1180	1187	1196	rBV	79198	128875	6.13%	1.957%
43	8.525	1218	1220	1221	rVB2	307	201	0.01%	0.003%
44	8.647	1234	1240	1248	rBV	298973	476953	22.69%	7.242%
45	8.720	1249	1252	1259	rVV2	5097	7939	0.38%	0.121%
46	8.952	1284	1290	1297	rBV	52169	75098	3.57%	1.140%
47	9.275	1339	1343	1349	rVB4	1350	2012	0.10%	0.031%
48	9.385	1355	1361	1376	rBV	191967	275310	13.10%	4.180%
49	9.616	1398	1399	1403	rVB2	441	306	0.01%	0.005%
50	9.653	1403	1405	1407	rBV2	176	186	0.01%	0.003%
51	9.933	1447	1451	1452	rVB2	257	234	0.01%	0.004%
52	9.994	1459	1461	1463	rBV	198	251	0.01%	0.004%
53	10.055	1465	1471	1486	rVV	335192	447999	21.32%	6.802%
54	10.201	1491	1495	1501	rVB3	694	1213	0.06%	0.018%
55	10.305	1508	1512	1517	rBV4	1160	1747	0.08%	0.027%
56	10.360	1519	1521	1525	rVB	267	199	0.01%	0.003%
57	10.433	1531	1533	1535	rBV	413	356	0.02%	0.005%
58	10.494	1541	1543	1548	rVB2	153	207	0.01%	0.003%
59	10.543	1548	1551	1557	rBV3	188	285	0.01%	0.004%
60	10.653	1565	1569	1573	rVB4	729	1075	0.05%	0.016%
61	10.903	1608	1610	1613	rBV2	194	219	0.01%	0.003%
62	11.079	1635	1639	1642	rBV3	1740	2436	0.12%	0.037%
63	11.116	1643	1645	1649	rVB2	1919	2175	0.10%	0.033%
64	11.195	1652	1658	1667	rBV	214084	280242	13.33%	4.255%
65	11.305	1674	1676	1683	rVB3	503	865	0.04%	0.013%
66	11.366	1683	1686	1687	rBV	226	185	0.01%	0.003%
67	11.451	1698	1700	1701	rBV2	273	191	0.01%	0.003%
68	11.549	1714	1716	1719	rVB2	250	209	0.01%	0.003%
69	11.750	1746	1749	1753	rVB3	1303	1958	0.09%	0.030%
70	11.811	1756	1759	1761	rVB2	217	257	0.01%	0.004%
71	11.835	1761	1763	1767	rBV2	398	466	0.02%	0.007%
72	11.933	1776	1779	1782	rBV3	882	1063	0.05%	0.016%
73	11.969	1782	1785	1789	rBV2	618	729	0.03%	0.011%
74	12.024	1789	1794	1806	rBV	318112	402119	19.13%	6.105%
75	12.146	1813	1814	1818	rVB3	974	990	0.05%	0.015%
76	12.219	1824	1826	1832	rBV3	619	711	0.03%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025947.D
 Acq On : 21 Dec 2021 11:29
 Operator : JC/MD
 Sample : M5150-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GBBX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

77	12.323	1837	1843	1851	rVB	290210	387058	18.42%	5.877%
78	12.427	1856	1860	1863	rVB2	488	521	0.02%	0.008%
79	12.482	1865	1869	1871	rBV	186	273	0.01%	0.004%
80	13.018	1955	1957	1960	rVB	331	258	0.01%	0.004%
81	13.116	1970	1973	1978	rVB3	459	665	0.03%	0.010%
82	13.158	1978	1980	1983	rBV2	183	192	0.01%	0.003%
83	13.372	2013	2015	2017	rVV2	256	207	0.01%	0.003%
84	13.512	2036	2038	2040	rVB2	312	233	0.01%	0.004%
85	13.591	2048	2051	2054	rVB2	746	663	0.03%	0.010%
86	13.646	2059	2060	2063	rVV2	248	219	0.01%	0.003%
87	13.780	2079	2082	2085	rVB2	655	640	0.03%	0.010%
88	13.823	2088	2089	2093	rVV	235	198	0.01%	0.003%
89	13.963	2111	2112	2115	rBV3	325	334	0.02%	0.005%
90	14.134	2137	2140	2142	rVB2	261	301	0.01%	0.005%
91	14.707	2230	2234	2237	rBV2	335	418	0.02%	0.006%
92	15.012	2281	2284	2289	rVB2	190	326	0.02%	0.005%
93	15.066	2289	2293	2294	rBV	369	445	0.02%	0.007%
94	15.213	2315	2317	2319	rBV2	297	216	0.01%	0.003%
95	15.451	2354	2356	2357	rBV2	276	211	0.01%	0.003%
96	15.615	2377	2383	2385	rBV3	279	589	0.03%	0.009%
97	15.713	2396	2399	2403	rBV3	230	363	0.02%	0.006%
98	15.889	2425	2428	2429	rBV2	224	215	0.01%	0.003%
99	15.938	2435	2436	2439	rBV2	221	193	0.01%	0.003%
100	16.517	2529	2531	2533	rBV	239	271	0.01%	0.004%




Sum of corrected areas: 6586228

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025947.D
Acq On : 21 Dec 2021 11:29
Operator : JC/MD
Sample : M5150-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

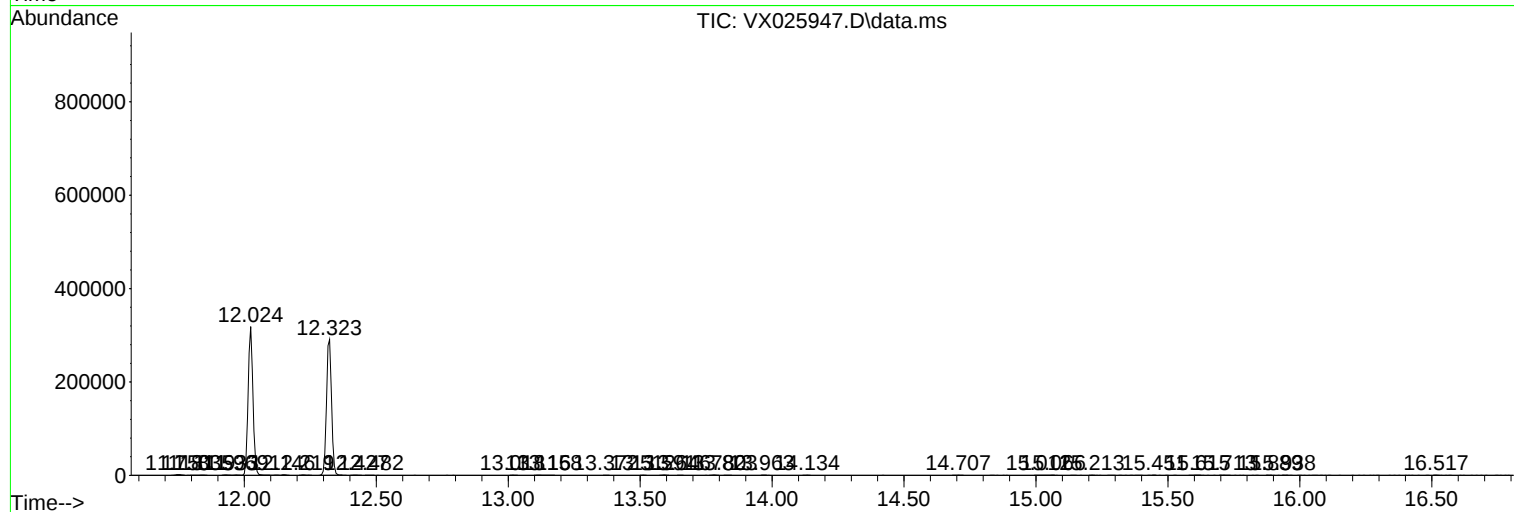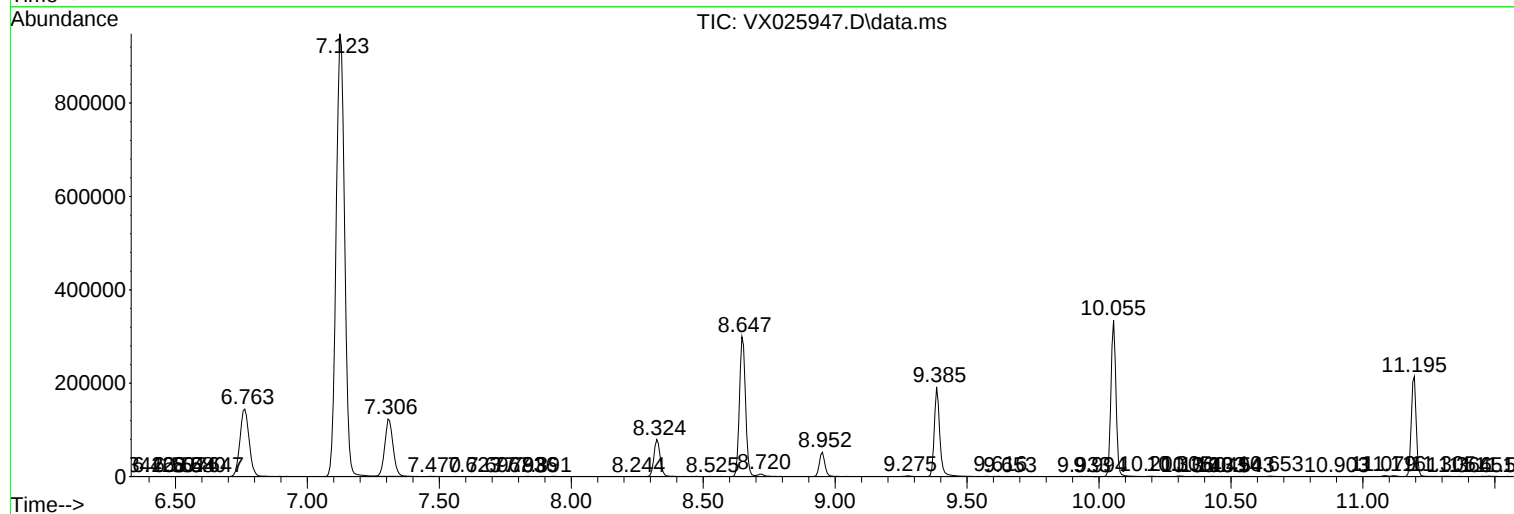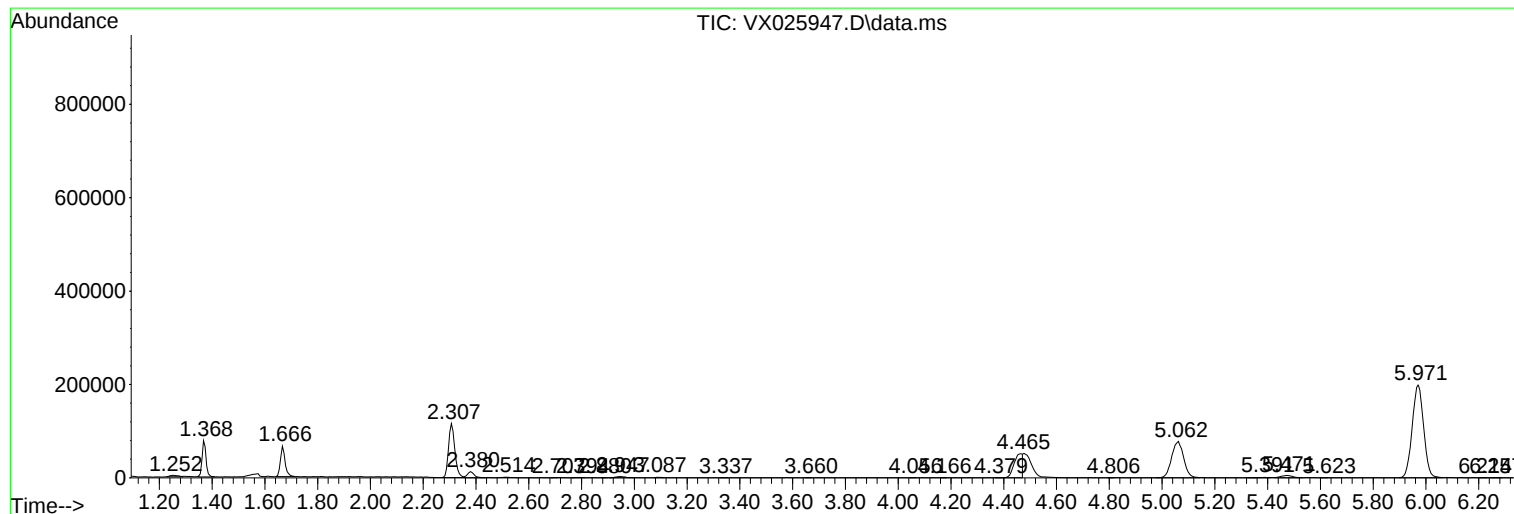

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025947.D
Acq On : 21 Dec 2021 11:29
Operator : JC/MD
Sample : M5150-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025947.D
Acq On : 21 Dec 2021 11:29
Operator : JC/MD
Sample : M5150-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GBBX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc