

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025948.D
 Acq On : 21 Dec 2021 11:52
 Operator : JC/MD
 Sample : M5126-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025948.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	54	rVB	86769	84466	13.24%	1.793%
2	1.666	91	95	104	rVB	67524	89763	14.07%	1.905%
3	2.307	194	200	211	rBV	121596	201349	31.56%	4.273%
4	2.611	248	250	253	rVB	257	260	0.04%	0.006%
5	2.709	262	266	269	rBV3	319	398	0.06%	0.008%
6	2.800	276	281	284	rVB2	467	783	0.12%	0.017%
7	2.837	284	287	290	rBV	275	264	0.04%	0.006%
8	2.947	298	305	315	rBV3	974	2285	0.36%	0.048%
9	3.099	326	330	332	rVB	371	389	0.06%	0.008%
10	3.142	335	337	339	rVV	237	194	0.03%	0.004%
11	3.258	354	356	358	rVB2	305	213	0.03%	0.005%
12	3.434	383	385	387	rBV2	212	188	0.03%	0.004%
13	3.849	450	453	455	rBV2	172	190	0.03%	0.004%
14	4.361	536	537	540	rBV2	238	225	0.04%	0.005%
15	4.459	540	553	568	rBV	47088	142656	22.36%	3.027%
16	4.702	591	593	598	rVB2	295	353	0.06%	0.007%
17	4.904	624	626	627	rBV	290	230	0.04%	0.005%
18	5.062	640	652	666	rBV2	90978	260926	40.90%	5.537%
19	5.184	671	672	675	rVB2	313	280	0.04%	0.006%
20	5.391	699	706	713	rVB4	1711	4424	0.69%	0.094%
21	5.532	727	729	731	rBV2	212	254	0.04%	0.005%
22	5.550	731	732	739	rVV2	404	686	0.11%	0.015%
23	5.977	790	802	818	rBV2	213304	637930	100.00%	13.538%
24	6.477	882	884	888	rVB2	269	288	0.05%	0.006%
25	6.525	890	892	893	rVV2	213	178	0.03%	0.004%
26	6.550	895	896	900	rVV	376	278	0.04%	0.006%
27	6.763	922	931	946	rVV	142732	337275	52.87%	7.158%
28	7.123	982	990	1000	rBV5	14719	34086	5.34%	0.723%
29	7.312	1012	1021	1030	rBV	133056	291983	45.77%	6.197%
30	7.476	1044	1048	1049	rBV4	443	531	0.08%	0.011%
31	7.580	1062	1065	1067	rVB	168	185	0.03%	0.004%
32	7.799	1097	1101	1102	rBV2	444	419	0.07%	0.009%
33	7.848	1107	1109	1114	rVB2	244	419	0.07%	0.009%
34	7.885	1114	1115	1120	rBV2	145	245	0.04%	0.005%
35	7.927	1120	1122	1123	rBV2	335	284	0.04%	0.006%
36	8.037	1138	1140	1143	rVB	259	195	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025948.D
 Acq On : 21 Dec 2021 11:52
 Operator : JC/MD
 Sample : M5126-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

37	8.129	1152	1155	1158	rBV2	216	291	0.05%	0.006%
38	8.324	1181	1187	1198	rBV	81524	134668	21.11%	2.858%
39	8.476	1208	1212	1213	rBV2	297	349	0.05%	0.007%
40	8.653	1234	1241	1248	rBV	313868	504010	79.01%	10.696%
41	8.952	1284	1290	1299	rBV	56718	80818	12.67%	1.715%
42	9.183	1325	1328	1329	rVB	320	203	0.03%	0.004%
43	9.275	1338	1343	1350	rBV2	16051	23537	3.69%	0.500%
44	9.385	1355	1361	1377	rBV	207056	306719	48.08%	6.509%
45	9.763	1420	1423	1425	rBV2	231	253	0.04%	0.005%
46	9.878	1436	1442	1444	rVB2	219	393	0.06%	0.008%
47	10.055	1465	1471	1485	rBV	329468	439357	68.87%	9.324%
48	10.195	1492	1494	1498	rVB2	311	378	0.06%	0.008%
49	10.244	1498	1502	1506	rVB3	616	996	0.16%	0.021%
50	10.299	1508	1511	1515	rBV3	719	865	0.14%	0.018%
51	10.427	1529	1532	1535	rBV	198	248	0.04%	0.005%
52	10.458	1535	1537	1538	rVV	250	184	0.03%	0.004%
53	10.647	1565	1568	1572	rBV2	325	391	0.06%	0.008%
54	11.122	1642	1646	1650	rVB2	1484	1680	0.26%	0.036%
55	11.195	1652	1658	1666	rBV	232895	307005	48.13%	6.515%
56	11.311	1675	1677	1682	rVB3	627	804	0.13%	0.017%
57	11.378	1686	1688	1690	rVV2	262	248	0.04%	0.005%
58	11.433	1693	1697	1698	rVV2	235	248	0.04%	0.005%
59	11.451	1698	1700	1701	rVV	262	213	0.03%	0.005%
60	11.482	1701	1705	1711	rVB4	703	1223	0.19%	0.026%
61	11.616	1724	1727	1729	rBV2	263	261	0.04%	0.006%
62	11.750	1745	1749	1757	rVV4	1330	1993	0.31%	0.042%
63	11.933	1776	1779	1782	rVV3	805	870	0.14%	0.018%
64	11.963	1782	1784	1786	rVV2	236	247	0.04%	0.005%
65	11.982	1786	1787	1789	rVV2	409	266	0.04%	0.006%
66	12.024	1789	1794	1804	rVV	310565	379560	59.50%	8.055%
67	12.128	1807	1811	1812	rVV2	790	795	0.12%	0.017%
68	12.152	1812	1815	1818	rVV	1304	1356	0.21%	0.029%
69	12.219	1822	1826	1835	rVV2	4417	7624	1.20%	0.162%
70	12.323	1837	1843	1854	rVV	321218	410738	64.39%	8.717%
71	12.427	1857	1860	1863	rVV4	451	514	0.08%	0.011%
72	12.482	1867	1869	1872	rVB3	410	413	0.06%	0.009%
73	12.585	1883	1886	1887	rBV2	180	199	0.03%	0.004%
74	12.610	1888	1890	1892	rVV2	277	208	0.03%	0.004%
75	12.939	1942	1944	1947	rVB	369	294	0.05%	0.006%
76	12.969	1947	1949	1951	rBV2	241	216	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025948.D
 Acq On : 21 Dec 2021 11:52
 Operator : JC/MD
 Sample : M5126-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

77	13.049	1959	1962	1963	rBV2	301	223	0.03%	0.005%
78	13.067	1963	1965	1968	rVV	292	319	0.05%	0.007%
79	13.122	1972	1974	1978	rBV2	181	247	0.04%	0.005%
80	13.335	2006	2009	2010	rBV2	221	241	0.04%	0.005%
81	13.567	2044	2047	2048	rBV	236	201	0.03%	0.004%
82	13.628	2054	2057	2059	rBV2	230	275	0.04%	0.006%
83	13.780	2080	2082	2087	rBV2	218	379	0.06%	0.008%
84	13.872	2094	2097	2098	rBV2	276	221	0.03%	0.005%
85	13.926	2104	2106	2109	rBV2	261	348	0.05%	0.007%
86	13.957	2109	2111	2113	rVV	344	270	0.04%	0.006%
87	14.006	2115	2119	2121	rVV2	160	225	0.04%	0.005%
88	14.231	2152	2156	2159	rVB2	219	240	0.04%	0.005%
89	14.292	2165	2166	2168	rBV2	194	185	0.03%	0.004%
90	14.682	2227	2230	2232	rBV2	353	344	0.05%	0.007%
91	14.896	2264	2265	2268	rVB	332	209	0.03%	0.004%
92	14.999	2280	2282	2283	rBV	277	179	0.03%	0.004%
93	15.188	2311	2313	2314	rBV2	267	210	0.03%	0.004%
94	15.432	2352	2353	2356	rBV3	297	393	0.06%	0.008%
95	15.609	2380	2382	2383	rBV	316	212	0.03%	0.004%
96	15.725	2399	2401	2404	rVB2	270	252	0.04%	0.005%
97	16.036	2450	2452	2453	rBV2	235	192	0.03%	0.004%
98	16.200	2476	2479	2482	rBV	274	412	0.06%	0.009%
99	16.328	2499	2500	2504	rVB2	380	304	0.05%	0.006%
100	16.487	2523	2526	2527	rBV2	278	253	0.04%	0.005%


Sum of corrected areas: 4712041

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025948.D
Acq On : 21 Dec 2021 11:52
Operator : JC/MD
Sample : M5126-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

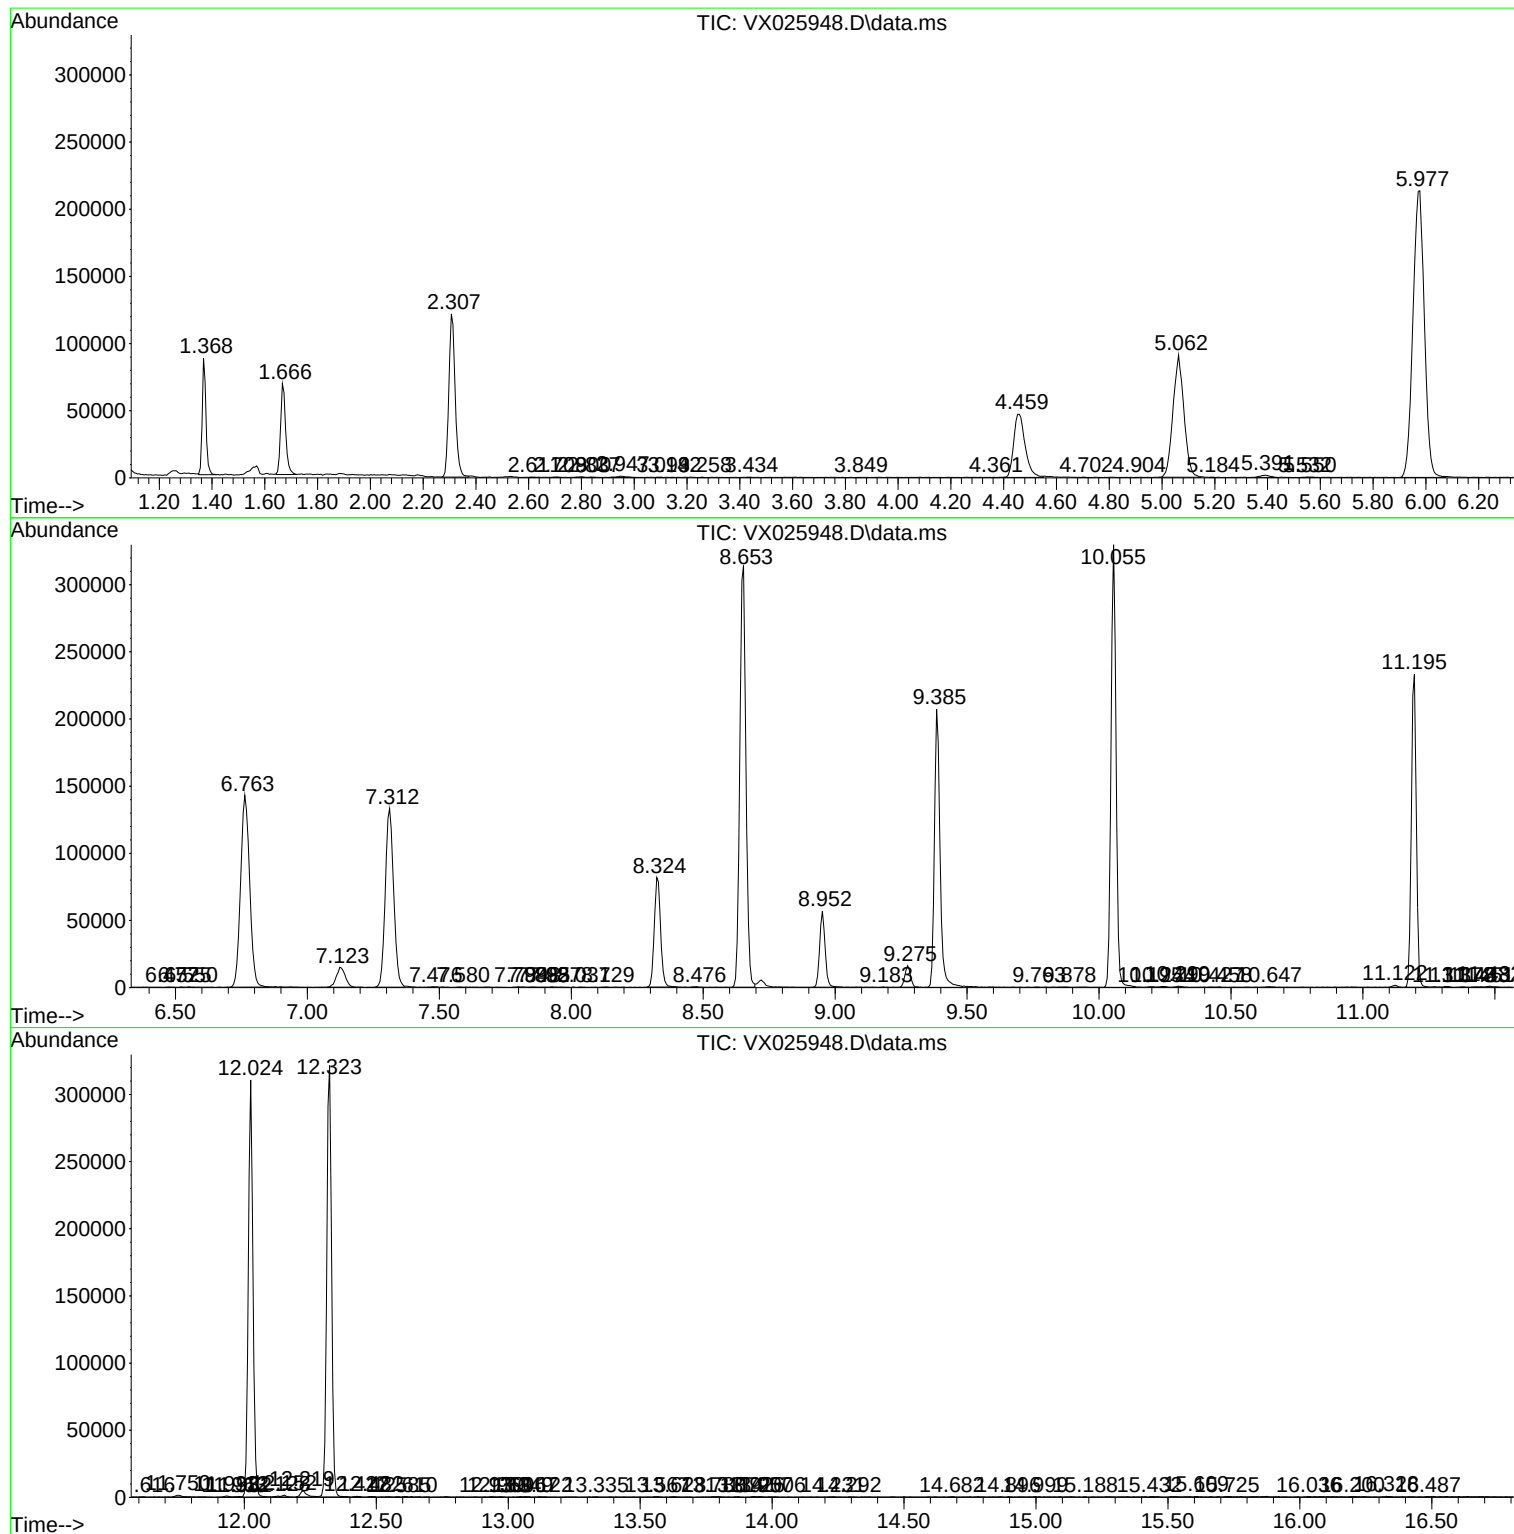

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025948.D
Acq On : 21 Dec 2021 11:52
Operator : JC/MD
Sample : M5126-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025948.D
Acq On : 21 Dec 2021 11:52
Operator : JC/MD
Sample : M5126-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc