

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025954.D
 Acq On : 21 Dec 2021 14:12
 Operator : JC/MD
 Sample : M5194-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGLC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025954.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	33	rBV2	5273	11199	2.00%	0.240%
2	1.367	43	46	57	rVB	72620	73592	13.11%	1.575%
3	1.666	91	95	105	rVB	60547	76361	13.60%	1.634%
4	2.306	194	200	209	rBV	102499	168410	30.00%	3.605%
5	2.380	209	212	222	rVB	3370	5493	0.98%	0.118%
6	2.477	225	228	229	rVB	333	285	0.05%	0.006%
7	2.495	229	231	232	rBV	298	259	0.05%	0.006%
8	2.538	233	238	250	rVB	3356	7224	1.29%	0.155%
9	2.642	250	255	259	rBV4	488	875	0.16%	0.019%
10	2.794	275	280	283	rBV3	452	621	0.11%	0.013%
11	2.953	298	306	309	rBV2	1003	2220	0.40%	0.048%
12	3.440	384	386	389	rVB2	298	244	0.04%	0.005%
13	3.471	389	391	394	rVV	280	230	0.04%	0.005%
14	3.605	410	413	416	rVB2	167	202	0.04%	0.004%
15	3.739	431	435	437	rBV3	257	402	0.07%	0.009%
16	4.068	486	489	492	rVB2	177	221	0.04%	0.005%
17	4.288	524	525	528	rBV2	163	187	0.03%	0.004%
18	4.458	542	553	568	rBV	44953	126990	22.62%	2.718%
19	4.721	589	596	608	rVB2	5108	14951	2.66%	0.320%
20	4.946	631	633	635	rBV2	252	220	0.04%	0.005%
21	5.062	640	652	669	rBV	79635	236623	42.16%	5.065%
22	5.562	731	734	738	rVB2	419	487	0.09%	0.010%
23	5.702	755	757	761	rVV	214	286	0.05%	0.006%
24	5.976	789	802	815	rBV2	185308	561298	100.00%	12.014%
25	6.092	820	821	824	rVB2	383	268	0.05%	0.006%
26	6.184	833	836	839	rBV2	197	282	0.05%	0.006%
27	6.251	845	847	850	rBV	156	236	0.04%	0.005%
28	6.543	893	895	900	rVB3	333	333	0.06%	0.007%
29	6.592	900	903	905	rBV2	303	302	0.05%	0.006%
30	6.659	911	914	915	rBV	166	193	0.03%	0.004%
31	6.763	922	931	949	rBV	179468	433203	77.18%	9.272%
32	7.043	975	977	979	rBV2	207	239	0.04%	0.005%
33	7.116	983	989	999	rVV6	5196	11808	2.10%	0.253%
34	7.312	1011	1021	1033	rBV	135648	306831	54.66%	6.567%
35	7.488	1046	1050	1051	rVV	371	384	0.07%	0.008%
36	7.580	1062	1065	1068	rVB	282	352	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025954.D
 Acq On : 21 Dec 2021 14:12
 Operator : JC/MD
 Sample : M5194-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGLC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

37	7.946	1120	1125	1126	rBV3	311	475	0.08%	0.010%
38	8.330	1181	1188	1203	rBV	79877	141280	25.17%	3.024%
39	8.567	1226	1227	1231	rVB2	390	485	0.09%	0.010%
40	8.647	1234	1240	1249	rBV	321036	534381	95.20%	11.438%
41	8.951	1284	1290	1299	rBV	60286	89268	15.90%	1.911%
42	9.275	1339	1343	1348	rBV4	1460	2307	0.41%	0.049%
43	9.348	1353	1355	1356	rBV	362	287	0.05%	0.006%
44	9.384	1356	1361	1380	rVV	233859	344577	61.39%	7.375%
45	9.525	1380	1384	1389	rVB3	3254	4882	0.87%	0.104%
46	9.689	1409	1411	1414	rBV2	139	188	0.03%	0.004%
47	9.774	1423	1425	1428	rBV2	159	202	0.04%	0.004%
48	10.055	1465	1471	1485	rVB	337101	443989	79.10%	9.503%
49	10.354	1517	1520	1521	rBV	192	233	0.04%	0.005%
50	10.488	1539	1542	1543	rBV2	212	241	0.04%	0.005%
51	10.604	1558	1561	1563	rBV2	232	271	0.05%	0.006%
52	10.646	1566	1568	1571	rVV2	303	377	0.07%	0.008%
53	10.695	1574	1576	1581	rVB2	271	389	0.07%	0.008%
54	10.780	1586	1590	1591	rVV2	212	230	0.04%	0.005%
55	10.927	1612	1614	1616	rVV	256	214	0.04%	0.005%
56	11.006	1621	1627	1628	rBV2	164	262	0.05%	0.006%
57	11.085	1635	1640	1643	rBV3	1185	1607	0.29%	0.034%
58	11.122	1643	1646	1652	rVB	1667	1898	0.34%	0.041%
59	11.195	1652	1658	1664	rBV	214431	281241	50.11%	6.020%
60	11.311	1673	1677	1680	rBV3	574	812	0.14%	0.017%
61	11.384	1687	1689	1691	rBV2	248	195	0.03%	0.004%
62	11.427	1693	1696	1698	rBV2	242	225	0.04%	0.005%
63	11.457	1698	1701	1702	rBV2	284	221	0.04%	0.005%
64	11.475	1702	1704	1707	rBV2	588	585	0.10%	0.013%
65	11.555	1715	1717	1719	rBV2	167	206	0.04%	0.004%
66	11.750	1744	1749	1754	rVB3	1323	2096	0.37%	0.045%
67	11.841	1763	1764	1767	rVV	285	275	0.05%	0.006%
68	11.933	1776	1779	1782	rVV4	1062	1139	0.20%	0.024%
69	11.969	1784	1785	1788	rVV2	346	211	0.04%	0.005%
70	12.024	1789	1794	1805	rVV	319881	395673	70.49%	8.469%
71	12.128	1805	1811	1812	rVV2	817	1162	0.21%	0.025%
72	12.152	1812	1815	1818	rVB	1085	1363	0.24%	0.029%
73	12.225	1823	1827	1833	rVB	1090	1683	0.30%	0.036%
74	12.274	1833	1835	1836	rBV	210	204	0.04%	0.004%
75	12.323	1836	1843	1850	rBV	282284	364083	64.86%	7.793%
76	12.433	1858	1861	1864	rVB3	627	652	0.12%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025954.D
 Acq On : 21 Dec 2021 14:12
 Operator : JC/MD
 Sample : M5194-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGLC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

77	12.658	1897	1898	1901	rBV2	417	359	0.06%	0.008%
78	12.762	1913	1915	1918	rBV	355	373	0.07%	0.008%
79	12.859	1928	1931	1934	rVB3	911	1060	0.19%	0.023%
80	13.097	1968	1970	1976	rVV4	1099	1599	0.28%	0.034%
81	13.426	2021	2024	2027	rVV2	198	210	0.04%	0.004%
82	13.731	2073	2074	2077	rVV2	250	240	0.04%	0.005%
83	13.780	2080	2082	2085	rVB2	335	387	0.07%	0.008%
84	14.188	2147	2149	2152	rVB2	219	179	0.03%	0.004%
85	14.286	2161	2165	2166	rBV	162	199	0.04%	0.004%
86	14.426	2184	2188	2189	rBV2	188	236	0.04%	0.005%
87	14.536	2205	2206	2212	rBV2	198	326	0.06%	0.007%
88	14.761	2240	2243	2244	rBV2	234	216	0.04%	0.005%
89	15.005	2281	2283	2286	rBV2	256	290	0.05%	0.006%
90	15.152	2304	2307	2311	rBV2	194	370	0.07%	0.008%
91	15.310	2331	2333	2336	rVB2	299	198	0.04%	0.004%
92	15.402	2346	2348	2351	rBV2	177	198	0.04%	0.004%
93	15.444	2354	2355	2358	rVV	278	245	0.04%	0.005%
94	15.493	2361	2363	2366	rBV3	261	269	0.05%	0.006%
95	15.773	2407	2409	2411	rVB	362	335	0.06%	0.007%
96	15.840	2416	2420	2422	rVB2	282	386	0.07%	0.008%
97	15.993	2443	2445	2447	rBV	173	214	0.04%	0.005%
98	16.304	2495	2496	2500	rBV2	212	229	0.04%	0.005%
99	16.377	2505	2508	2509	rBV2	222	270	0.05%	0.006%
100	16.523	2529	2532	2536	rBV3	212	364	0.06%	0.008%




Sum of corrected areas: 4672132

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025954.D
Acq On : 21 Dec 2021 14:12
Operator : JC/MD
Sample : M5194-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGLC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

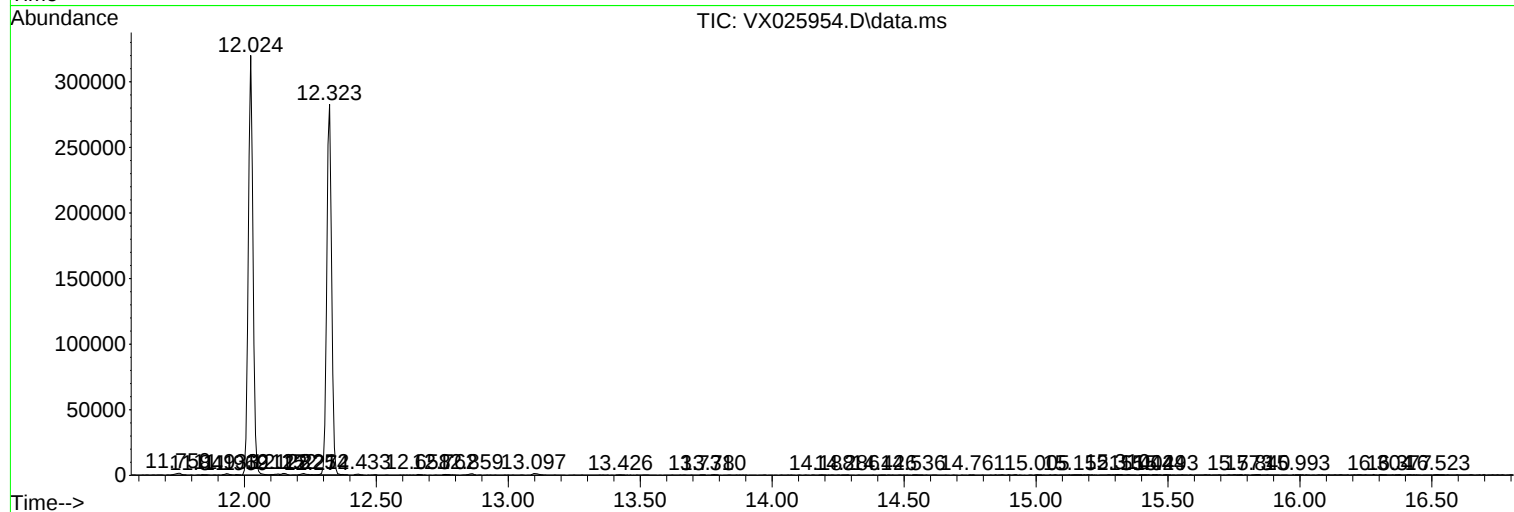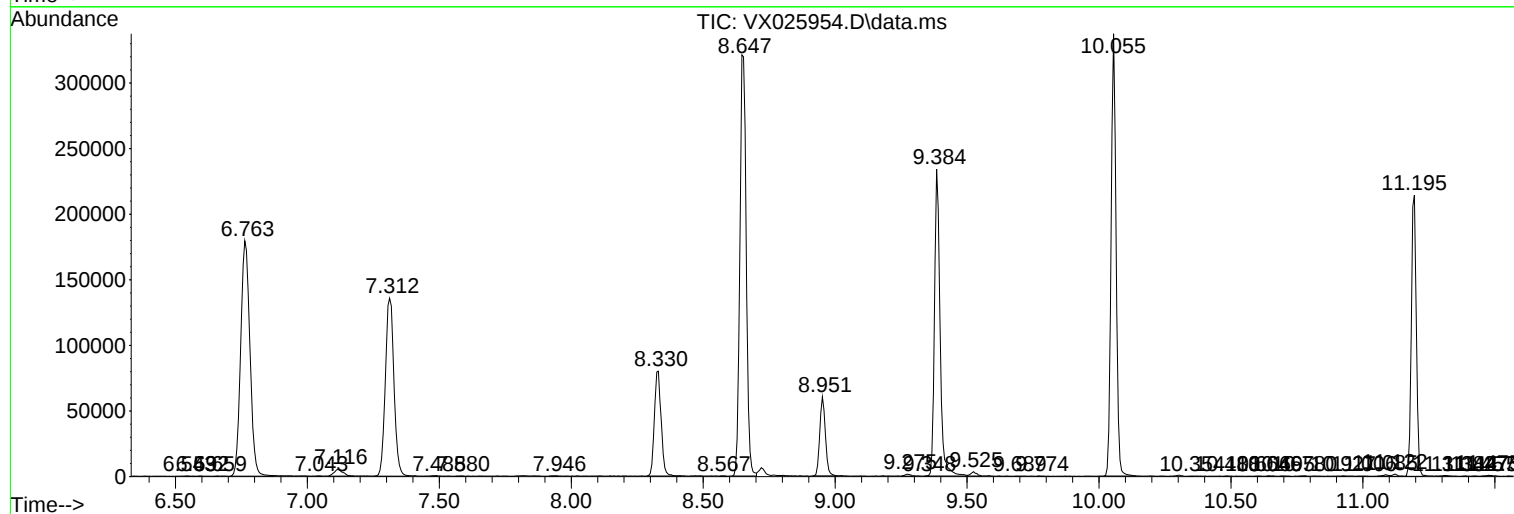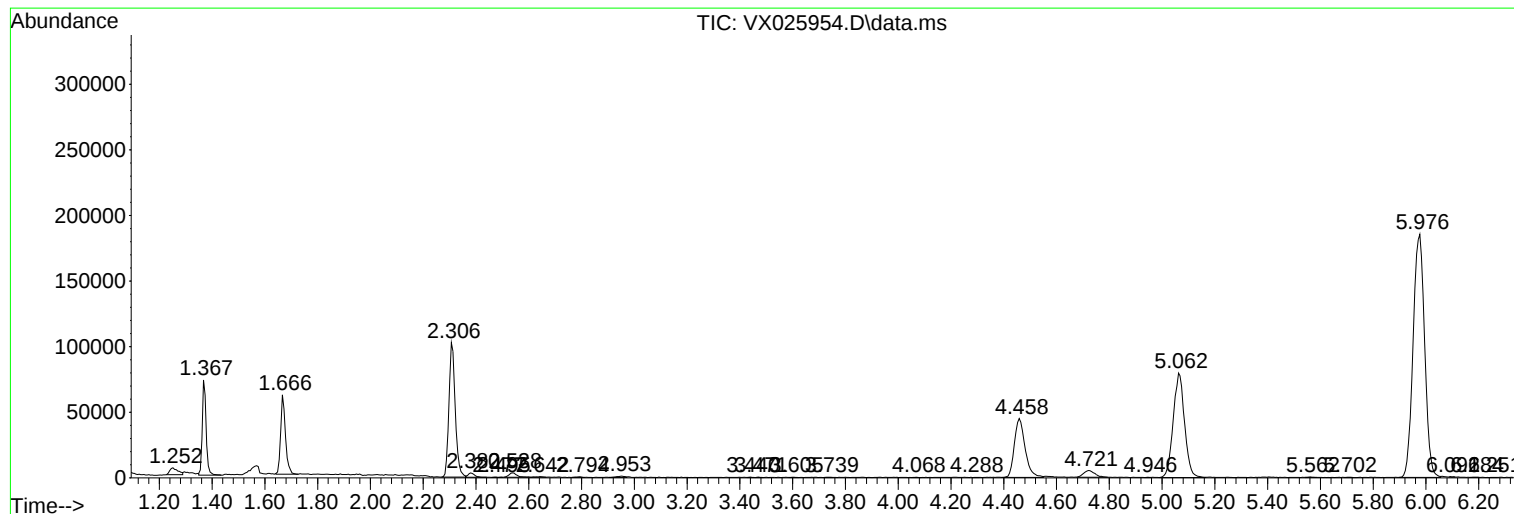

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025954.D
Acq On : 21 Dec 2021 14:12
Operator : JC/MD
Sample : M5194-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGLC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025954.D
Acq On : 21 Dec 2021 14:12
Operator : JC/MD
Sample : M5194-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGLC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc