

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025959.D
 Acq On : 21 Dec 2021 16:09
 Operator : JC/MD
 Sample : M5194-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGLC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M

Title : VOC Analysis

Signal : TIC: VX025959.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	32	rBV3	3519	5810	0.86%	0.111%
2	1.368	43	46	54	rVB	98408	98996	14.74%	1.898%
3	1.666	91	95	106	rVB	78417	98778	14.70%	1.894%
4	2.306	194	200	209	rBV	141301	227770	33.91%	4.367%
5	2.380	209	212	218	rVB	3132	5149	0.77%	0.099%
6	2.538	232	238	244	rBV	4025	7726	1.15%	0.148%
7	2.794	276	280	284	rVB3	351	481	0.07%	0.009%
8	2.892	294	296	298	rBV	252	216	0.03%	0.004%
9	2.953	300	306	312	rVV5	1148	2781	0.41%	0.053%
10	3.117	332	333	335	rBV	293	214	0.03%	0.004%
11	3.227	349	351	353	rVB	281	199	0.03%	0.004%
12	3.245	353	354	357	rBV	275	187	0.03%	0.004%
13	3.318	363	366	368	rBV2	241	264	0.04%	0.005%
14	3.440	381	386	387	rBV2	174	248	0.04%	0.005%
15	3.489	392	394	397	rVB	290	236	0.04%	0.005%
16	3.575	406	408	410	rVB2	306	253	0.04%	0.005%
17	4.361	535	537	539	rVB	331	200	0.03%	0.004%
18	4.385	539	541	543	rBV	241	261	0.04%	0.005%
19	4.458	544	553	568	rBV	43466	124804	18.58%	2.393%
20	4.660	584	586	588	rBV3	213	219	0.03%	0.004%
21	4.727	588	597	606	rVV3	5319	15399	2.29%	0.295%
22	5.056	640	651	668	rBV	85909	263059	39.16%	5.044%
23	5.208	674	676	679	rVB	315	303	0.05%	0.006%
24	5.245	679	682	683	rBV	267	258	0.04%	0.005%
25	5.373	698	703	704	rBV2	206	285	0.04%	0.005%
26	5.434	711	713	716	rVB2	216	212	0.03%	0.004%
27	5.544	728	731	732	rBV2	206	220	0.03%	0.004%
28	5.562	732	734	735	rBV	206	200	0.03%	0.004%
29	5.708	753	758	761	rBV2	198	311	0.05%	0.006%
30	5.824	775	777	780	rBV2	150	196	0.03%	0.004%
31	5.879	784	786	789	rBV2	224	281	0.04%	0.005%
32	5.970	789	801	820	rBV2	215081	650163	96.79%	12.466%
33	6.153	829	831	834	rBV2	248	296	0.04%	0.006%
34	6.233	842	844	848	rBV2	257	222	0.03%	0.004%
35	6.306	853	856	858	rBV	286	316	0.05%	0.006%
36	6.348	862	863	866	rBV2	334	320	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025959.D
 Acq On : 21 Dec 2021 16:09
 Operator : JC/MD
 Sample : M5194-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGLC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

37	6.550	892	896	899	rBV2	216	235	0.03%	0.005%
38	6.763	921	931	946	rBV	145151	343365	51.11%	6.584%
39	7.123	981	990	999	rVB7	4317	10900	1.62%	0.209%
40	7.208	999	1004	1006	rBV3	204	318	0.05%	0.006%
41	7.312	1012	1021	1033	rBV2	132718	290368	43.23%	5.568%
42	7.440	1041	1042	1045	rVB2	268	216	0.03%	0.004%
43	7.476	1045	1048	1049	rBV2	496	499	0.07%	0.010%
44	7.812	1099	1103	1105	rBV2	470	787	0.12%	0.015%
45	7.866	1110	1112	1115	rBV	216	202	0.03%	0.004%
46	8.324	1181	1187	1203	rBV	103539	173341	25.80%	3.324%
47	8.653	1233	1241	1248	rBV	412910	671755	100.00%	12.880%
48	8.720	1249	1252	1261	rVB2	7831	12938	1.93%	0.248%
49	8.952	1284	1290	1296	rBV	65990	96229	14.33%	1.845%
50	9.275	1339	1343	1352	rVB4	1408	2061	0.31%	0.040%
51	9.384	1356	1361	1381	rVV	276167	414088	61.64%	7.940%
52	9.525	1381	1384	1392	rVB4	2761	4772	0.71%	0.091%
53	9.836	1432	1435	1438	rVB2	220	276	0.04%	0.005%
54	10.055	1465	1471	1487	rBV	418119	560330	83.41%	10.744%
55	10.195	1491	1494	1495	rBV2	455	547	0.08%	0.010%
56	10.299	1509	1511	1517	rVB3	1255	1597	0.24%	0.031%
57	10.768	1583	1588	1593	rBV4	457	1129	0.17%	0.022%
58	10.915	1609	1612	1613	rBV2	228	227	0.03%	0.004%
59	10.988	1622	1624	1625	rVB	312	177	0.03%	0.003%
60	11.024	1628	1630	1634	rBV	431	382	0.06%	0.007%
61	11.122	1642	1646	1650	rVB2	4305	4995	0.74%	0.096%
62	11.189	1652	1657	1668	rBV	245998	313423	46.66%	6.010%
63	11.299	1674	1675	1676	rBV	461	295	0.04%	0.006%
64	11.384	1687	1689	1690	rVB2	258	176	0.03%	0.003%
65	11.433	1695	1697	1701	rVV2	195	220	0.03%	0.004%
66	11.482	1701	1705	1707	rVV4	876	1294	0.19%	0.025%
67	11.549	1714	1716	1719	rVB	350	311	0.05%	0.006%
68	11.640	1726	1731	1733	rBV2	262	389	0.06%	0.007%
69	11.689	1737	1739	1742	rVV2	473	425	0.06%	0.008%
70	11.750	1745	1749	1753	rVV4	2666	3549	0.53%	0.068%
71	11.799	1753	1757	1758	rVV	199	210	0.03%	0.004%
72	11.841	1762	1764	1768	rVB3	605	716	0.11%	0.014%
73	11.933	1775	1779	1784	rVB3	1377	1869	0.28%	0.036%
74	12.024	1789	1794	1800	rBV	296254	378463	56.34%	7.257%
75	12.128	1806	1811	1812	rBV2	1044	1462	0.22%	0.028%
76	12.152	1812	1815	1820	rVB2	2181	2901	0.43%	0.056%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025959.D
 Acq On : 21 Dec 2021 16:09
 Operator : JC/MD
 Sample : M5194-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGLC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

77	12.225	1823	1827	1832	rBV5	1407	2296	0.34%	0.044%
78	12.323	1835	1843	1850	rBV	315070	400423	59.61%	7.678%
79	12.427	1857	1860	1863	rVB2	847	994	0.15%	0.019%
80	12.475	1866	1868	1872	rVB4	613	674	0.10%	0.013%
81	12.585	1884	1886	1888	rBV	266	266	0.04%	0.005%
82	12.762	1911	1915	1918	rBV2	374	481	0.07%	0.009%
83	12.859	1928	1931	1933	rVB3	566	456	0.07%	0.009%
84	13.048	1960	1962	1967	rBV4	491	717	0.11%	0.014%
85	13.097	1968	1970	1975	rVB4	999	1180	0.18%	0.023%
86	13.195	1982	1986	1987	rBV	232	253	0.04%	0.005%
87	13.561	2044	2046	2047	rBV	331	183	0.03%	0.004%
88	13.780	2080	2082	2086	rVV2	300	364	0.05%	0.007%
89	14.030	2119	2123	2124	rBV2	268	348	0.05%	0.007%
90	14.213	2152	2153	2156	rVB2	381	182	0.03%	0.003%
91	14.384	2179	2181	2184	rVB	285	182	0.03%	0.003%
92	14.548	2206	2208	2210	rVB2	247	184	0.03%	0.004%
93	14.670	2227	2228	2231	rBV	225	221	0.03%	0.004%
94	15.585	2376	2378	2380	rBV	229	207	0.03%	0.004%
95	15.883	2424	2427	2430	rBB2	250	309	0.05%	0.006%
96	15.908	2430	2431	2434	rBV2	231	206	0.03%	0.004%
97	15.944	2434	2437	2440	rVV2	209	232	0.03%	0.004%
98	16.127	2465	2467	2469	rBV	321	322	0.05%	0.006%
99	16.353	2502	2504	2506	rBV	321	209	0.03%	0.004%
100	16.578	2539	2541	2543	rVB	287	219	0.03%	0.004%




Sum of corrected areas: 5215378

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025959.D
Acq On : 21 Dec 2021 16:09
Operator : JC/MD
Sample : M5194-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGLC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

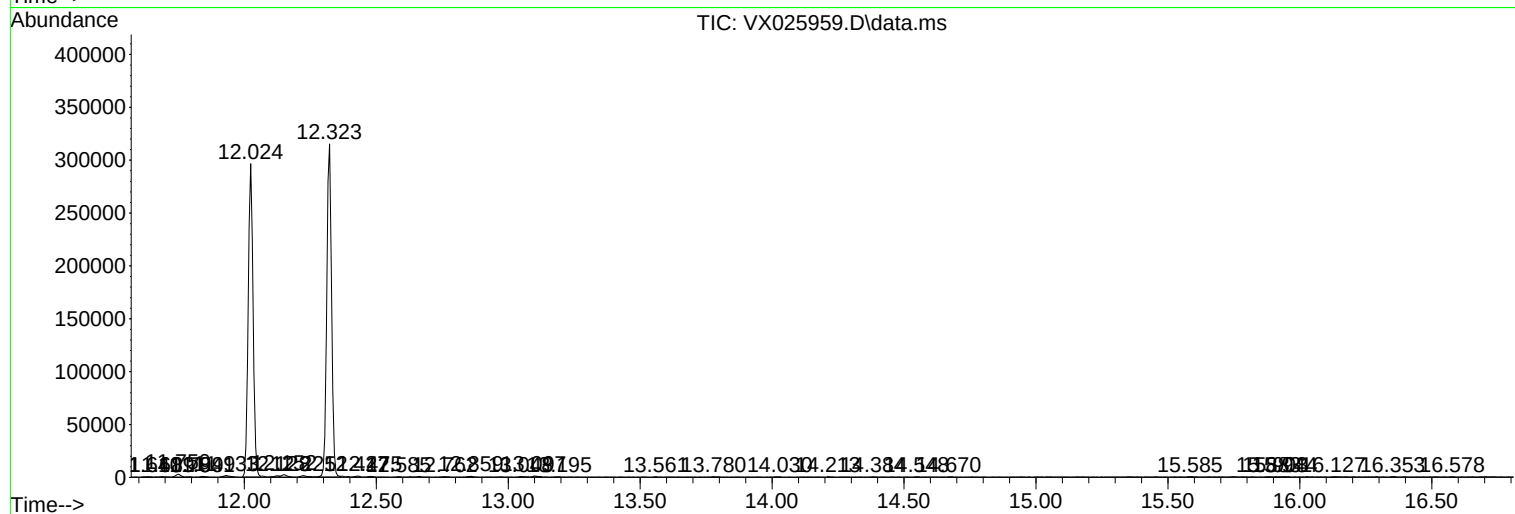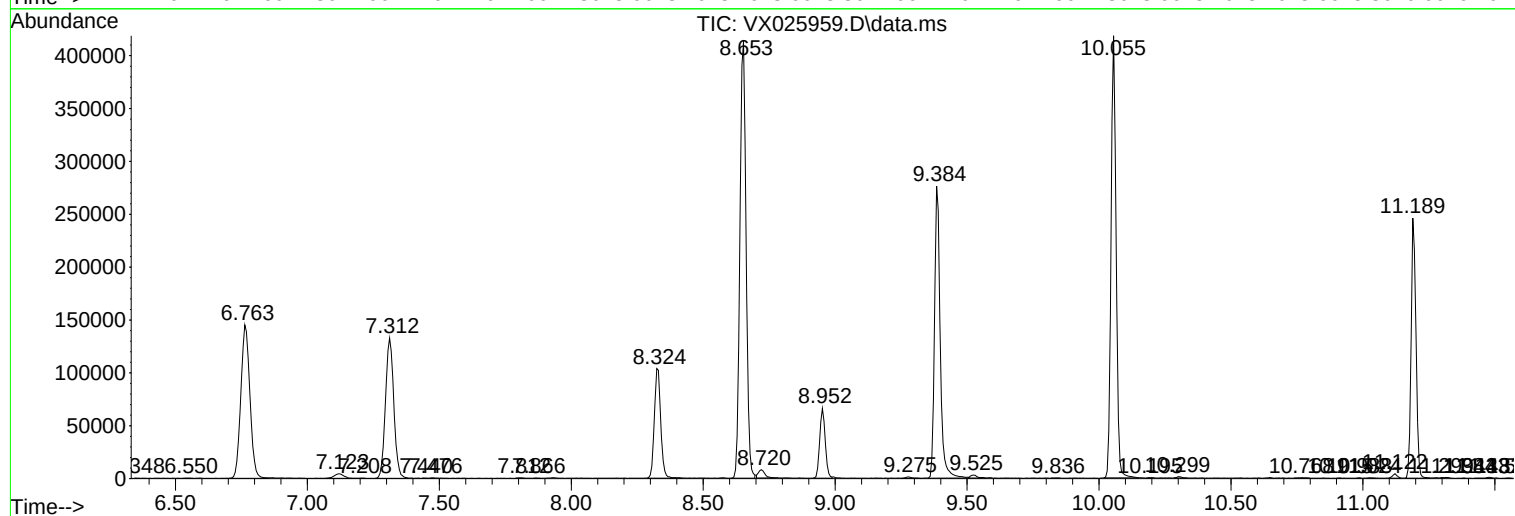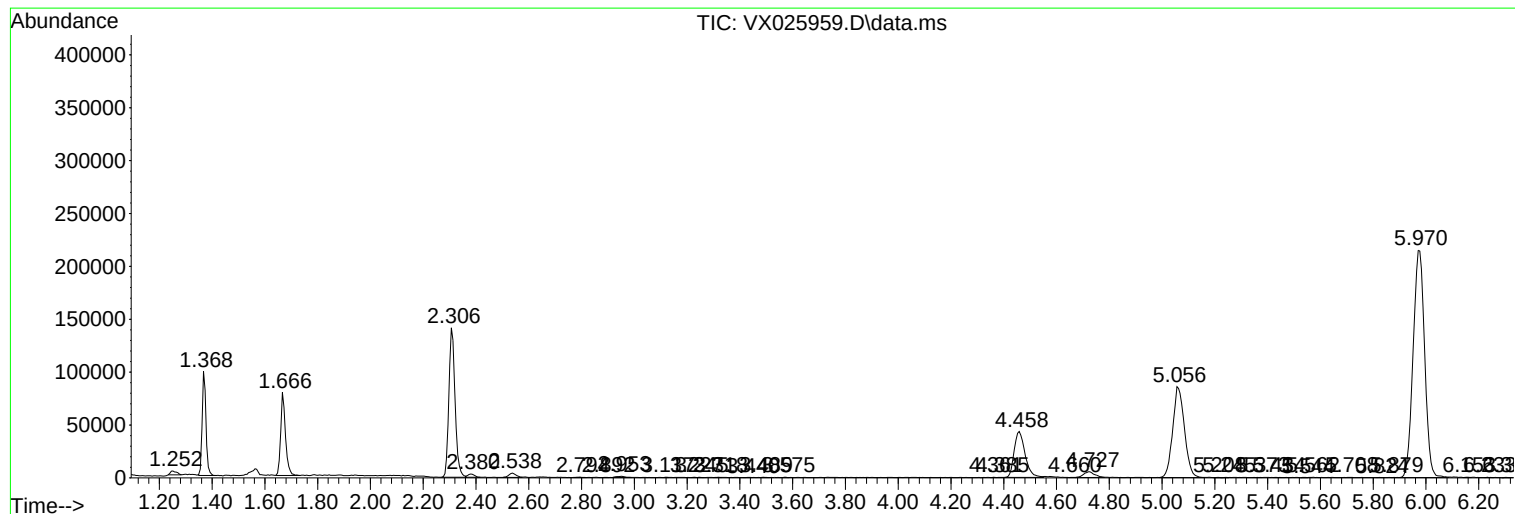

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025959.D
Acq On : 21 Dec 2021 16:09
Operator : JC/MD
Sample : M5194-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGLC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025959.D
Acq On : 21 Dec 2021 16:09
Operator : JC/MD
Sample : M5194-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGLC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------