

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025960.D
 Acq On : 21 Dec 2021 16:32
 Operator : JC/MD
 Sample : M5126-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025960.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	42	rBV2	4685	12583	1.92%	0.239%
2	1.368	43	46	55	rVB	83547	85328	13.03%	1.621%
3	1.666	91	95	108	rVB	68242	91315	13.94%	1.734%
4	2.252	190	191	194	rBV2	283	352	0.05%	0.007%
5	2.306	194	200	209	rVV	124786	203745	31.11%	3.870%
6	2.703	264	265	266	rBV	379	188	0.03%	0.004%
7	2.764	272	275	276	rBV2	198	219	0.03%	0.004%
8	2.788	276	279	282	rVB3	526	696	0.11%	0.013%
9	2.819	282	284	289	rBV2	201	301	0.05%	0.006%
10	2.898	293	297	298	rBV2	228	188	0.03%	0.004%
11	2.947	301	305	306	rBV	793	943	0.14%	0.018%
12	3.130	333	335	337	rVB	371	226	0.03%	0.004%
13	3.227	347	351	353	rBV2	188	248	0.04%	0.005%
14	3.325	363	367	368	rBV2	424	527	0.08%	0.010%
15	3.495	391	395	398	rBV2	199	289	0.04%	0.005%
16	4.026	481	482	486	rBV2	173	193	0.03%	0.004%
17	4.093	492	493	495	rBV2	203	191	0.03%	0.004%
18	4.209	510	512	513	rBV	504	366	0.06%	0.007%
19	4.459	541	553	569	rBV	51392	148386	22.66%	2.818%
20	4.690	589	591	592	rBV	292	215	0.03%	0.004%
21	4.837	614	615	619	rVB	318	214	0.03%	0.004%
22	4.922	625	629	630	rBV	224	198	0.03%	0.004%
23	5.062	640	652	670	rVB2	91449	267379	40.83%	5.078%
24	5.544	729	731	733	rBV2	383	392	0.06%	0.007%
25	5.653	745	749	751	rVB2	136	178	0.03%	0.003%
26	5.873	782	785	788	rBV2	186	181	0.03%	0.003%
27	5.977	788	802	815	rBV2	221177	654932	100.00%	12.439%
28	6.227	841	843	848	rBV3	221	280	0.04%	0.005%
29	6.281	850	852	858	rVB	214	241	0.04%	0.005%
30	6.361	861	865	867	rBV2	287	387	0.06%	0.007%
31	6.537	892	894	896	rBV2	239	199	0.03%	0.004%
32	6.763	922	931	945	rBV	189535	458804	70.05%	8.714%
33	7.007	969	971	974	rBV	249	230	0.04%	0.004%
34	7.056	978	979	982	rBV	296	250	0.04%	0.005%
35	7.110	982	988	996	rBV5	4880	11447	1.75%	0.217%
36	7.232	1006	1008	1011	rVB2	255	233	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025960.D
 Acq On : 21 Dec 2021 16:32
 Operator : JC/MD
 Sample : M5126-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

37	7.312	1011	1021	1034	rBV	167476	369159	56.37%	7.011%
38	7.476	1046	1048	1053	rBV4	314	530	0.08%	0.010%
39	7.860	1106	1111	1116	rVB2	2178	4191	0.64%	0.080%
40	7.927	1121	1122	1124	rVB2	361	216	0.03%	0.004%
41	8.330	1181	1188	1199	rBV	97016	158919	24.26%	3.018%
42	8.580	1227	1229	1231	rBV	487	327	0.05%	0.006%
43	8.653	1234	1241	1248	rBV	383181	638396	97.48%	12.125%
44	8.952	1284	1290	1302	rBV	65139	91838	14.02%	1.744%
45	9.037	1302	1304	1306	rVB2	340	244	0.04%	0.005%
46	9.141	1319	1321	1323	rBV	300	262	0.04%	0.005%
47	9.275	1340	1343	1345	rBV2	537	579	0.09%	0.011%
48	9.384	1356	1361	1380	rBV	269626	410962	62.75%	7.805%
49	9.677	1407	1409	1410	rVB	308	215	0.03%	0.004%
50	10.055	1465	1471	1487	rBV	372508	533505	81.46%	10.133%
51	10.195	1491	1494	1497	rVB3	354	495	0.08%	0.009%
52	10.244	1497	1502	1504	rBV3	799	1089	0.17%	0.021%
53	10.305	1509	1512	1517	rVV2	688	773	0.12%	0.015%
54	10.409	1527	1529	1532	rBB	211	184	0.03%	0.003%
55	10.470	1538	1539	1541	rBV	256	214	0.03%	0.004%
56	10.525	1545	1548	1551	rVV2	152	182	0.03%	0.003%
57	10.653	1566	1569	1570	rVB	388	286	0.04%	0.005%
58	11.031	1627	1631	1636	rVB2	794	1204	0.18%	0.023%
59	11.122	1642	1646	1649	rBV4	1478	1859	0.28%	0.035%
60	11.195	1652	1658	1668	rVV	242209	313092	47.81%	5.946%
61	11.476	1702	1704	1707	rVB	740	600	0.09%	0.011%
62	11.512	1709	1710	1713	rBV	150	177	0.03%	0.003%
63	11.640	1728	1731	1735	rVB	411	544	0.08%	0.010%
64	11.683	1735	1738	1741	rBV2	315	497	0.08%	0.009%
65	11.719	1741	1744	1746	rVV	259	352	0.05%	0.007%
66	11.750	1746	1749	1755	rVV4	1374	1954	0.30%	0.037%
67	11.811	1757	1759	1762	rVV2	180	181	0.03%	0.003%
68	11.847	1762	1765	1768	rVB2	330	364	0.06%	0.007%
69	11.939	1776	1780	1782	rVB2	921	925	0.14%	0.018%
70	12.024	1789	1794	1804	rVB	292648	369063	56.35%	7.009%
71	12.152	1812	1815	1818	rVB3	1011	1159	0.18%	0.022%
72	12.225	1823	1827	1832	rVV4	1895	2938	0.45%	0.056%
73	12.323	1836	1843	1849	rVV	318314	408050	62.30%	7.750%
74	12.396	1853	1855	1858	rVV	343	408	0.06%	0.008%
75	12.433	1858	1861	1864	rVV2	420	640	0.10%	0.012%
76	12.488	1868	1870	1873	rVV2	324	307	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025960.D
 Acq On : 21 Dec 2021 16:32
 Operator : JC/MD
 Sample : M5126-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

77	12.664	1897	1899	1901	rVB	287	223	0.03%	0.004%
78	12.731	1908	1910	1912	rBV	244	246	0.04%	0.005%
79	13.067	1961	1965	1967	rBV2	301	406	0.06%	0.008%
80	13.475	2029	2032	2033	rBV	256	255	0.04%	0.005%
81	13.792	2082	2084	2088	rBV	244	306	0.05%	0.006%
82	13.865	2093	2096	2099	rBV2	179	219	0.03%	0.004%
83	14.158	2142	2144	2146	rBV2	246	216	0.03%	0.004%
84	14.280	2162	2164	2167	rVB	222	195	0.03%	0.004%
85	14.304	2167	2168	2171	rBV2	299	252	0.04%	0.005%
86	14.432	2187	2189	2194	rBV2	172	268	0.04%	0.005%
87	14.481	2194	2197	2201	rVV2	207	296	0.05%	0.006%
88	14.512	2201	2202	2206	rVV2	234	210	0.03%	0.004%
89	14.542	2206	2207	2210	rVV2	226	225	0.03%	0.004%
90	14.713	2232	2235	2238	rBV	268	417	0.06%	0.008%
91	14.944	2272	2273	2276	rBV2	240	207	0.03%	0.004%
92	15.127	2301	2303	2306	rBV	283	276	0.04%	0.005%
93	15.304	2331	2332	2335	rBV2	296	239	0.04%	0.005%
94	15.518	2365	2367	2368	rBV	318	298	0.05%	0.006%
95	15.566	2373	2375	2379	rVV	313	368	0.06%	0.007%
96	15.780	2408	2410	2411	rBV	340	227	0.03%	0.004%
97	16.249	2483	2487	2488	rBV2	194	186	0.03%	0.004%
98	16.395	2509	2511	2513	rBV2	344	325	0.05%	0.006%
99	16.530	2528	2533	2534	rBV2	261	264	0.04%	0.005%
100	16.773	2571	2573	2575	rBV2	215	210	0.03%	0.004%




Sum of corrected areas: 5265258

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025960.D
Acq On : 21 Dec 2021 16:32
Operator : JC/MD
Sample : M5126-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

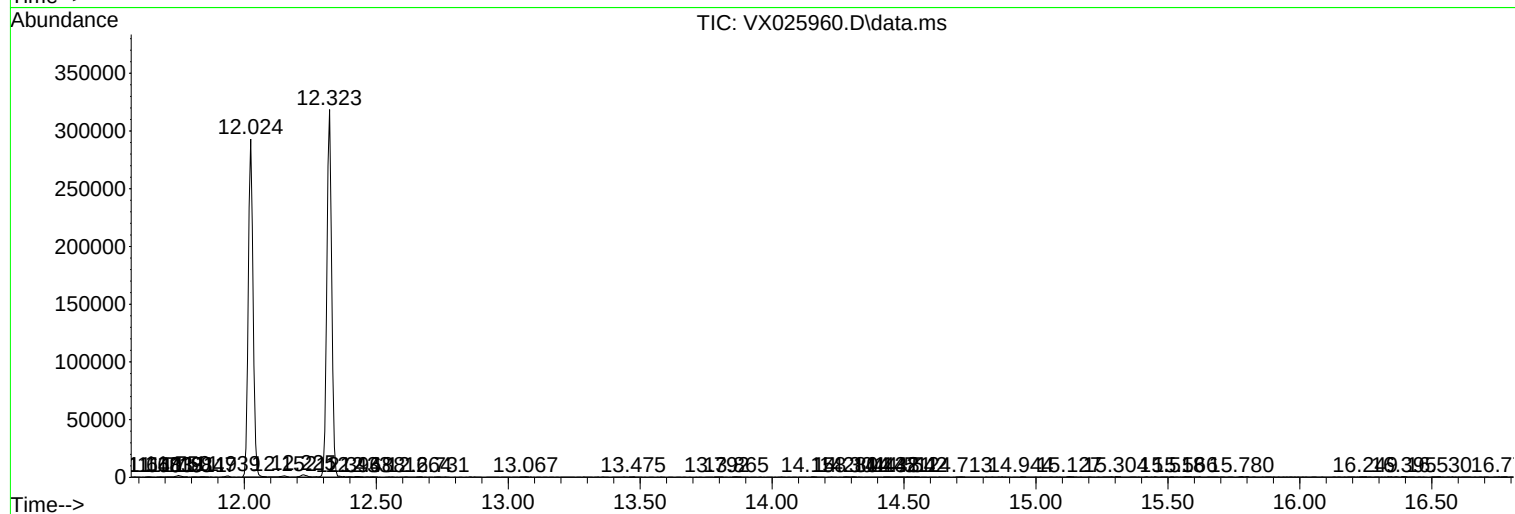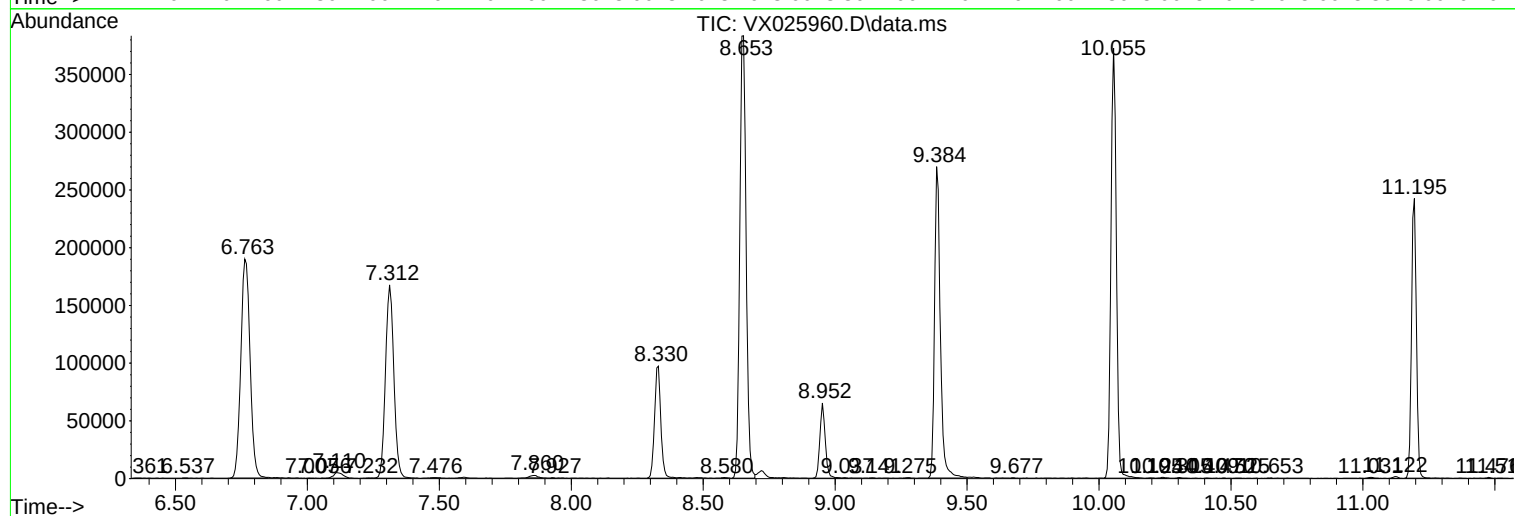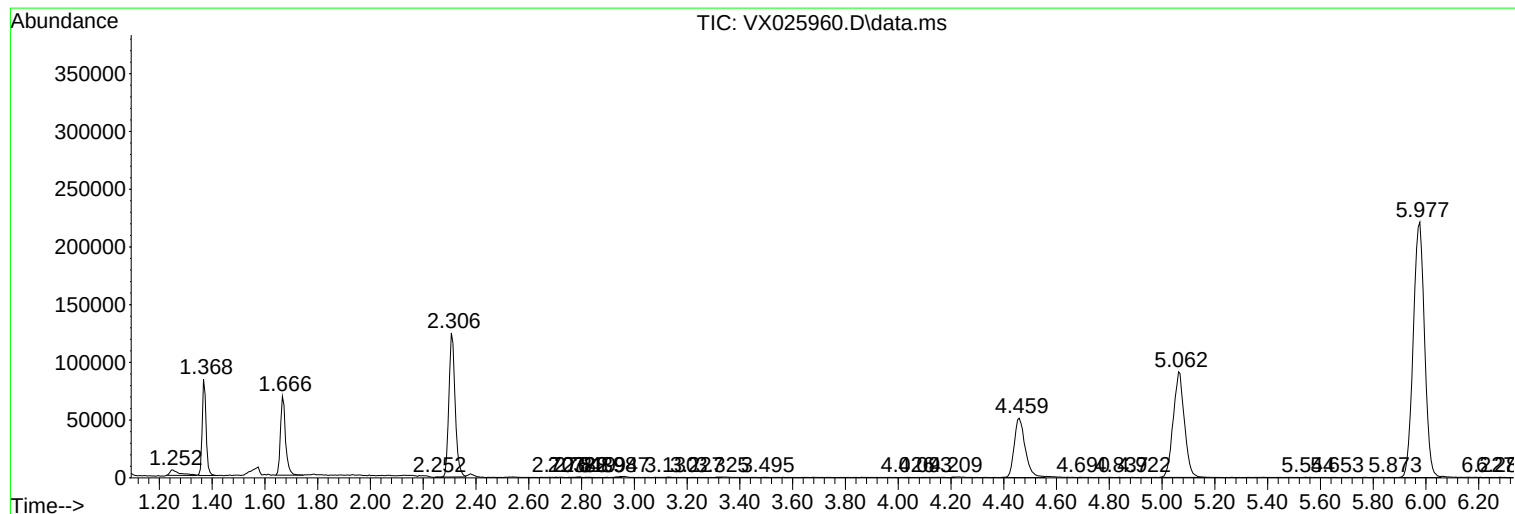

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025960.D
Acq On : 21 Dec 2021 16:32
Operator : JC/MD
Sample : M5126-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025960.D
Acq On : 21 Dec 2021 16:32
Operator : JC/MD
Sample : M5126-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------