

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025961.D
 Acq On : 21 Dec 2021 16:55
 Operator : JC/MD
 Sample : M5194-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025961.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	33	rBV2	4090	8532	1.46%	0.178%
2	1.368	43	46	55	rVB	67239	70806	12.11%	1.480%
3	1.666	91	95	104	rBV	60004	79383	13.58%	1.660%
4	2.306	194	200	210	rBV	104892	174940	29.93%	3.658%
5	2.428	218	220	223	rBV	225	221	0.04%	0.005%
6	2.544	237	239	243	rBV2	283	262	0.04%	0.005%
7	2.642	252	255	257	rBV	173	231	0.04%	0.005%
8	2.794	275	280	284	rBV3	1240	2216	0.38%	0.046%
9	3.117	328	333	334	rBV2	162	258	0.04%	0.005%
10	3.276	357	359	361	rVB	341	225	0.04%	0.005%
11	3.343	366	370	373	rVB2	199	280	0.05%	0.006%
12	3.379	373	376	378	rVB2	225	274	0.05%	0.006%
13	3.532	399	401	404	rVV	239	209	0.04%	0.004%
14	3.757	437	438	440	rBV	322	200	0.03%	0.004%
15	3.788	440	443	444	rVB2	204	185	0.03%	0.004%
16	3.898	459	461	465	rVB	211	226	0.04%	0.005%
17	4.141	500	501	504	rBV	219	177	0.03%	0.004%
18	4.178	504	507	508	rBV2	217	191	0.03%	0.004%
19	4.379	538	540	543	rBV2	227	173	0.03%	0.004%
20	4.458	544	553	571	rBV	48267	136805	23.40%	2.860%
21	4.708	592	594	597	rVB3	316	323	0.06%	0.007%
22	4.739	597	599	602	rBV2	194	320	0.05%	0.007%
23	5.062	639	652	672	rVB	83648	243260	41.62%	5.086%
24	5.318	693	694	698	rVB2	313	230	0.04%	0.005%
25	5.379	702	704	708	rBV3	277	475	0.08%	0.010%
26	5.458	716	717	719	rBV2	242	186	0.03%	0.004%
27	5.556	731	733	734	rBV	268	256	0.04%	0.005%
28	5.660	746	750	751	rBV2	156	200	0.03%	0.004%
29	5.830	775	778	781	rBV2	147	218	0.04%	0.005%
30	5.970	786	801	815	rBV2	195526	578951	99.05%	12.105%
31	6.409	869	873	876	rBV	175	262	0.04%	0.005%
32	6.489	883	886	889	rVB2	224	219	0.04%	0.005%
33	6.525	889	892	893	rBV2	196	177	0.03%	0.004%
34	6.763	921	931	943	rBV	128435	307334	52.58%	6.426%
35	6.940	958	960	964	rVB3	281	298	0.05%	0.006%
36	7.031	974	975	978	rBV	194	200	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025961.D
 Acq On : 21 Dec 2021 16:55
 Operator : JC/MD
 Sample : M5194-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

37	7.123	983	990	998	rVB5	3974	9755	1.67%	0.204%
38	7.312	1012	1021	1036	rBV	154128	337051	57.66%	7.047%
39	7.482	1046	1049	1053	rBV3	562	901	0.15%	0.019%
40	7.562	1059	1062	1064	rBV	228	316	0.05%	0.007%
41	7.799	1096	1101	1102	rBV2	403	509	0.09%	0.011%
42	7.897	1115	1117	1120	rBV	323	396	0.07%	0.008%
43	8.324	1181	1187	1200	rBV	106674	177595	30.38%	3.713%
44	8.653	1234	1241	1248	rBV	367010	584519	100.00%	12.222%
45	8.952	1284	1290	1301	rBV	57893	87193	14.92%	1.823%
46	9.238	1335	1337	1340	rBV2	213	204	0.03%	0.004%
47	9.275	1340	1343	1344	rBV2	275	291	0.05%	0.006%
48	9.384	1356	1361	1376	rBV	280933	414162	70.86%	8.660%
49	9.567	1390	1391	1394	rVB	412	208	0.04%	0.004%
50	9.634	1400	1402	1404	rBV2	172	170	0.03%	0.004%
51	9.775	1423	1425	1427	rVB2	345	317	0.05%	0.007%
52	10.055	1465	1471	1487	rBV	399138	539377	92.28%	11.278%
53	10.195	1492	1494	1497	rVB	379	252	0.04%	0.005%
54	10.250	1500	1503	1504	rBV2	314	288	0.05%	0.006%
55	10.305	1509	1512	1517	rVV2	615	850	0.15%	0.018%
56	10.628	1563	1565	1568	rVB2	177	181	0.03%	0.004%
57	10.945	1614	1617	1619	rBV	169	188	0.03%	0.004%
58	10.970	1619	1621	1626	rVB2	204	302	0.05%	0.006%
59	11.018	1626	1629	1632	rBV2	226	285	0.05%	0.006%
60	11.122	1642	1646	1652	rBV5	923	1302	0.22%	0.027%
61	11.195	1652	1658	1666	rBV	227512	289670	49.56%	6.057%
62	11.274	1669	1671	1673	rVV	277	219	0.04%	0.005%
63	11.378	1684	1688	1689	rVB2	152	174	0.03%	0.004%
64	11.390	1689	1690	1693	rBV	181	236	0.04%	0.005%
65	11.725	1741	1745	1746	rBV2	294	384	0.07%	0.008%
66	11.750	1746	1749	1753	rVV4	1013	1199	0.21%	0.025%
67	11.927	1774	1778	1783	rVB2	646	841	0.14%	0.018%
68	12.024	1789	1794	1805	rVV	272652	342000	58.51%	7.151%
69	12.152	1812	1815	1819	rVB3	896	1127	0.19%	0.024%
70	12.189	1819	1821	1823	rBV	240	219	0.04%	0.005%
71	12.323	1837	1843	1851	rVV	296527	374340	64.04%	7.827%
72	12.427	1858	1860	1863	rVB2	263	220	0.04%	0.005%
73	12.555	1877	1881	1882	rBV2	324	297	0.05%	0.006%
74	12.719	1906	1908	1909	rBV	281	207	0.04%	0.004%
75	12.762	1913	1915	1918	rVV2	253	259	0.04%	0.005%
76	12.841	1924	1928	1930	rBV	146	204	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025961.D
 Acq On : 21 Dec 2021 16:55
 Operator : JC/MD
 Sample : M5194-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

77	13.042	1959	1961	1966	rVB2	169	188	0.03%	0.004%
78	13.268	1995	1998	2001	rBV2	161	215	0.04%	0.004%
79	13.634	2057	2058	2062	rBV2	220	221	0.04%	0.005%
80	13.695	2067	2068	2070	rVB	378	185	0.03%	0.004%
81	13.896	2099	2101	2102	rBV	298	188	0.03%	0.004%
82	13.932	2105	2107	2109	rVB	326	206	0.04%	0.004%
83	14.030	2119	2123	2124	rBV2	200	276	0.05%	0.006%
84	14.073	2127	2130	2132	rBV	225	187	0.03%	0.004%
85	14.188	2148	2149	2152	rVB2	328	251	0.04%	0.005%
86	14.219	2152	2154	2157	rBV2	276	246	0.04%	0.005%
87	14.475	2191	2196	2197	rBV2	141	230	0.04%	0.005%
88	14.579	2211	2213	2215	rVB2	173	182	0.03%	0.004%
89	14.676	2227	2229	2232	rVB2	218	230	0.04%	0.005%
90	15.133	2302	2304	2305	rBV	248	266	0.05%	0.006%
91	15.243	2320	2322	2323	rBV	226	193	0.03%	0.004%
92	15.304	2330	2332	2336	rBV2	133	184	0.03%	0.004%
93	15.420	2349	2351	2355	rVV2	306	351	0.06%	0.007%
94	15.682	2391	2394	2396	rBV2	268	293	0.05%	0.006%
95	15.889	2426	2428	2431	rBV3	275	332	0.06%	0.007%
96	16.048	2452	2454	2457	rVB3	200	170	0.03%	0.004%
97	16.212	2479	2481	2484	rVB2	366	347	0.06%	0.007%
98	16.395	2508	2511	2512	rBV2	229	252	0.04%	0.005%
99	16.414	2512	2514	2516	rVV2	392	309	0.05%	0.006%
100	16.633	2549	2550	2552	rBV2	248	212	0.04%	0.004%




Sum of corrected areas: 4782625

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025961.D
Acq On : 21 Dec 2021 16:55
Operator : JC/MD
Sample : M5194-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

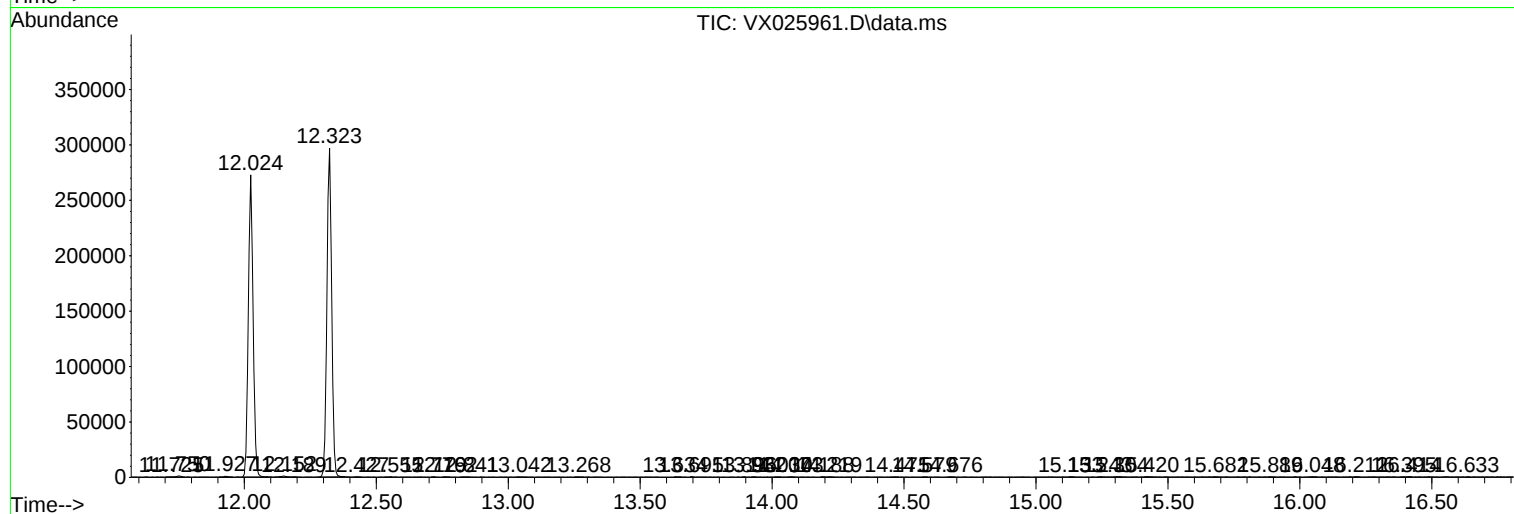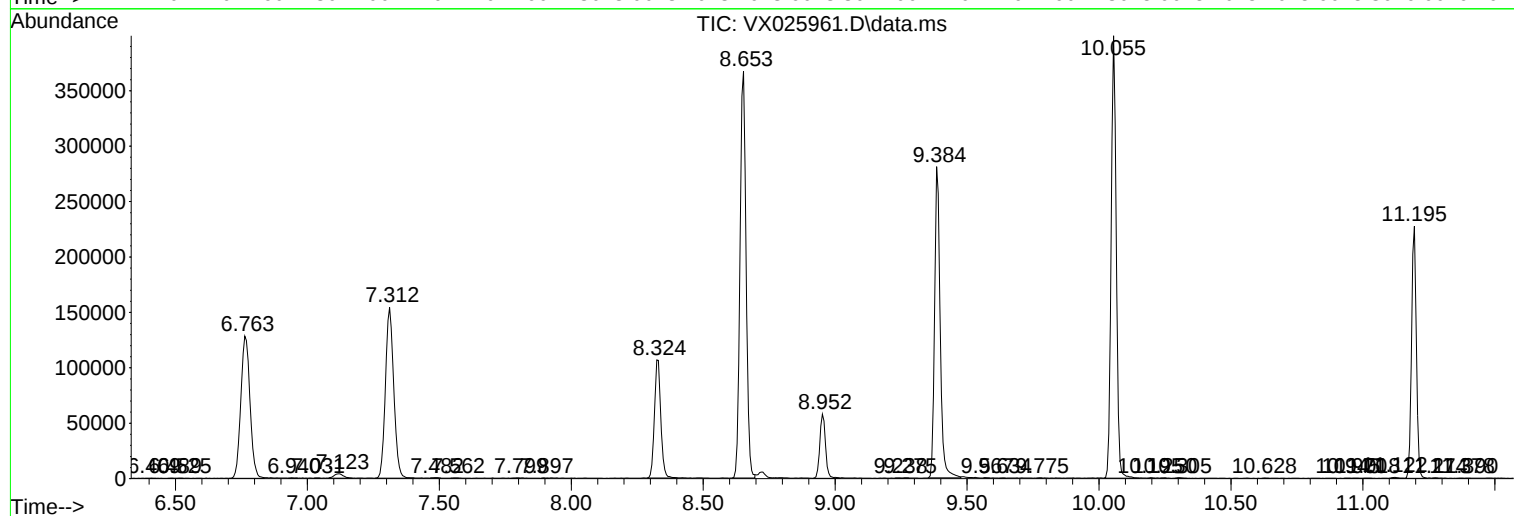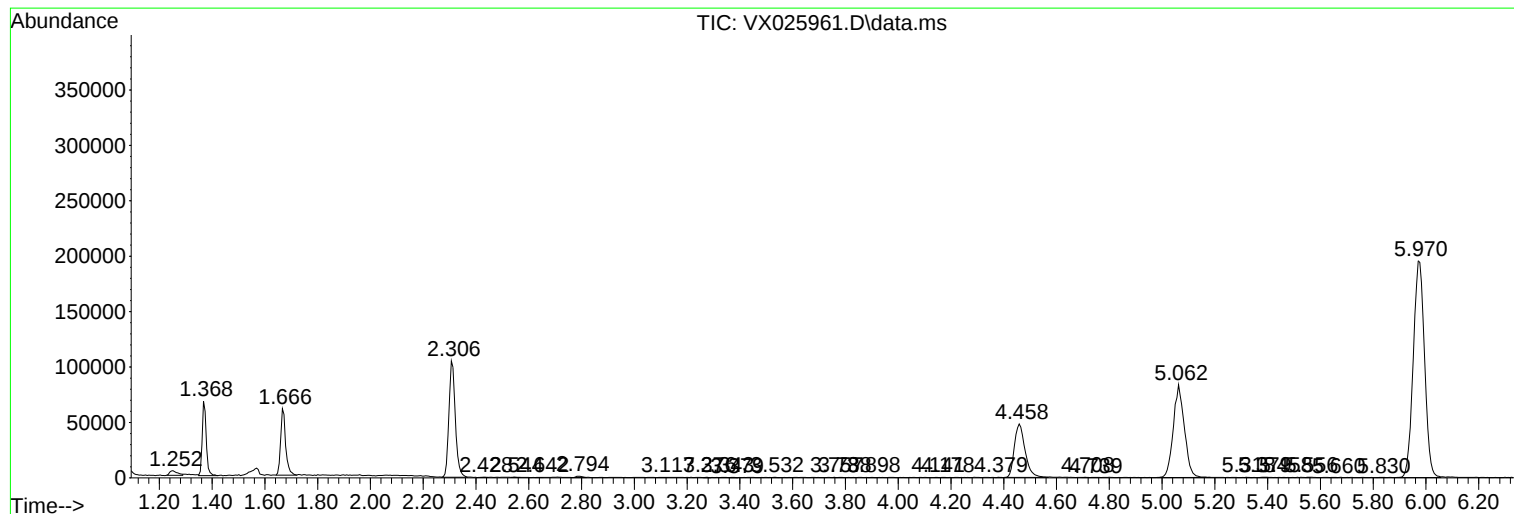

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025961.D
Acq On : 21 Dec 2021 16:55
Operator : JC/MD
Sample : M5194-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025961.D
Acq On : 21 Dec 2021 16:55
Operator : JC/MD
Sample : M5194-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc