

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025962.D
 Acq On : 21 Dec 2021 17:19
 Operator : JC/MD
 Sample : M5126-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025962.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	52	rVB	83855	82877	12.01%	1.655%
2	1.666	91	95	105	rVB	73116	94512	13.69%	1.888%
3	2.306	194	200	210	rBV	123004	199752	28.94%	3.990%
4	2.611	248	250	252	rVB2	272	211	0.03%	0.004%
5	2.660	256	258	260	rVB2	292	238	0.03%	0.005%
6	2.703	263	265	267	rVV2	228	183	0.03%	0.004%
7	2.751	270	273	274	rVV2	239	201	0.03%	0.004%
8	2.794	276	280	283	rVB3	359	488	0.07%	0.010%
9	2.861	288	291	292	rBV2	227	268	0.04%	0.005%
10	2.916	298	300	301	rBV	207	210	0.03%	0.004%
11	3.172	338	342	344	rBV2	201	279	0.04%	0.006%
12	3.386	375	377	379	rBV	213	164	0.02%	0.003%
13	3.446	385	387	389	rBV	280	169	0.02%	0.003%
14	3.690	423	427	428	rBV	276	249	0.04%	0.005%
15	3.892	456	460	461	rBV2	147	179	0.03%	0.004%
16	4.196	508	510	512	rVB2	240	187	0.03%	0.004%
17	4.355	533	536	538	rBV2	182	247	0.04%	0.005%
18	4.458	544	553	573	rBV	47115	138437	20.06%	2.765%
19	4.690	588	591	596	rBV2	318	502	0.07%	0.010%
20	4.745	598	600	601	rVV	288	171	0.02%	0.003%
21	4.788	605	607	610	rVV2	142	189	0.03%	0.004%
22	5.056	639	651	668	rBV	84773	266766	38.65%	5.328%
23	5.202	673	675	677	rVB2	276	220	0.03%	0.004%
24	5.233	677	680	684	rVB2	255	374	0.05%	0.007%
25	5.263	684	685	688	rBV	134	163	0.02%	0.003%
26	5.385	699	705	711	rBV2	1468	3645	0.53%	0.073%
27	5.458	716	717	719	rBV	380	241	0.03%	0.005%
28	5.544	729	731	732	rBV	374	225	0.03%	0.004%
29	5.611	739	742	743	rBV2	184	193	0.03%	0.004%
30	5.830	777	778	780	rBV2	175	180	0.03%	0.004%
31	5.970	789	801	820	rBV3	219834	648378	93.94%	12.950%
32	6.269	847	850	852	rVB	238	203	0.03%	0.004%
33	6.348	859	863	866	rBV2	309	283	0.04%	0.006%
34	6.525	889	892	893	rBV2	240	177	0.03%	0.004%
35	6.550	893	896	897	rVV2	240	213	0.03%	0.004%
36	6.568	897	899	902	rVV	217	187	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025962.D
 Acq On : 21 Dec 2021 17:19
 Operator : JC/MD
 Sample : M5126-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

37	6.641	909	911	913	rBV	294	251	0.04%	0.005%
38	6.763	922	931	942	rVV	125946	301819	43.73%	6.028%
39	7.013	970	972	975	rVB	374	271	0.04%	0.005%
40	7.129	982	991	1001	rVB4	16681	39935	5.79%	0.798%
41	7.208	1001	1004	1006	rBV2	331	279	0.04%	0.006%
42	7.312	1012	1021	1033	rBV	159989	357059	51.73%	7.132%
43	7.519	1052	1055	1056	rBV	360	327	0.05%	0.007%
44	8.098	1149	1150	1154	rBV2	180	258	0.04%	0.005%
45	8.330	1181	1188	1196	rVV	101729	170733	24.74%	3.410%
46	8.488	1212	1214	1218	rVB2	574	623	0.09%	0.012%
47	8.653	1234	1241	1248	rBV	433119	690213	100.00%	13.786%
48	8.952	1284	1290	1298	rBV	83530	118993	17.24%	2.377%
49	9.232	1333	1336	1337	rBV	255	219	0.03%	0.004%
50	9.275	1337	1343	1350	rVV	20867	31361	4.54%	0.626%
51	9.384	1356	1361	1381	rBV	284677	417988	60.56%	8.349%
52	9.738	1417	1419	1425	rVB2	180	337	0.05%	0.007%
53	9.829	1431	1434	1436	rBV2	237	293	0.04%	0.006%
54	9.884	1439	1443	1445	rBV2	210	191	0.03%	0.004%
55	10.055	1465	1471	1483	rBV	281195	383171	55.51%	7.653%
56	10.195	1491	1494	1497	rBV2	360	408	0.06%	0.008%
57	10.244	1499	1502	1506	rVV4	662	806	0.12%	0.016%
58	10.299	1509	1511	1518	rVV3	508	736	0.11%	0.015%
59	10.372	1521	1523	1525	rVV2	172	175	0.03%	0.003%
60	10.409	1527	1529	1532	rVV2	165	208	0.03%	0.004%
61	10.628	1562	1565	1566	rBV	242	188	0.03%	0.004%
62	10.939	1615	1616	1621	rVB2	136	165	0.02%	0.003%
63	11.122	1642	1646	1649	rVB3	1294	1685	0.24%	0.034%
64	11.195	1652	1658	1666	rVV	235326	299202	43.35%	5.976%
65	11.305	1673	1676	1677	rBV2	359	213	0.03%	0.004%
66	11.451	1698	1700	1702	rBV	273	168	0.02%	0.003%
67	11.482	1702	1705	1711	rVV3	711	952	0.14%	0.019%
68	11.591	1721	1723	1726	rBV	159	165	0.02%	0.003%
69	11.750	1745	1749	1753	rVB3	1234	1556	0.23%	0.031%
70	11.860	1765	1767	1770	rVB2	178	181	0.03%	0.004%
71	11.933	1777	1779	1783	rVB3	611	694	0.10%	0.014%
72	12.024	1789	1794	1803	rVB	261084	328442	47.59%	6.560%
73	12.091	1803	1805	1808	rBV2	244	281	0.04%	0.006%
74	12.225	1823	1827	1832	rBV4	2711	4155	0.60%	0.083%
75	12.323	1835	1843	1851	rBV	315033	403960	58.53%	8.069%
76	12.427	1857	1860	1864	rVB4	339	550	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025962.D
 Acq On : 21 Dec 2021 17:19
 Operator : JC/MD
 Sample : M5126-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

77	13.048	1960	1962	1965	rVB2	207	165	0.02%	0.003%
78	13.372	2011	2015	2018	rVB2	140	211	0.03%	0.004%
79	13.402	2018	2020	2023	rBV	148	217	0.03%	0.004%
80	13.963	2111	2112	2116	rBV	124	169	0.02%	0.003%
81	14.134	2137	2140	2141	rVB	230	173	0.03%	0.003%
82	14.243	2155	2158	2160	rBV	246	219	0.03%	0.004%
83	14.323	2169	2171	2174	rBV	236	229	0.03%	0.005%
84	14.365	2176	2178	2181	rVB	177	164	0.02%	0.003%
85	14.396	2181	2183	2188	rVB2	258	405	0.06%	0.008%
86	14.451	2188	2192	2194	rBV2	233	327	0.05%	0.007%
87	14.530	2202	2205	2206	rBV2	253	208	0.03%	0.004%
88	14.585	2211	2214	2217	rBV	272	258	0.04%	0.005%
89	14.627	2219	2221	2222	rBV	206	186	0.03%	0.004%
90	14.829	2251	2254	2259	rBV2	308	496	0.07%	0.010%
91	14.999	2280	2282	2284	rVV	288	245	0.04%	0.005%
92	15.060	2289	2292	2293	rBV2	195	222	0.03%	0.004%
93	15.420	2349	2351	2352	rVB	301	176	0.03%	0.004%
94	15.499	2362	2364	2369	rBV	362	433	0.06%	0.009%
95	15.542	2369	2371	2372	rVV	308	201	0.03%	0.004%
96	15.578	2375	2377	2381	rBV3	221	257	0.04%	0.005%
97	15.761	2405	2407	2412	rBV3	265	396	0.06%	0.008%
98	15.938	2435	2436	2440	rBV2	278	338	0.05%	0.007%
99	16.115	2463	2465	2468	rBV2	230	309	0.04%	0.006%
100	16.225	2481	2483	2485	rBV	367	224	0.03%	0.004%




Sum of corrected areas: 5006600

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025962.D
Acq On : 21 Dec 2021 17:19
Operator : JC/MD
Sample : M5126-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

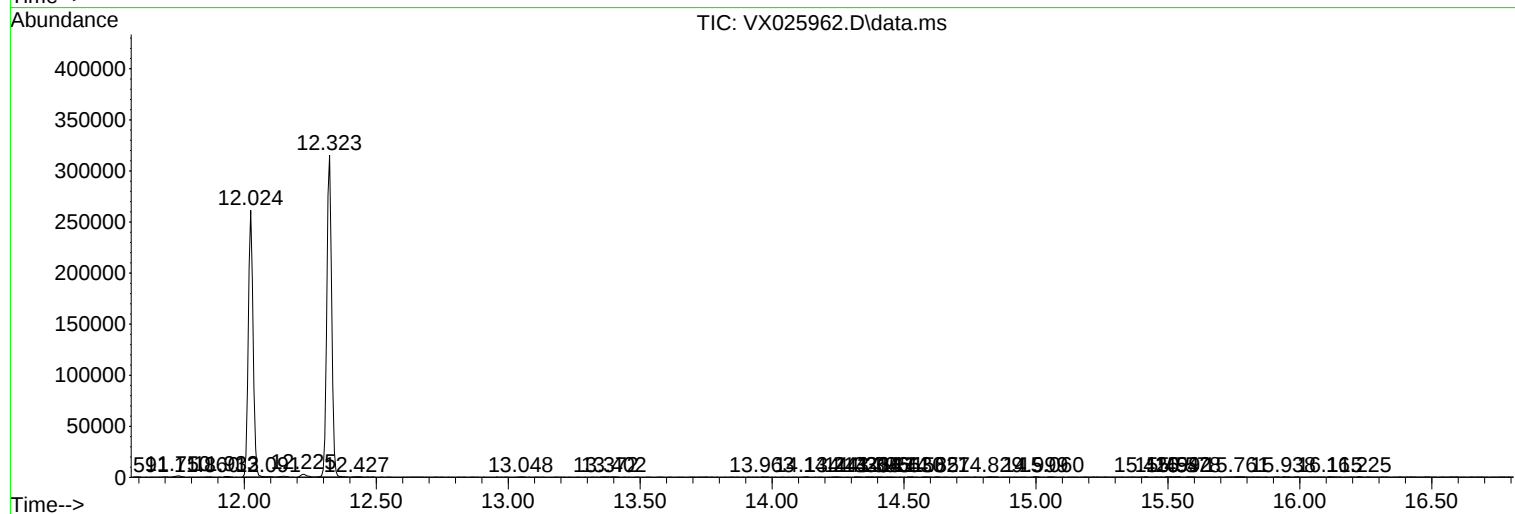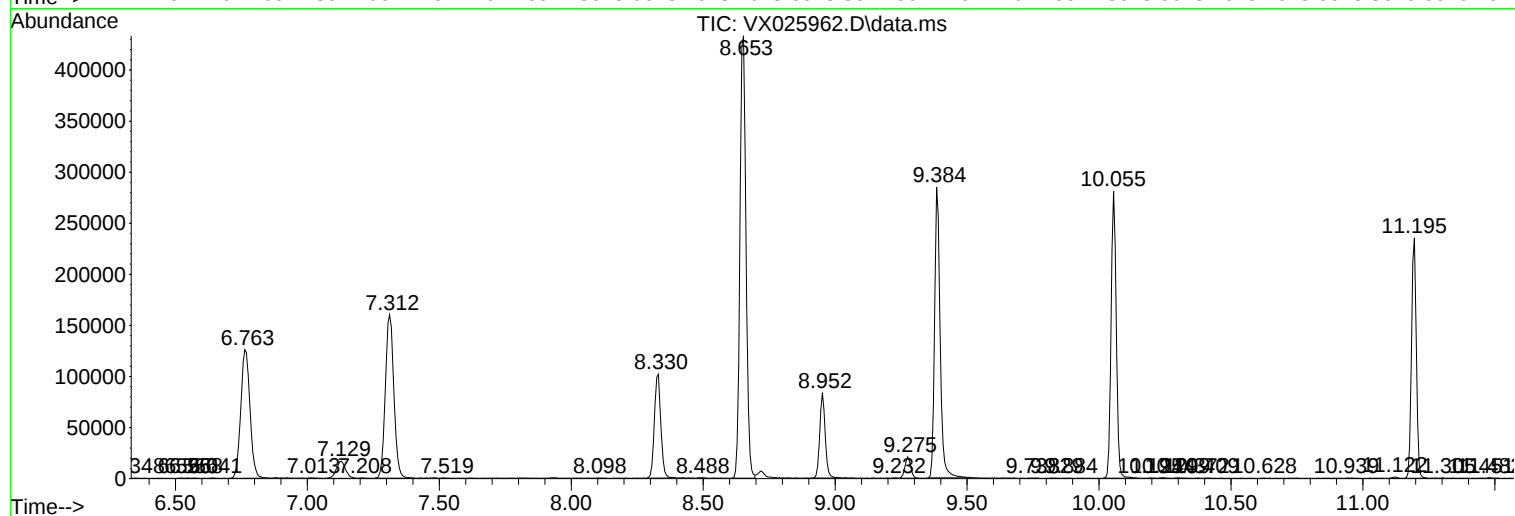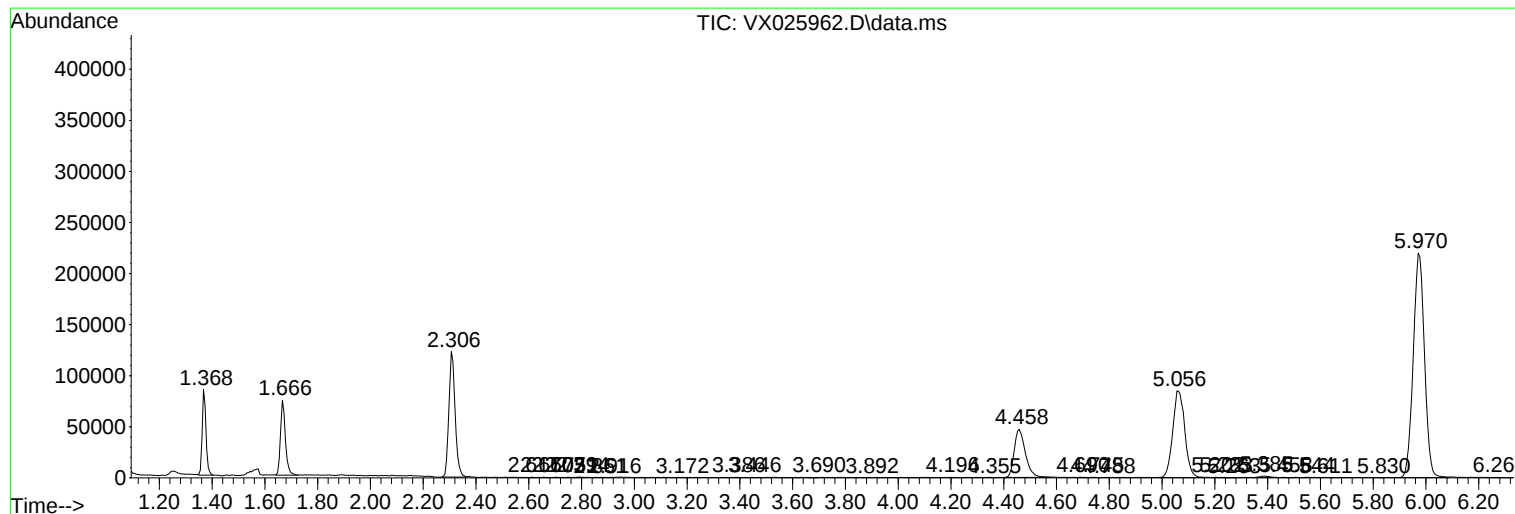

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025962.D
Acq On : 21 Dec 2021 17:19
Operator : JC/MD
Sample : M5126-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025962.D
Acq On : 21 Dec 2021 17:19
Operator : JC/MD
Sample : M5126-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc