

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025963.D
 Acq On : 21 Dec 2021 17:42
 Operator : JC/MD
 Sample : M5126-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025963.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	36	rVB2	4030	6934	1.04%	0.127%
2	1.368	43	46	55	rVB	83778	85046	12.79%	1.554%
3	1.666	91	95	105	rVB	73861	95582	14.37%	1.747%
4	1.892	128	132	139	rVB	5598	9263	1.39%	0.169%
5	2.306	194	200	211	rBV2	130158	224995	33.82%	4.112%
6	2.666	255	259	260	rBV2	197	261	0.04%	0.005%
7	2.794	277	280	285	rVB4	672	916	0.14%	0.017%
8	2.831	285	286	289	rBV	223	177	0.03%	0.003%
9	2.941	299	304	305	rBV2	849	1012	0.15%	0.018%
10	3.099	327	330	333	rBV3	326	440	0.07%	0.008%
11	3.251	352	355	356	rBV2	215	163	0.02%	0.003%
12	3.623	407	416	422	rVV2	1476	3259	0.49%	0.060%
13	3.721	431	432	437	rVB2	152	190	0.03%	0.003%
14	3.812	444	447	448	rBV	204	265	0.04%	0.005%
15	3.922	462	465	466	rBV2	189	217	0.03%	0.004%
16	3.977	469	474	476	rVB	233	334	0.05%	0.006%
17	4.459	544	553	574	rBV	50973	167726	25.21%	3.065%
18	4.934	630	631	634	rVB2	206	176	0.03%	0.003%
19	5.056	640	651	666	rVV	88410	269859	40.57%	4.932%
20	5.385	697	705	715	rVB3	3946	11224	1.69%	0.205%
21	5.556	730	733	738	rVB3	266	410	0.06%	0.007%
22	5.599	738	740	742	rBV	340	166	0.02%	0.003%
23	5.666	749	751	752	rBV	223	166	0.02%	0.003%
24	5.830	775	778	779	rBV	239	258	0.04%	0.005%
25	5.977	789	802	816	rVV2	216250	657317	98.82%	12.013%
26	6.092	819	821	825	rVB3	527	668	0.10%	0.012%
27	6.208	838	840	844	rVB2	285	294	0.04%	0.005%
28	6.294	852	854	860	rBV2	226	303	0.05%	0.006%
29	6.355	860	864	866	rVB2	208	255	0.04%	0.005%
30	6.464	877	882	885	rVB2	209	231	0.03%	0.004%
31	6.507	885	889	893	rBV2	125	178	0.03%	0.003%
32	6.544	893	895	898	rVB2	255	245	0.04%	0.004%
33	6.604	904	905	907	rBV	223	177	0.03%	0.003%
34	6.763	921	931	950	rBV	144330	341224	51.30%	6.236%
35	6.909	954	955	958	rBV	288	306	0.05%	0.006%
36	7.129	982	991	1002	rBV2	77781	178199	26.79%	3.257%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025963.D
 Acq On : 21 Dec 2021 17:42
 Operator : JC/MD
 Sample : M5126-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

37	7.312	1010	1021	1035	rBV	140391	298452	44.87%	5.454%
38	7.781	1097	1098	1100	rBV	211	204	0.03%	0.004%
39	7.940	1122	1124	1129	rVB3	456	495	0.07%	0.009%
40	8.330	1181	1188	1199	rVV	104278	175612	26.40%	3.209%
41	8.458	1208	1209	1211	rBV	323	272	0.04%	0.005%
42	8.500	1214	1216	1219	rBV3	493	341	0.05%	0.006%
43	8.586	1228	1230	1233	rVB	248	193	0.03%	0.004%
44	8.653	1233	1241	1249	rBV	446485	665189	100.00%	12.157%
45	8.885	1277	1279	1281	rBV2	268	231	0.03%	0.004%
46	8.952	1284	1290	1304	rVB	71002	104414	15.70%	1.908%
47	9.275	1339	1343	1350	rVB3	4606	6715	1.01%	0.123%
48	9.342	1352	1354	1356	rBV	363	402	0.06%	0.007%
49	9.384	1356	1361	1381	rBV	250742	393563	59.17%	7.193%
50	9.683	1408	1410	1413	rVB	333	229	0.03%	0.004%
51	9.775	1423	1425	1428	rBV2	211	292	0.04%	0.005%
52	9.860	1436	1439	1442	rBV2	267	347	0.05%	0.006%
53	10.055	1465	1471	1479	rBV	402763	518908	78.01%	9.483%
54	10.238	1498	1501	1507	rBV2	600	984	0.15%	0.018%
55	10.342	1516	1518	1520	rBV	263	255	0.04%	0.005%
56	10.646	1565	1568	1570	rBV3	499	571	0.09%	0.010%
57	11.018	1628	1629	1633	rBV	192	251	0.04%	0.005%
58	11.122	1642	1646	1650	rVB	2096	2731	0.41%	0.050%
59	11.195	1652	1658	1668	rVV	343930	447871	67.33%	8.185%
60	11.482	1698	1705	1708	rBV3	925	1758	0.26%	0.032%
61	11.549	1714	1716	1718	rBV2	364	286	0.04%	0.005%
62	11.750	1745	1749	1755	rVB3	1222	1564	0.24%	0.029%
63	11.811	1757	1759	1761	rBV	185	163	0.02%	0.003%
64	11.933	1776	1779	1782	rVB2	800	696	0.10%	0.013%
65	11.963	1782	1784	1786	rVB2	265	191	0.03%	0.003%
66	12.024	1789	1794	1805	rVB	287838	367118	55.19%	6.709%
67	12.110	1805	1808	1809	rBV	427	390	0.06%	0.007%
68	12.152	1813	1815	1819	rVB3	985	1085	0.16%	0.020%
69	12.225	1822	1827	1831	rBV2	1524	2106	0.32%	0.038%
70	12.323	1837	1843	1851	rBV	317992	411917	61.92%	7.528%
71	12.481	1867	1869	1871	rBV2	370	355	0.05%	0.006%
72	12.664	1897	1899	1904	rVB3	365	435	0.07%	0.008%
73	12.731	1908	1910	1914	rVB	232	294	0.04%	0.005%
74	13.036	1958	1960	1962	rBV	262	255	0.04%	0.005%
75	13.256	1994	1996	1998	rVV2	224	205	0.03%	0.004%
76	13.298	2001	2003	2006	rVV2	145	162	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025963.D
 Acq On : 21 Dec 2021 17:42
 Operator : JC/MD
 Sample : M5126-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
 Title : VOC Analysis

77	13.408	2017	2021	2024	rBV2	331	341	0.05%	0.006%
78	13.487	2033	2034	2040	rBV	219	315	0.05%	0.006%
79	13.646	2059	2060	2062	rVB2	335	206	0.03%	0.004%
80	13.670	2062	2064	2065	rBV2	214	169	0.03%	0.003%
81	13.798	2083	2085	2087	rVB	255	201	0.03%	0.004%
82	14.067	2127	2129	2133	rVB2	211	240	0.04%	0.004%
83	14.164	2141	2145	2148	rBV2	130	233	0.04%	0.004%
84	14.304	2166	2168	2170	rVV2	314	240	0.04%	0.004%
85	14.566	2210	2211	2214	rVV2	229	179	0.03%	0.003%
86	14.621	2219	2220	2223	rVB	289	253	0.04%	0.005%
87	14.646	2223	2224	2226	rBV2	186	181	0.03%	0.003%
88	14.786	2245	2247	2249	rVB	257	167	0.03%	0.003%
89	14.816	2249	2252	2255	rBV2	247	309	0.05%	0.006%
90	14.951	2272	2274	2276	rBV2	150	172	0.03%	0.003%
91	15.170	2306	2310	2312	rBV3	246	292	0.04%	0.005%
92	15.219	2316	2318	2321	rBV2	174	186	0.03%	0.003%
93	15.249	2321	2323	2325	rBV2	207	230	0.03%	0.004%
94	15.329	2333	2336	2338	rBV3	322	304	0.05%	0.006%
95	15.371	2340	2343	2345	rBV2	212	230	0.03%	0.004%
96	15.822	2414	2417	2419	rBV	202	250	0.04%	0.005%
97	15.975	2441	2442	2446	rBV2	228	303	0.05%	0.006%
98	16.109	2462	2464	2468	rVB2	229	245	0.04%	0.004%
99	16.481	2523	2525	2527	rVB	303	205	0.03%	0.004%
100	16.572	2538	2540	2543	rBV2	247	352	0.05%	0.006%




Sum of corrected areas: 5471741

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025963.D
Acq On : 21 Dec 2021 17:42
Operator : JC/MD
Sample : M5126-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

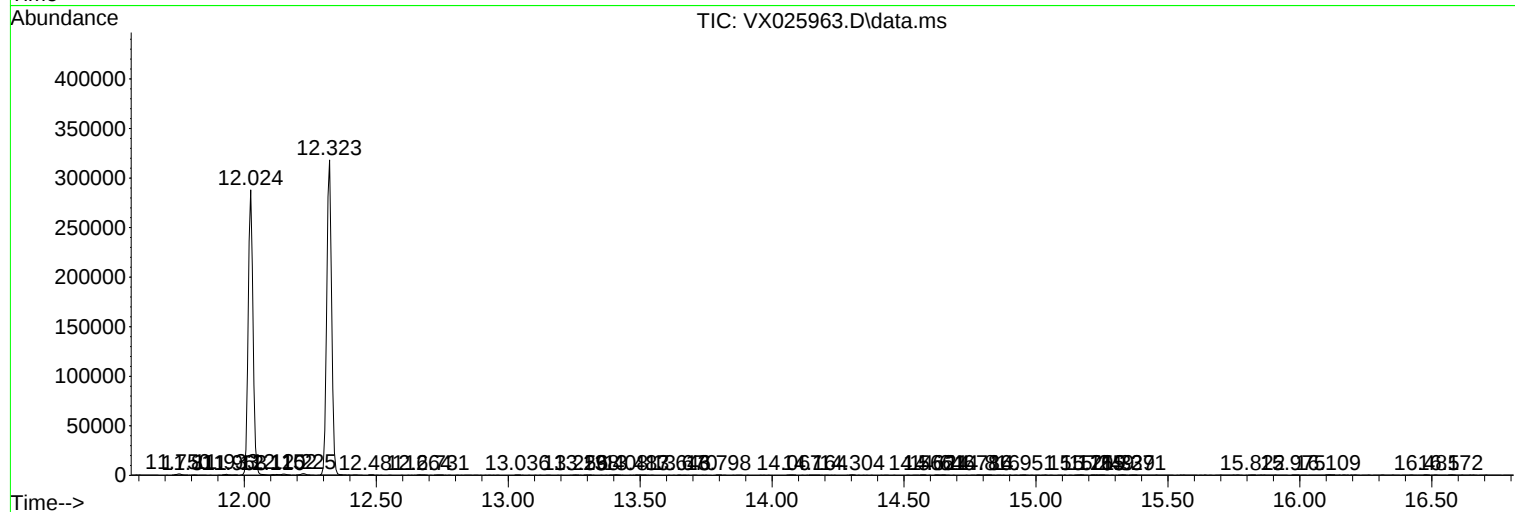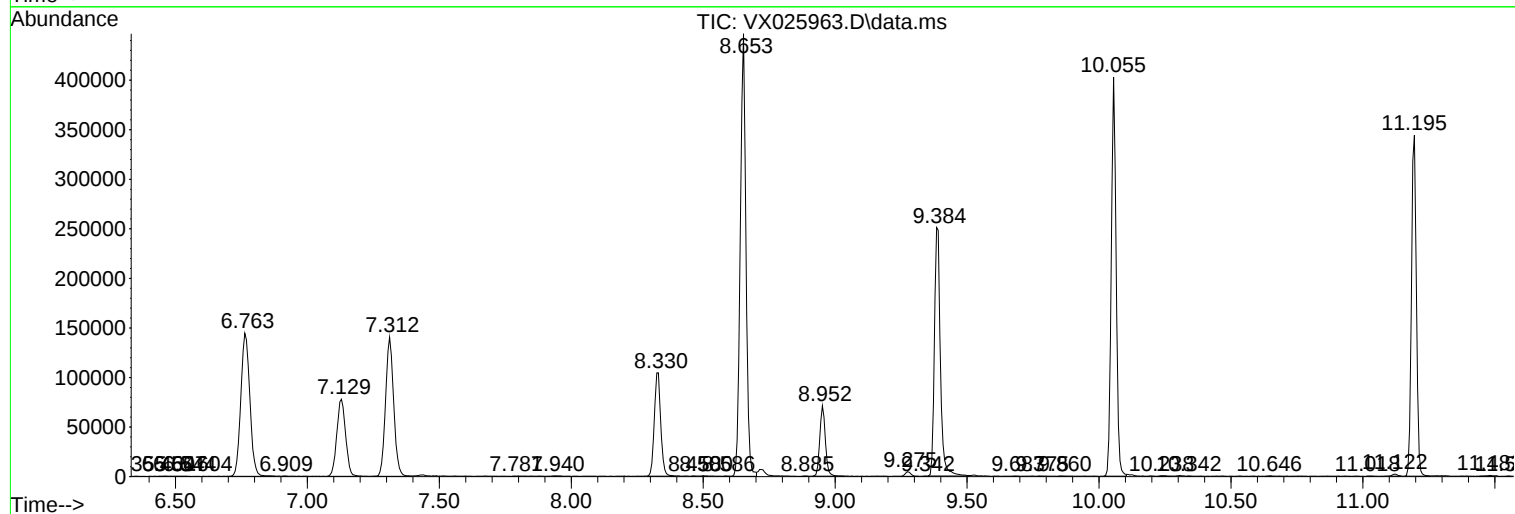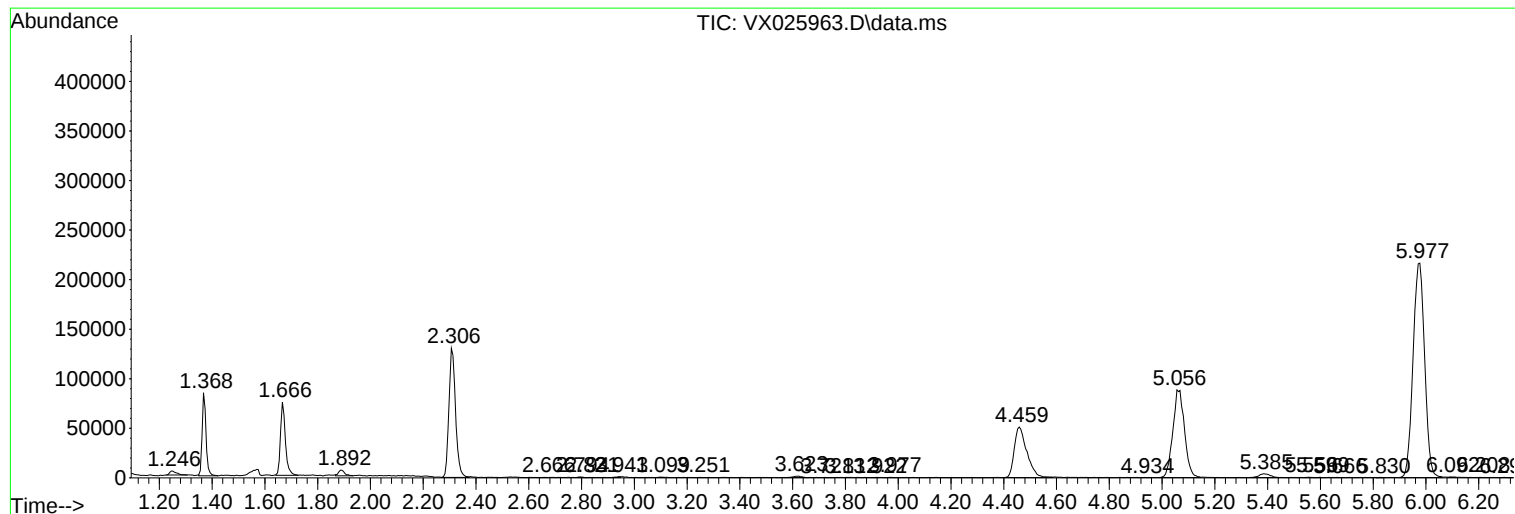

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025963.D
Acq On : 21 Dec 2021 17:42
Operator : JC/MD
Sample : M5126-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025963.D
Acq On : 21 Dec 2021 17:42
Operator : JC/MD
Sample : M5126-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
