

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025968.D
 Acq On : 21 Dec 2021 19:38
 Operator : JC/MD
 Sample : M5126-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

Signal : TIC: VX025968.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	24	26	33	rBV3	3386	6876	0.87%	0.126%
2	1.368	43	46	53	rVB	78460	79917	10.08%	1.461%
3	1.666	91	95	104	rBV	70406	93195	11.76%	1.703%
4	2.306	194	200	211	rBV	130100	217641	27.45%	3.978%
5	2.532	235	237	241	rBV2	566	611	0.08%	0.011%
6	2.605	248	249	257	rVB2	232	398	0.05%	0.007%
7	2.684	259	262	263	rBV	175	195	0.02%	0.004%
8	2.898	295	297	298	rVB	382	187	0.02%	0.003%
9	2.916	298	300	301	rBV	295	246	0.03%	0.004%
10	2.947	301	305	310	rVV	756	1728	0.22%	0.032%
11	3.007	313	315	317	rVB	294	195	0.02%	0.004%
12	3.251	353	355	358	rBV2	214	268	0.03%	0.005%
13	3.361	370	373	374	rBV2	175	158	0.02%	0.003%
14	3.434	381	385	386	rBV	250	244	0.03%	0.004%
15	4.245	516	518	521	rBV2	231	296	0.04%	0.005%
16	4.458	544	553	569	rBV2	46065	136246	17.19%	2.490%
17	4.727	596	597	599	rBV	308	231	0.03%	0.004%
18	4.782	604	606	609	rVV2	248	243	0.03%	0.004%
19	5.068	640	653	666	rBV	86694	272172	34.33%	4.974%
20	5.257	681	684	685	rVV3	242	187	0.02%	0.003%
21	5.470	716	719	721	rBV2	159	170	0.02%	0.003%
22	5.556	729	733	736	rBV3	327	515	0.06%	0.009%
23	5.830	776	778	781	rVB2	237	194	0.02%	0.004%
24	5.976	789	802	819	rBV2	219117	649740	81.96%	11.875%
25	6.233	843	844	846	rBV2	246	185	0.02%	0.003%
26	6.586	900	902	903	rBV	249	205	0.03%	0.004%
27	6.763	922	931	946	rBV	195725	455977	57.52%	8.333%
28	7.129	982	991	1001	rVB5	20054	49189	6.20%	0.899%
29	7.312	1012	1021	1032	rBV	163556	364232	45.94%	6.657%
30	7.440	1040	1042	1043	rVB	228	166	0.02%	0.003%
31	7.488	1045	1050	1053	rVV2	279	605	0.08%	0.011%
32	7.757	1092	1094	1096	rBV2	261	267	0.03%	0.005%
33	7.909	1118	1119	1120	rBV	254	173	0.02%	0.003%
34	7.940	1120	1124	1126	rVV2	601	864	0.11%	0.016%
35	8.330	1181	1188	1203	rBV	120454	202544	25.55%	3.702%
36	8.433	1203	1205	1208	rBV2	322	349	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025968.D
 Acq On : 21 Dec 2021 19:38
 Operator : JC/MD
 Sample : M5126-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

37	8.653	1234	1241	1249	rBV	497133	792760	100.00%	14.488%
38	8.952	1284	1290	1299	rBV	83649	120534	15.20%	2.203%
39	9.171	1322	1326	1330	rBV3	196	338	0.04%	0.006%
40	9.256	1338	1340	1341	rBV	318	209	0.03%	0.004%
41	9.275	1341	1343	1347	rVB3	1104	1325	0.17%	0.024%
42	9.384	1356	1361	1381	rBV	317736	474329	59.83%	8.669%
43	10.055	1465	1471	1488	rVB	320609	435852	54.98%	7.966%
44	10.195	1492	1494	1498	rBV2	285	379	0.05%	0.007%
45	10.244	1498	1502	1507	rVB3	521	842	0.11%	0.015%
46	10.299	1507	1511	1512	rBV2	383	454	0.06%	0.008%
47	10.311	1512	1513	1517	rVB3	653	449	0.06%	0.008%
48	10.378	1522	1524	1526	rBV	353	246	0.03%	0.004%
49	10.573	1555	1556	1558	rBV2	173	176	0.02%	0.003%
50	10.640	1566	1567	1570	rVB	292	235	0.03%	0.004%
51	10.872	1601	1605	1607	rVB2	186	223	0.03%	0.004%
52	10.988	1622	1624	1627	rBV2	203	166	0.02%	0.003%
53	11.122	1642	1646	1652	rVB4	1107	1244	0.16%	0.023%
54	11.195	1652	1658	1669	rBV	240246	304949	38.47%	5.573%
55	11.305	1673	1676	1677	rBV2	303	256	0.03%	0.005%
56	11.451	1698	1700	1702	rBV2	226	217	0.03%	0.004%
57	11.555	1715	1717	1720	rVB2	189	164	0.02%	0.003%
58	11.683	1737	1738	1741	rVB2	197	191	0.02%	0.003%
59	11.750	1746	1749	1754	rVB4	904	1198	0.15%	0.022%
60	11.811	1757	1759	1762	rBV	309	189	0.02%	0.003%
61	11.933	1777	1779	1783	rVB3	392	468	0.06%	0.009%
62	12.024	1789	1794	1801	rBV	308480	379698	47.90%	6.939%
63	12.152	1812	1815	1819	rVB5	694	826	0.10%	0.015%
64	12.225	1823	1827	1832	rVV4	971	1741	0.22%	0.032%
65	12.323	1836	1843	1853	rVV	321609	406607	51.29%	7.431%
66	12.427	1857	1860	1862	rBV2	231	186	0.02%	0.003%
67	12.811	1921	1923	1925	rBV2	220	176	0.02%	0.003%
68	13.109	1968	1972	1977	rVB2	242	315	0.04%	0.006%
69	13.371	2012	2015	2019	rBV	330	410	0.05%	0.007%
70	13.414	2019	2022	2025	rVV2	210	320	0.04%	0.006%
71	13.512	2036	2038	2042	rVV	223	237	0.03%	0.004%
72	13.609	2052	2054	2057	rBV	278	222	0.03%	0.004%
73	13.774	2080	2081	2085	rBV	182	202	0.03%	0.004%
74	13.847	2090	2093	2094	rVV	154	159	0.02%	0.003%
75	13.920	2103	2105	2108	rVV2	182	212	0.03%	0.004%
76	14.018	2120	2121	2123	rBV	328	216	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
 Data File : VX025968.D
 Acq On : 21 Dec 2021 19:38
 Operator : JC/MD
 Sample : M5126-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0J26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
 Title : VOC Analysis

77	14.073	2128	2130	2131	rBV2	309	161	0.02%	0.003%
78	14.201	2149	2151	2152	rBV	210	171	0.02%	0.003%
79	14.316	2167	2170	2176	rBV2	271	434	0.05%	0.008%
80	14.396	2180	2183	2185	rBV2	166	180	0.02%	0.003%
81	14.530	2204	2205	2208	rBV2	225	244	0.03%	0.004%
82	14.560	2208	2210	2212	rVB	323	201	0.03%	0.004%
83	14.633	2219	2222	2223	rVV2	204	249	0.03%	0.005%
84	14.701	2228	2233	2238	rVB2	295	506	0.06%	0.009%
85	14.761	2238	2243	2246	rBV2	319	492	0.06%	0.009%
86	14.841	2252	2256	2257	rBV2	264	335	0.04%	0.006%
87	14.944	2270	2273	2277	rBV3	318	544	0.07%	0.010%
88	14.981	2277	2279	2280	rBV	366	219	0.03%	0.004%
89	15.078	2292	2295	2298	rBV2	207	251	0.03%	0.005%
90	15.127	2302	2303	2306	rBV	260	170	0.02%	0.003%
91	15.249	2321	2323	2325	rVB2	217	162	0.02%	0.003%
92	15.267	2325	2326	2329	rBV2	288	219	0.03%	0.004%
93	15.359	2340	2341	2344	rVB2	235	165	0.02%	0.003%
94	15.383	2344	2345	2346	rBV	336	165	0.02%	0.003%
95	16.097	2460	2462	2466	rBV2	210	220	0.03%	0.004%
96	16.347	2502	2503	2505	rBV	239	226	0.03%	0.004%
97	16.383	2507	2509	2512	rBV2	230	300	0.04%	0.005%
98	16.682	2556	2558	2559	rBV	212	180	0.02%	0.003%
99	16.700	2559	2561	2562	rVB	330	172	0.02%	0.003%
100	16.761	2569	2571	2573	rBV	238	197	0.02%	0.004%




Sum of corrected areas: 5471692

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025968.D
Acq On : 21 Dec 2021 19:38
Operator : JC/MD
Sample : M5126-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

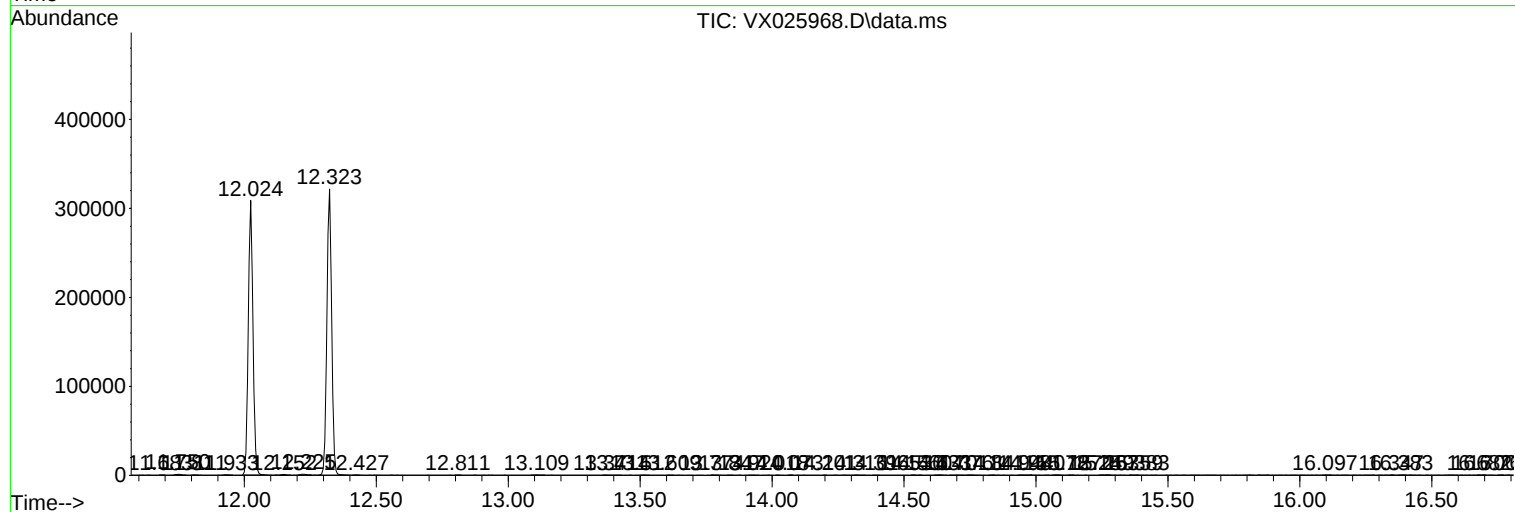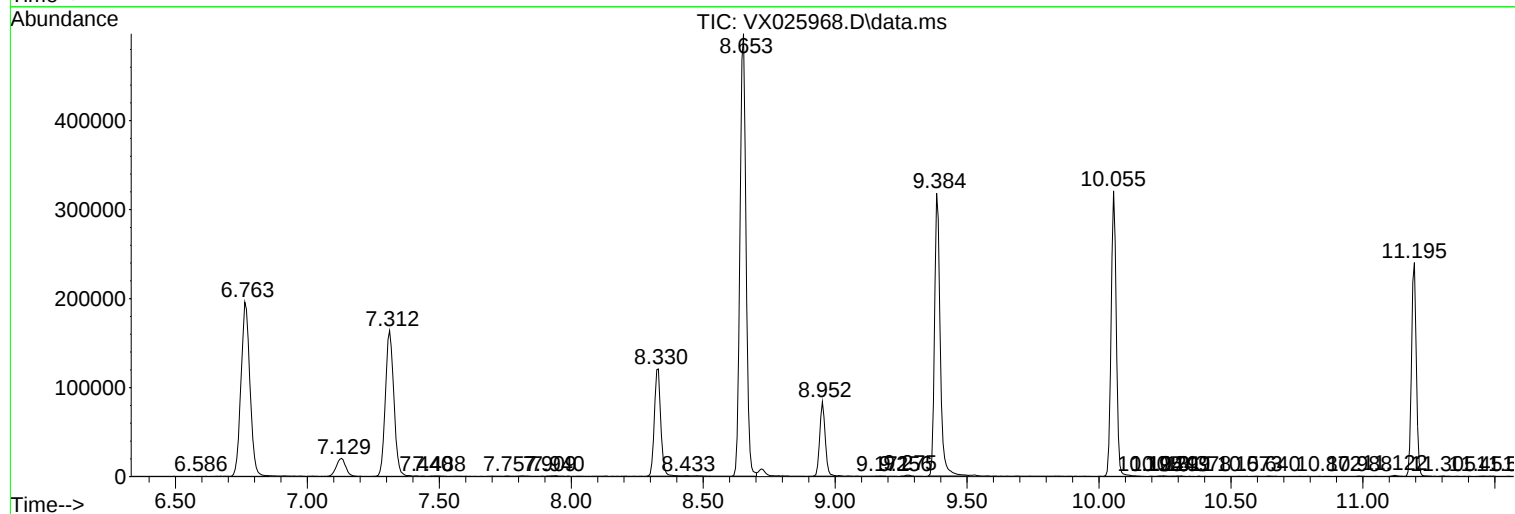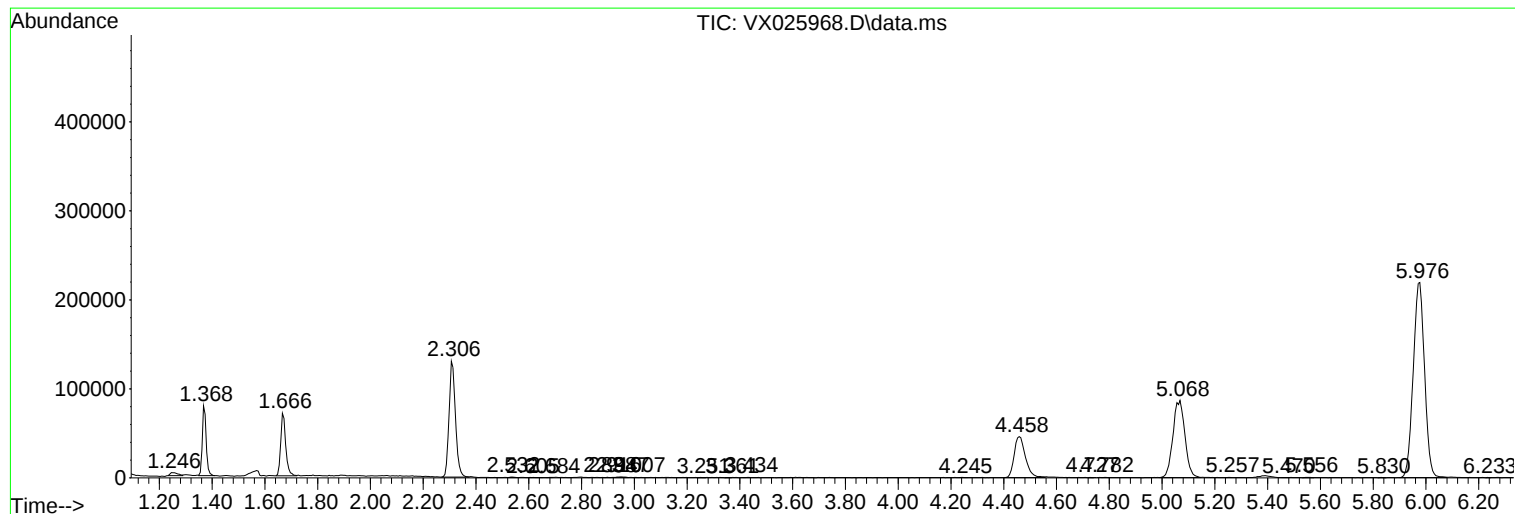

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025968.D
Acq On : 21 Dec 2021 19:38
Operator : JC/MD
Sample : M5126-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122121\
Data File : VX025968.D
Acq On : 21 Dec 2021 19:38
Operator : JC/MD
Sample : M5126-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0J26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122021WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc